

Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
Data File : FE027014.D
Signal(s) : FID1B.CH
Acq On : 09 May 2018 9:46
Operator : UA/AJ
Sample : J2759-05 50X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 10:40:10 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	15.512	481736	2.860 ug/ml
12)	N-OCTACOSANE	17.480	376363	2.278 ug/ml
14)	N-DOTRIACONTANE	19.211	124490	0.725 ug/ml
16)	N-HEXATRIACONTANE	20.758	395405	2.247 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
Data File : FE027014.D
Signal(s) : FID1B.CH
Acq On : 09 May 2018 9:46
Operator : UA/AJ
Sample : J2759-05 50X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 10:40:10 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

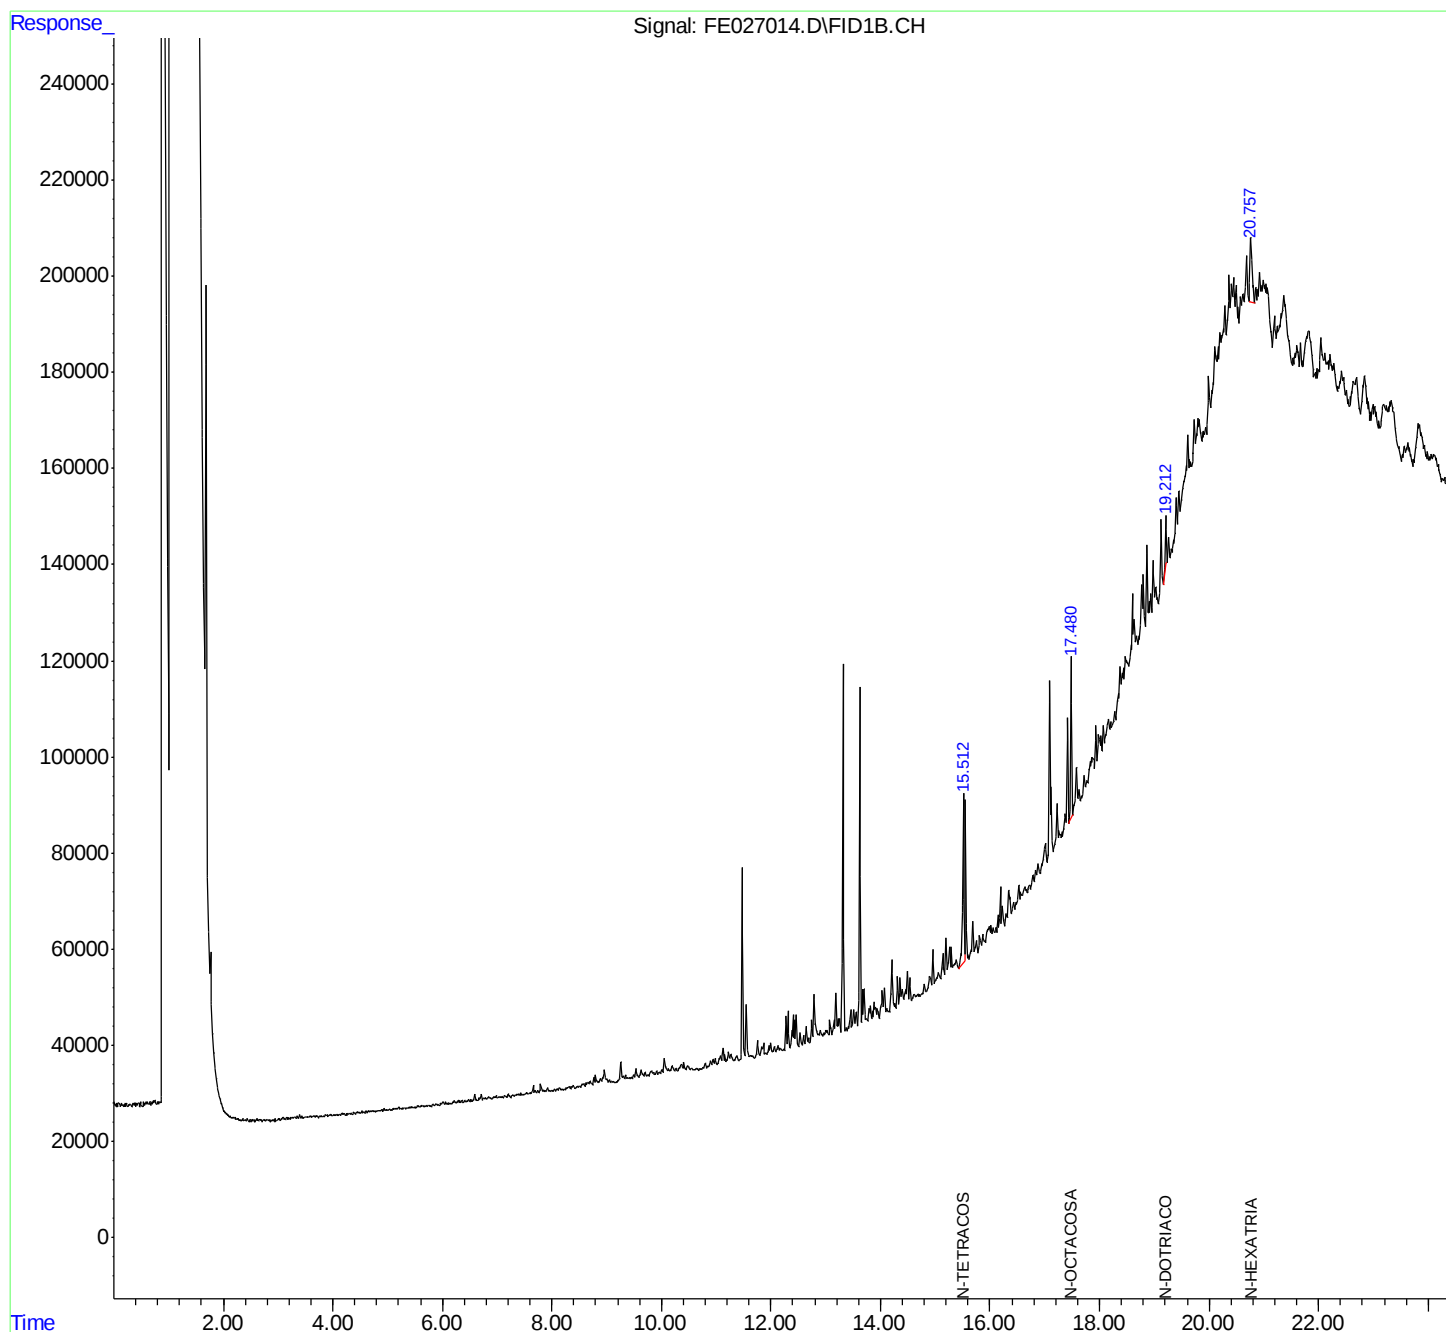


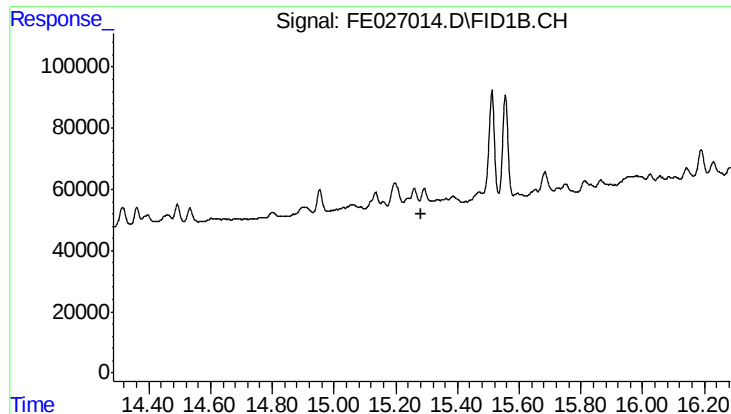

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.285 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

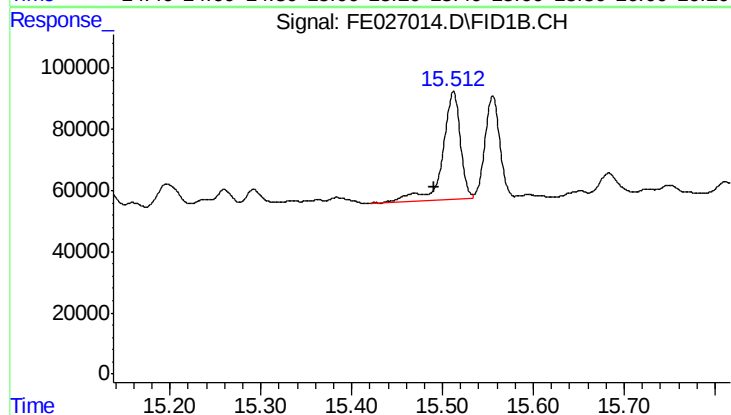


#10 N-TETRACOSANE

R.T.: 15.512 min
Delta R.T.: 0.021 min
Response: 481736
Conc: 2.86 ug/ml

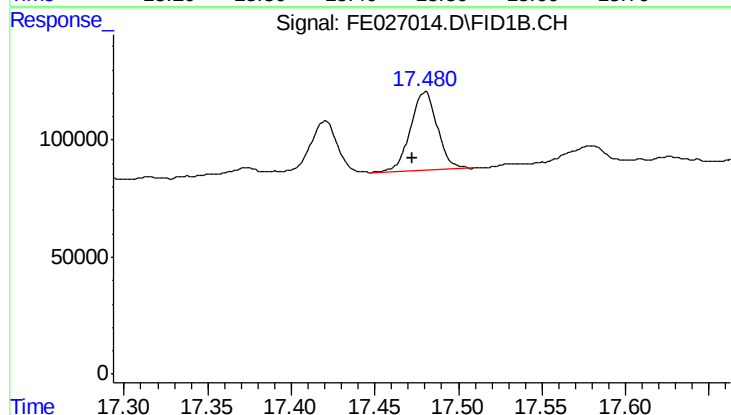


#12 N-OCTACOSANE

R.T.: 17.480 min
Delta R.T.: 0.008 min
Response: 376363
Conc: 2.28 ug/ml

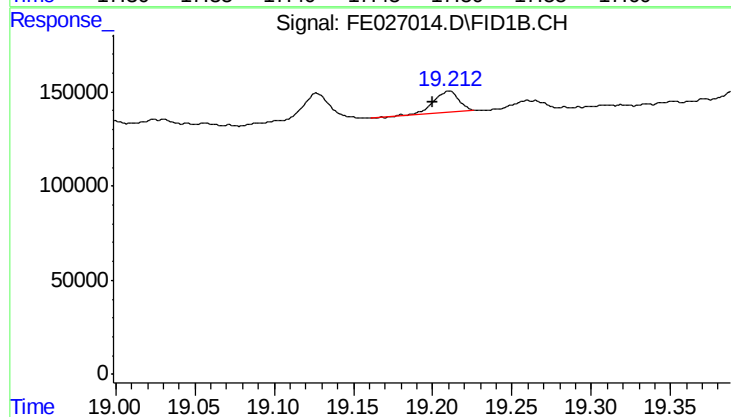

#14 N-DOTRIACONTANE

R.T.: 19.211 min
Delta R.T.: 0.011 min
Response: 124490
Conc: 0.72 ug/ml

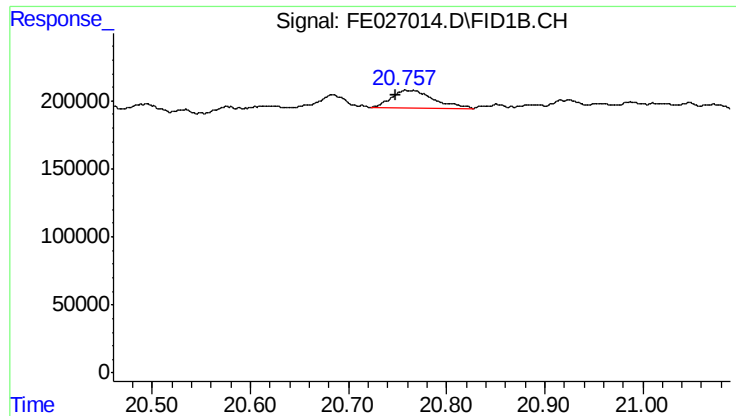

#16 N-HEXATRIACONTANE

R.T.: 20.758 min
Delta R.T.: 0.010 min
Response: 395405
Conc: 2.25 ug/ml

Instrument :
FID_E
ClientSampleId :