

Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
 Data File : FE027015.D
 Signal(s) : FID1B.CH
 Acq On : 09 May 2018 10:20
 Operator : UA/AJ
 Sample : J2674-01 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 09 17:00:17 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.294	545367	3.704 ug/ml
Target Compounds			
7) N-EICOSANE	13.186	261354	1.372 ug/ml
8) N-DOCOSANE	14.361	146689	0.822 ug/ml
10) N-TETRACOSANE	15.514	913198	5.422 ug/ml
12) N-OCTACOSANE	17.482	779158	4.715 ug/ml
13) N-TRIACONTANE	18.374	155823	0.926 ug/ml
14) N-DOTRIACONTANE	19.209	328926	1.914 ug/ml
15) N-TETRATRIACONTANE	19.998	171494	0.957 ug/ml
16) N-HEXATRIACONTANE	20.763	425753	2.420 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
Data File : FE027015.D
Signal(s) : FID1B.CH
Acq On : 09 May 2018 10:20
Operator : UA/AJ
Sample : J2674-01 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: May 09 17:00:17 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

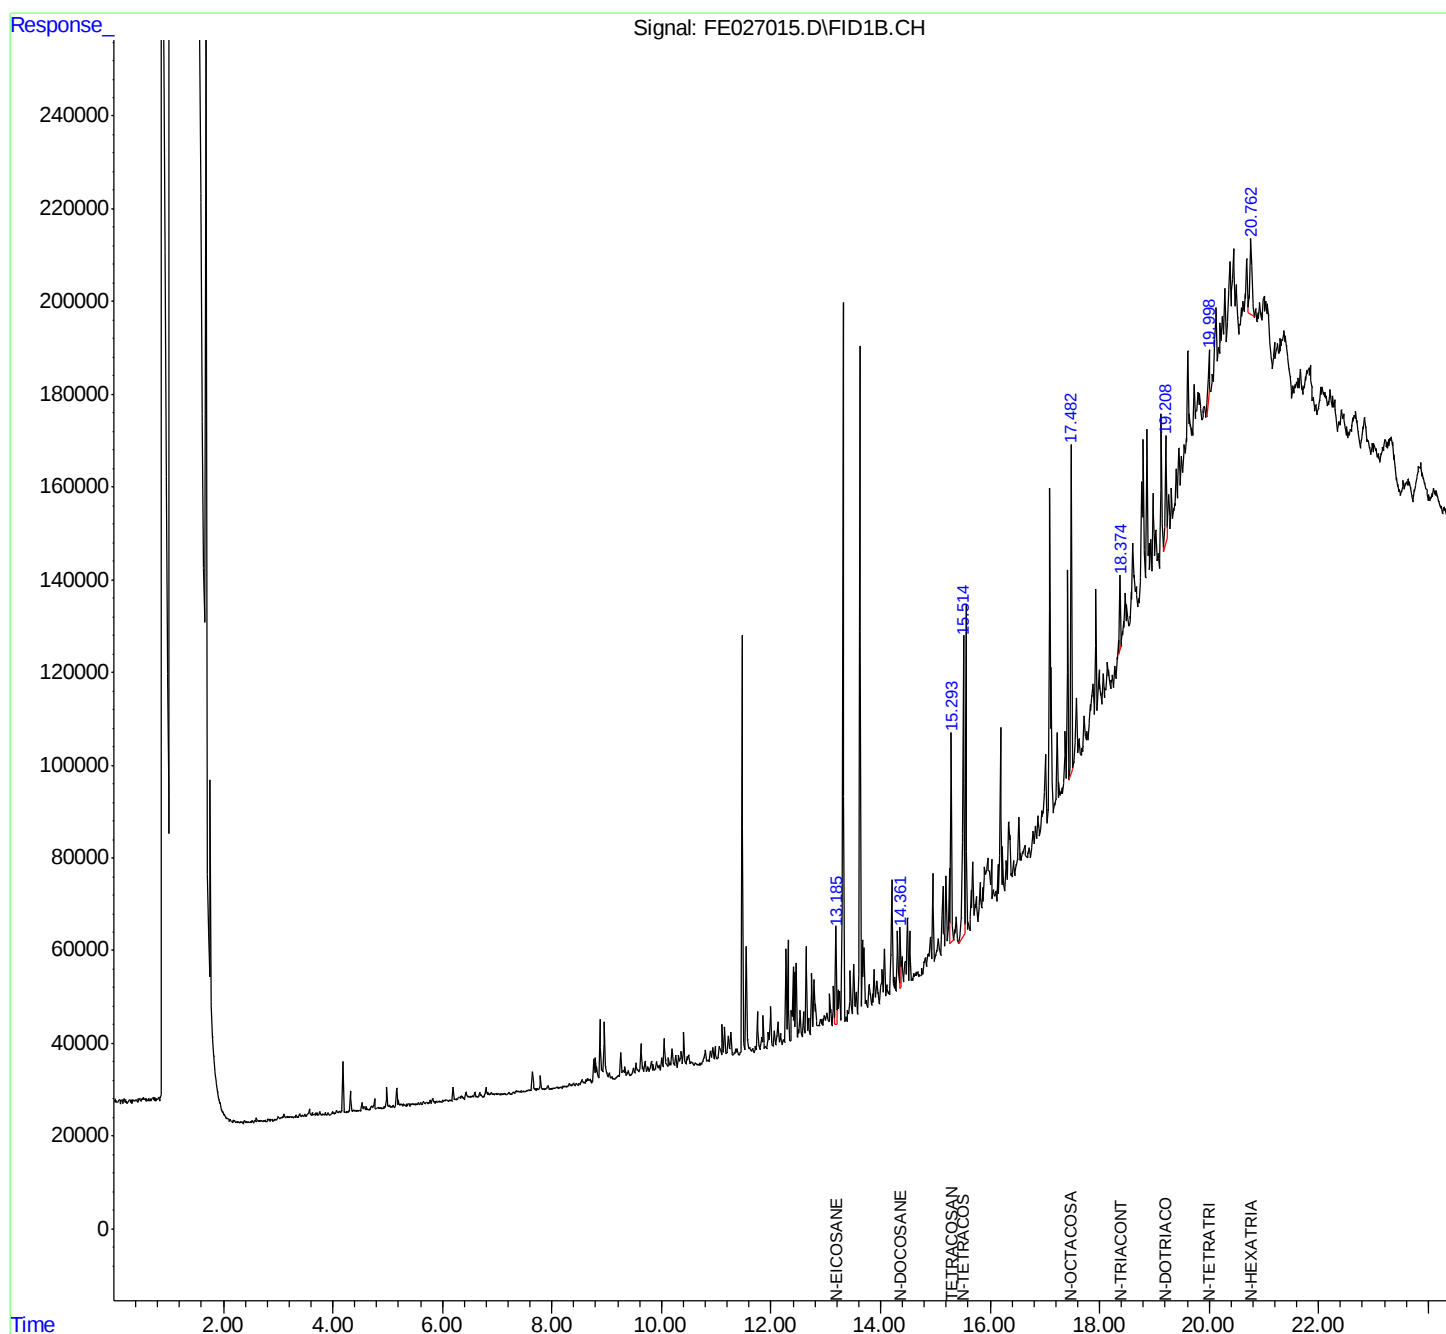


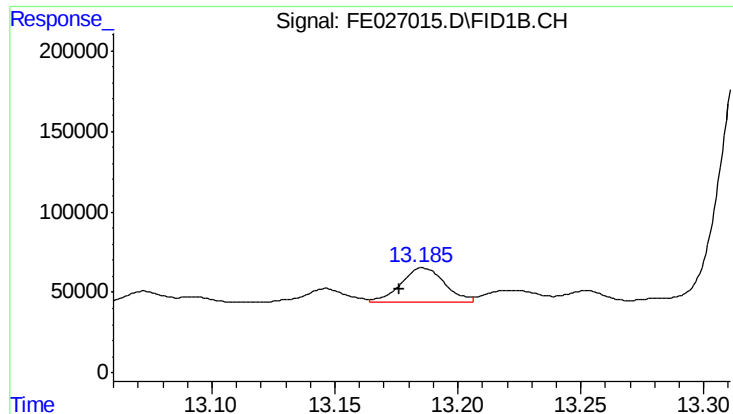

#7 N-EICOSANE


R.T.: 13.186 min
Delta R.T.: 0.010 min
Response: 261354
Conc: 1.37 ug/ml

Instrument :
FID_E
ClientSampleId :

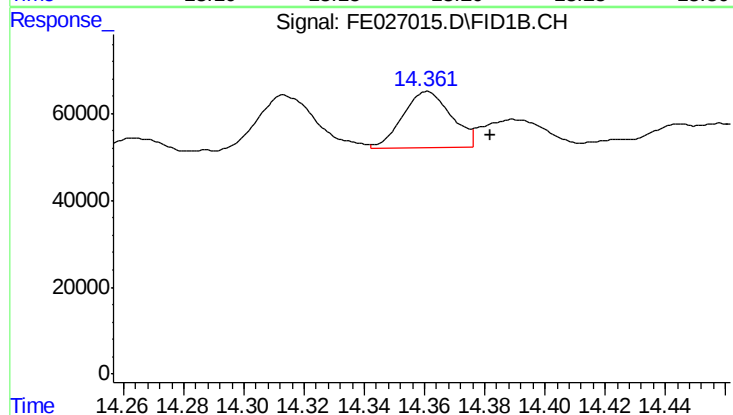


#8 N-DOCOSANE

R.T.: 14.361 min
Delta R.T.: -0.021 min
Response: 146689
Conc: 0.82 ug/ml

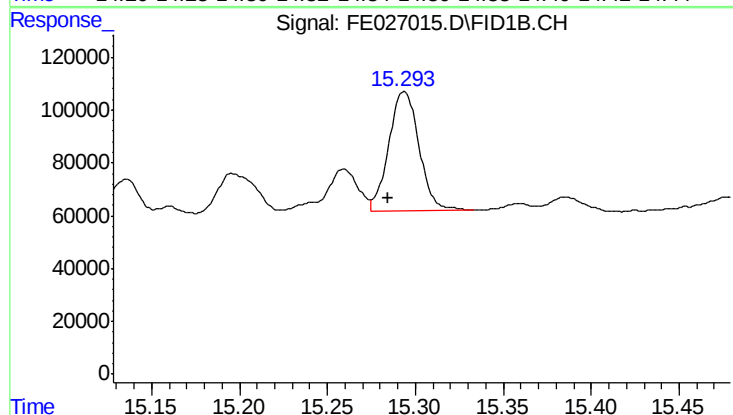


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.294 min
Delta R.T.: 0.009 min
Response: 545367
Conc: 3.70 ug/ml

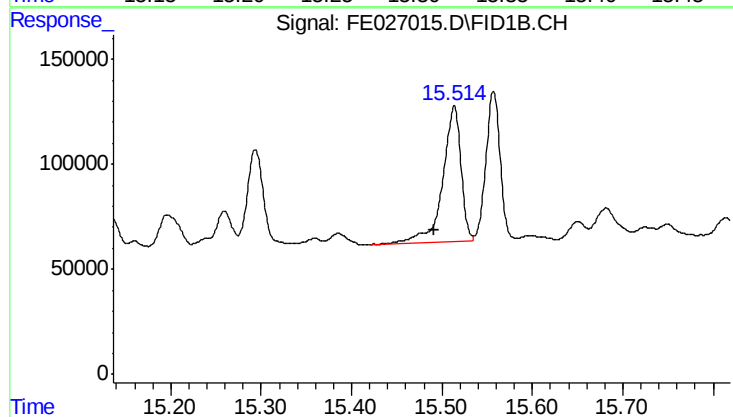

#10 N-TETRACOSANE


R.T.: 15.514 min
Delta R.T.: 0.023 min
Response: 913198
Conc: 5.42 ug/ml

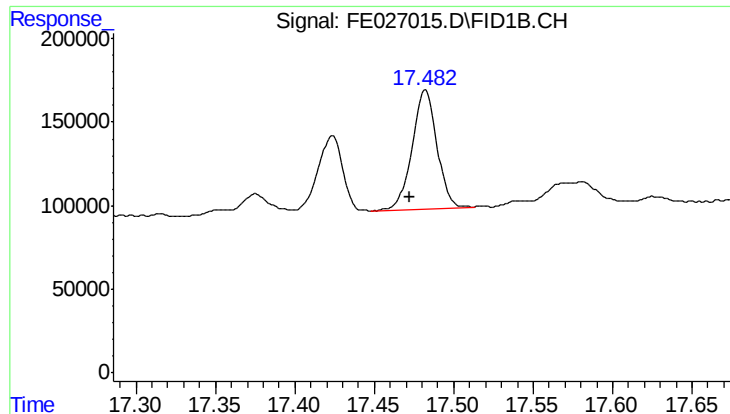

#12 N-OCTACOSANE


R.T.: 17.482 min
Delta R.T.: 0.010 min
Response: 779158
Conc: 4.72 ug/ml

Instrument :
FID_E
ClientSampleId :

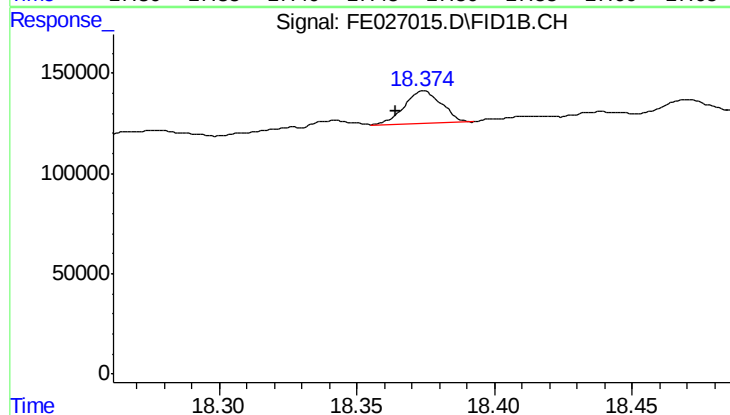


#13 N-TRIACONTANE

R.T.: 18.374 min
Delta R.T.: 0.010 min
Response: 155823
Conc: 0.93 ug/ml

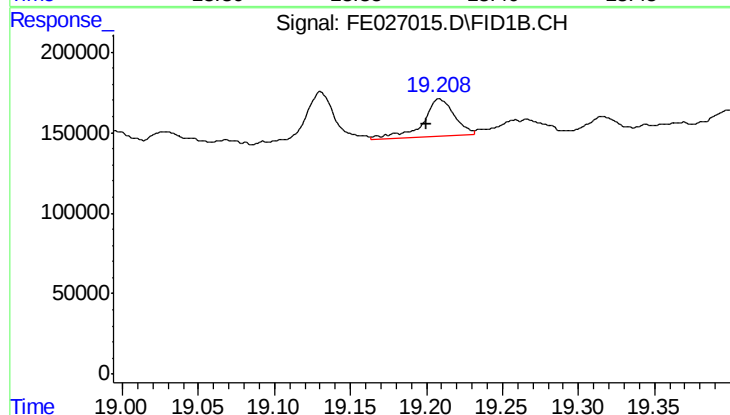


#14 N-DOTRIACONTANE

R.T.: 19.209 min
Delta R.T.: 0.009 min
Response: 328926
Conc: 1.91 ug/ml

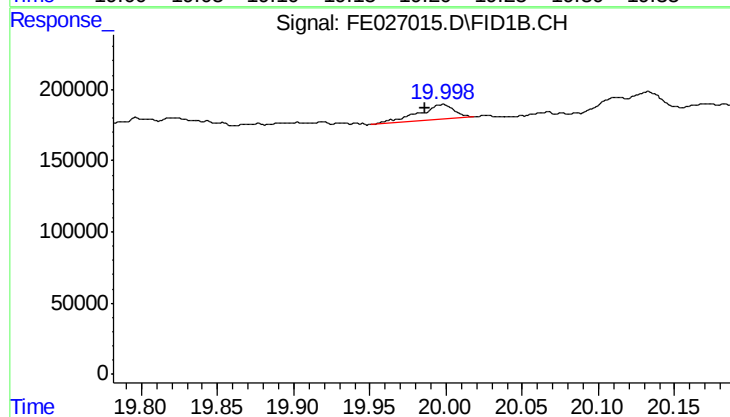

#15 N-TETRATRIACONTANE

R.T.: 19.998 min
Delta R.T.: 0.011 min
Response: 171494
Conc: 0.96 ug/ml

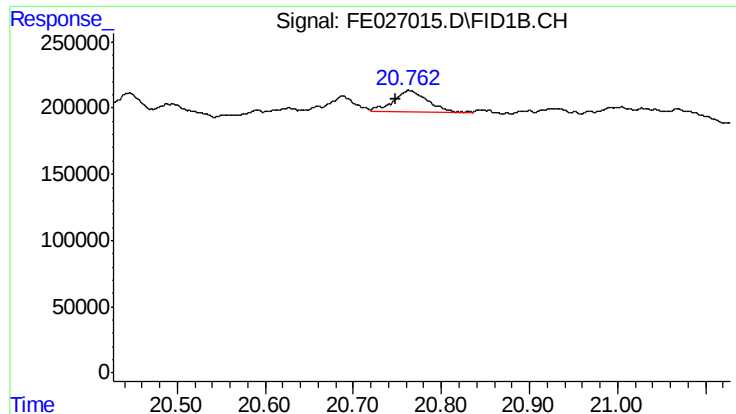

#16 N-HEXATRIACONTANE

R.T.: 20.763 min
Delta R.T.: 0.015 min
Response: 425753
Conc: 2.42 ug/ml

Instrument :
FID_E
ClientSampleId :