

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050923AL\
 Data File : FE041826.D
 Signal(s) : FID1B.ch
 Acq On : 09 May 2023 22:57
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 10 00:23:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.119	11515	0.076 ug/ml
18) T n-Dotriacontane (C32)	18.951	42572	0.286 ug/ml
19) T n-Tetratriacontane (C34)	19.706	137000	0.972 ug/ml
20) T n-Hexatriacontane (C36)	20.467	33163	0.248 ug/ml
21) T n-Octatriacontane (C38)	21.247	61709	0.467 ug/ml
22) T n-Tetracontane (C40)	22.217f	26497	0.209 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050923AL\
Data File : FE041826.D
Signal(s) : FID1B.ch
Acq On : 09 May 2023 22:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 00:23:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

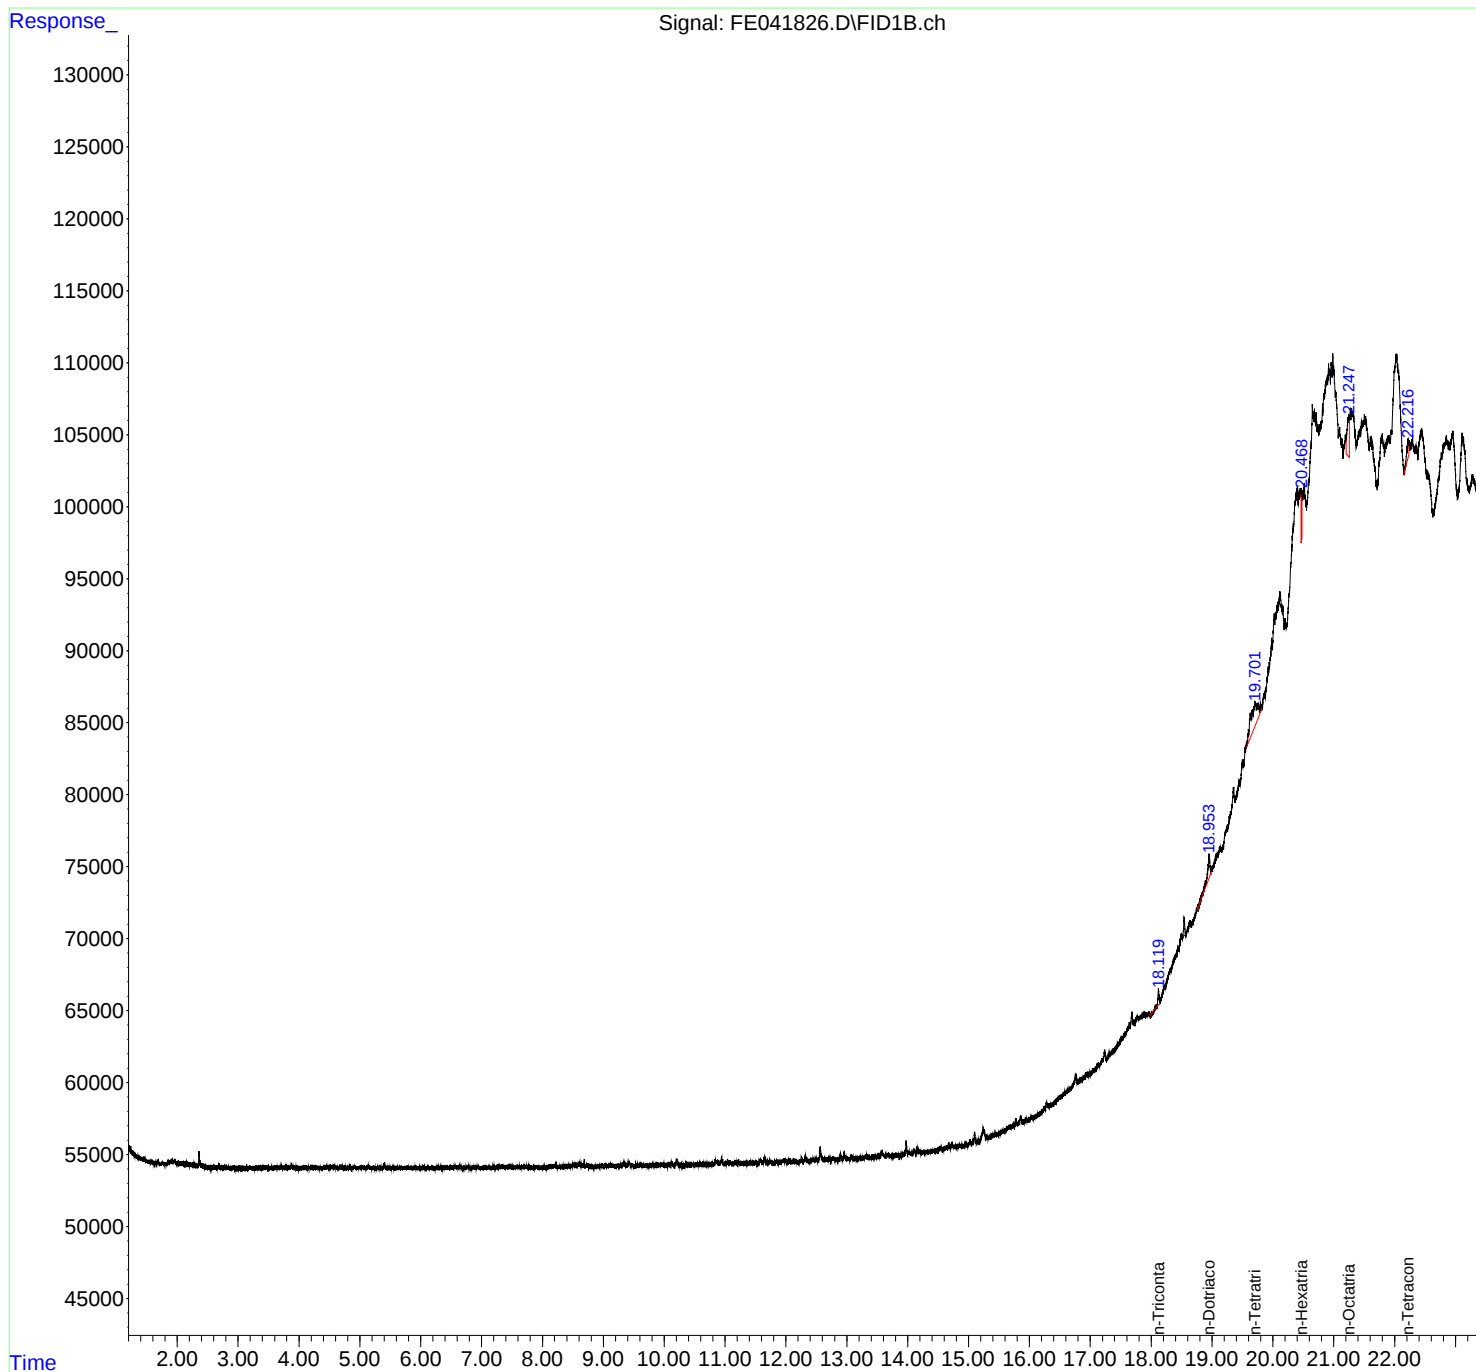


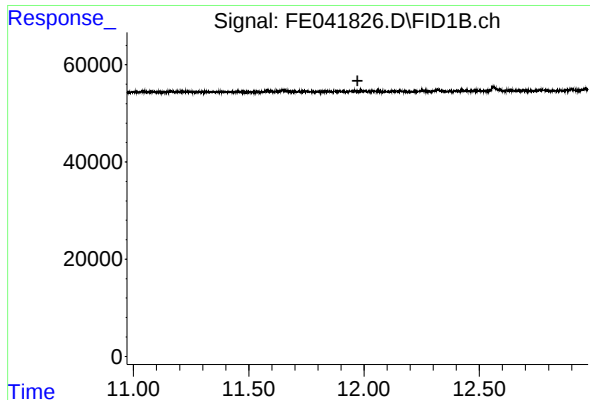

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

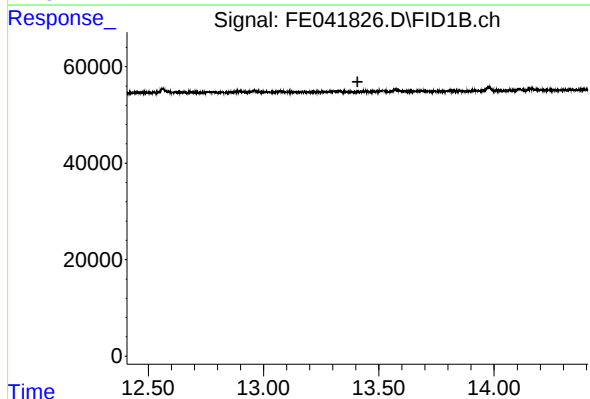


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

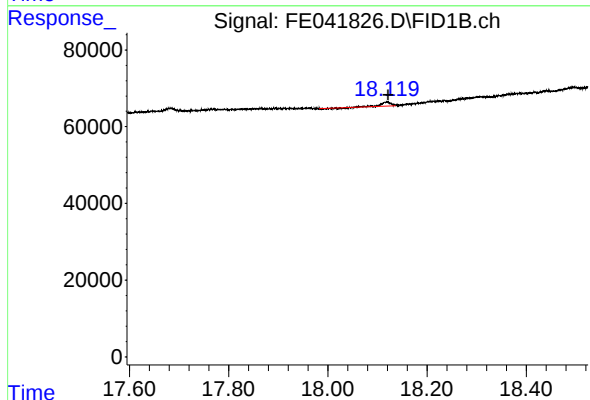


#17 n-Tricontane (C30)

R.T.: 18.119 min
Delta R.T.: -0.002 min
Response: 11515
Conc: 0.08 ug/ml

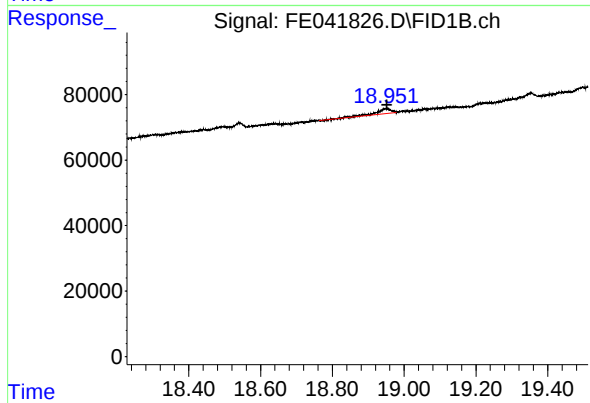

#18 n-Dotriacontane (C32)


R.T.: 18.951 min
Delta R.T.: 0.000 min
Response: 42572
Conc: 0.29 ug/ml

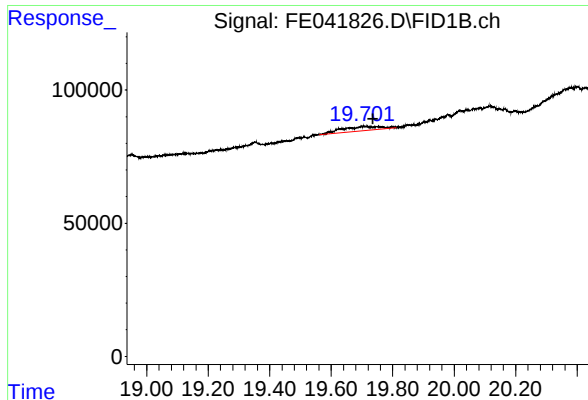

#19 n-Tetratriacontane (C34)


R.T.: 19.706 min
Delta R.T.: -0.030 min
Response: 137000
Conc: 0.97 ug/ml

Instrument :
FID_E
ClientSampleId :

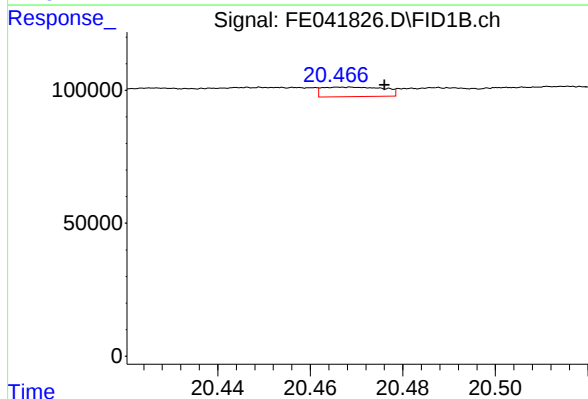


#20 n-Hexatriacontane (C36)

R.T.: 20.467 min
Delta R.T.: -0.009 min
Response: 33163
Conc: 0.25 ug/ml

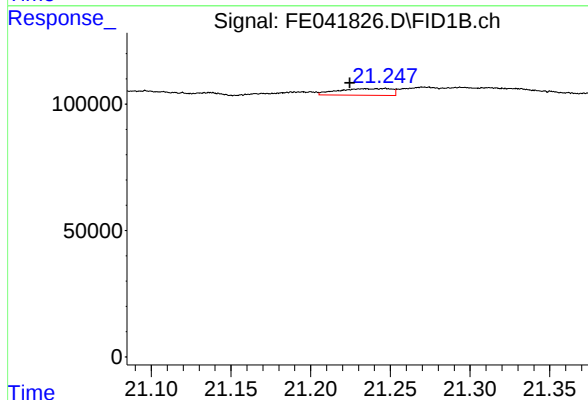

#21 n-Octatriacontane (C38)

R.T.: 21.247 min
Delta R.T.: 0.022 min
Response: 61709
Conc: 0.47 ug/ml

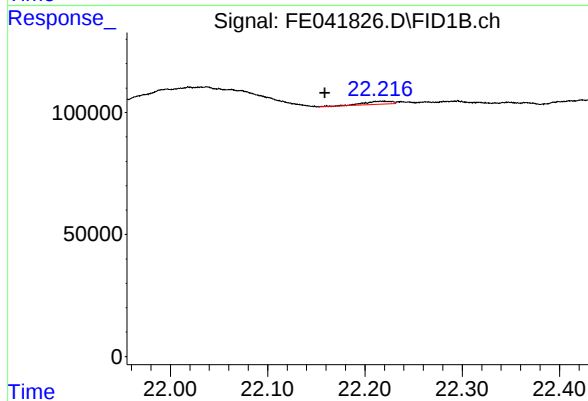

#22 n-Tetracontane (C40)

R.T.: 22.217 min
Delta R.T.: 0.059 min
Response: 26497
Conc: 0.21 ug/ml