

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050924\
Data File : FE048058.D
Signal(s) : FID1B.ch
Acq On : 09 May 2024 22:55
Operator : YP\AJ
Sample : PB160780BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 01:56:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050924.M
Quant Title :
QLast Update : Fri May 10 01:45:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.050	2120807	18.397 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.943	54161	0.378 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050924\
Data File : FE048058.D
Signal(s) : FID1B.ch
Acq On : 09 May 2024 22:55
Operator : YP\AJ
Sample : PB160780BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 01:56:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050924.M
Quant Title :
QLast Update : Fri May 10 01:45:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

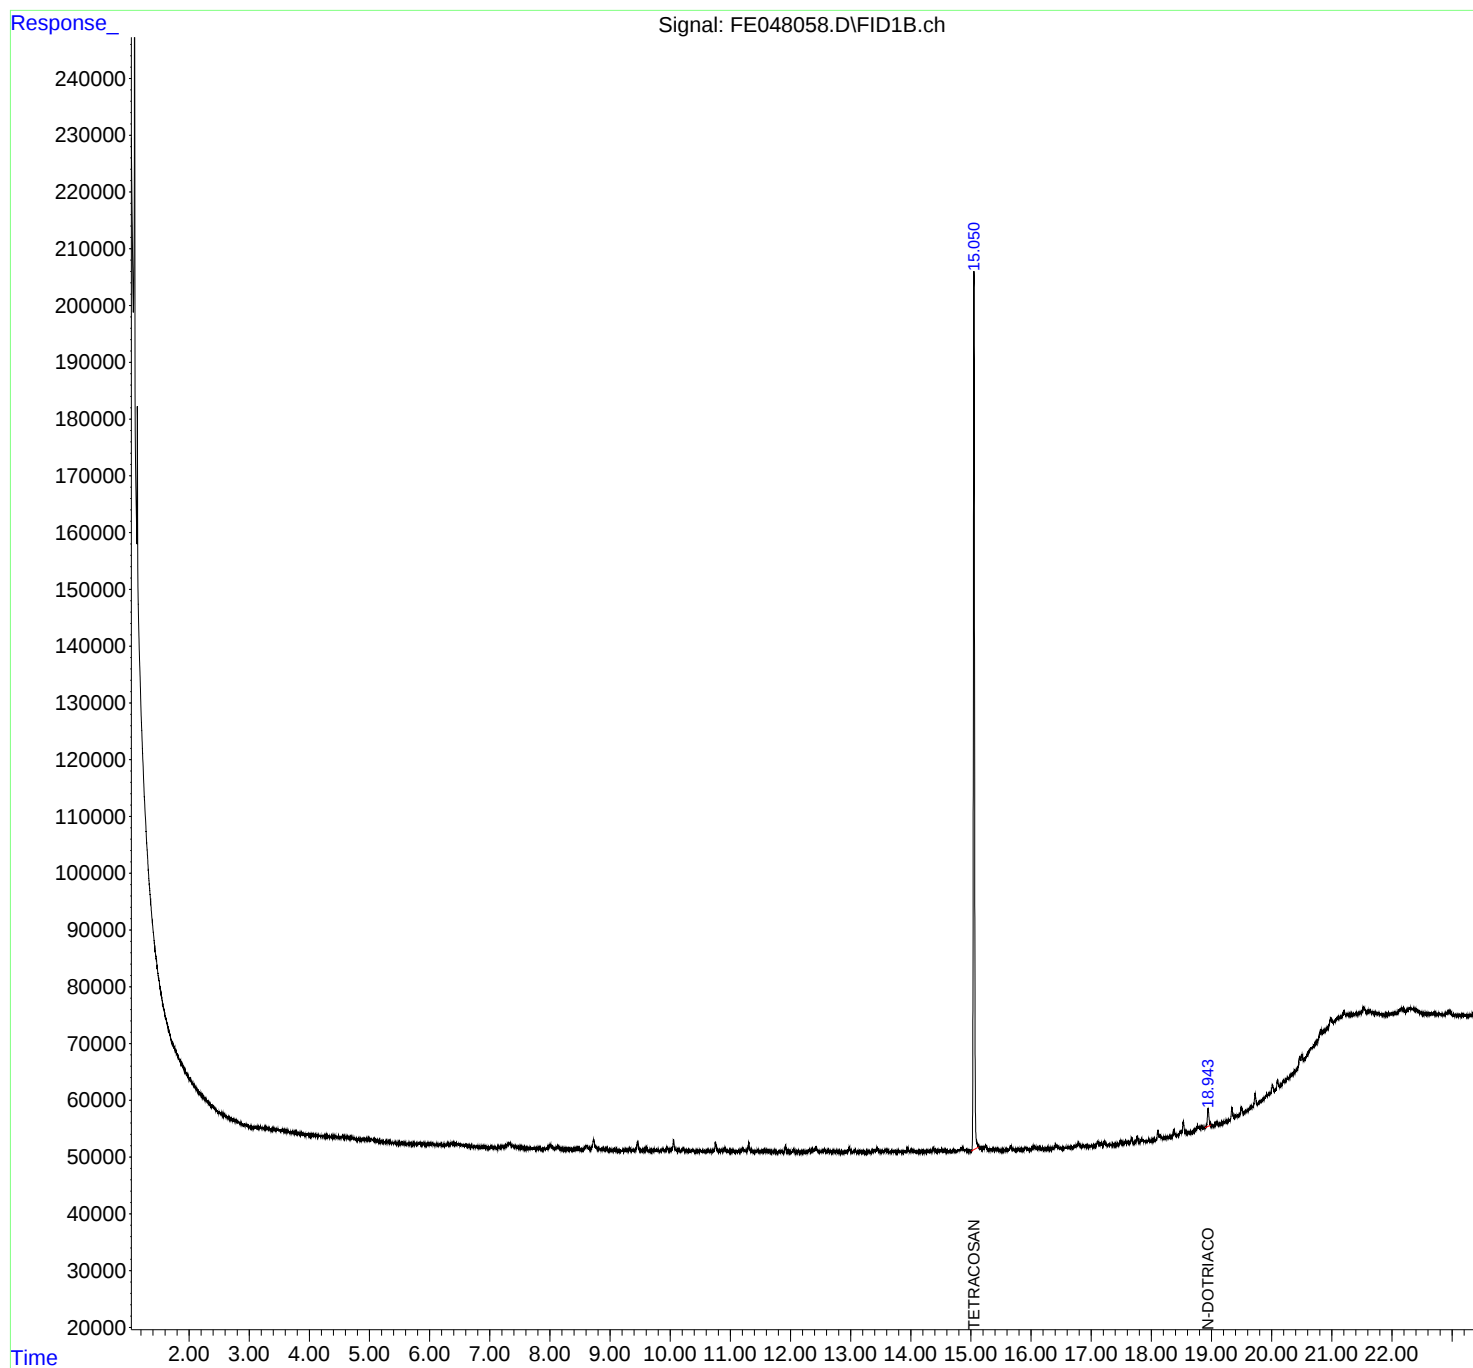


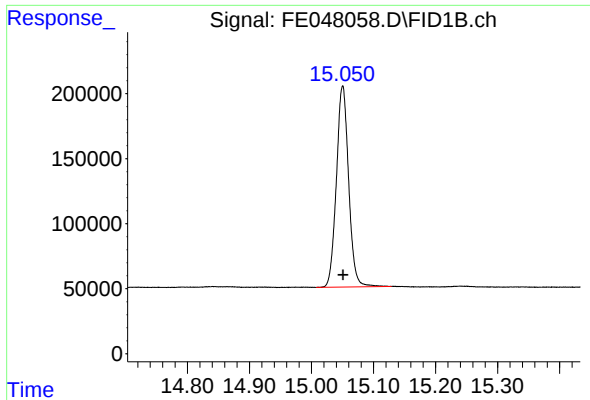

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.050 min
Delta R.T.: 0.000 min
Response: 2120807
Conc: 18.40 ug/ml

Instrument :
FID_E
ClientSampleId :

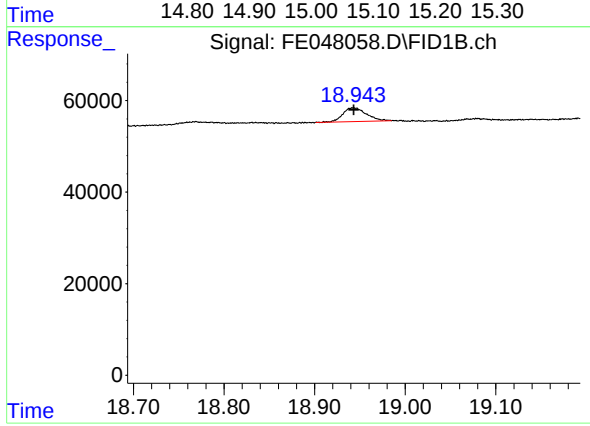

#14 N-DOTRIACONTANE

R.T.: 18.943 min
Delta R.T.: 0.000 min
Response: 54161
Conc: 0.38 ug/ml