

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051024\
Data File : FE048072.D
Signal(s) : FID1B.ch
Acq On : 10 May 2024 07:01
Operator : YP\AJ
Sample : PB160785BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB160785BL

Integration File: autoint1.e
Quant Time: May 11 00:38:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050924.M
Quant Title :
QLast Update : Fri May 10 23:54:11 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.048	2277050	19.752 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051024\
Data File : FE048072.D
Signal(s) : FID1B.ch
Acq On : 10 May 2024 07:01
Operator : YP\AJ
Sample : PB160785BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB160785BL

Integration File: autoint1.e
Quant Time: May 11 00:38:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050924.M
Quant Title :
QLast Update : Fri May 10 23:54:11 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

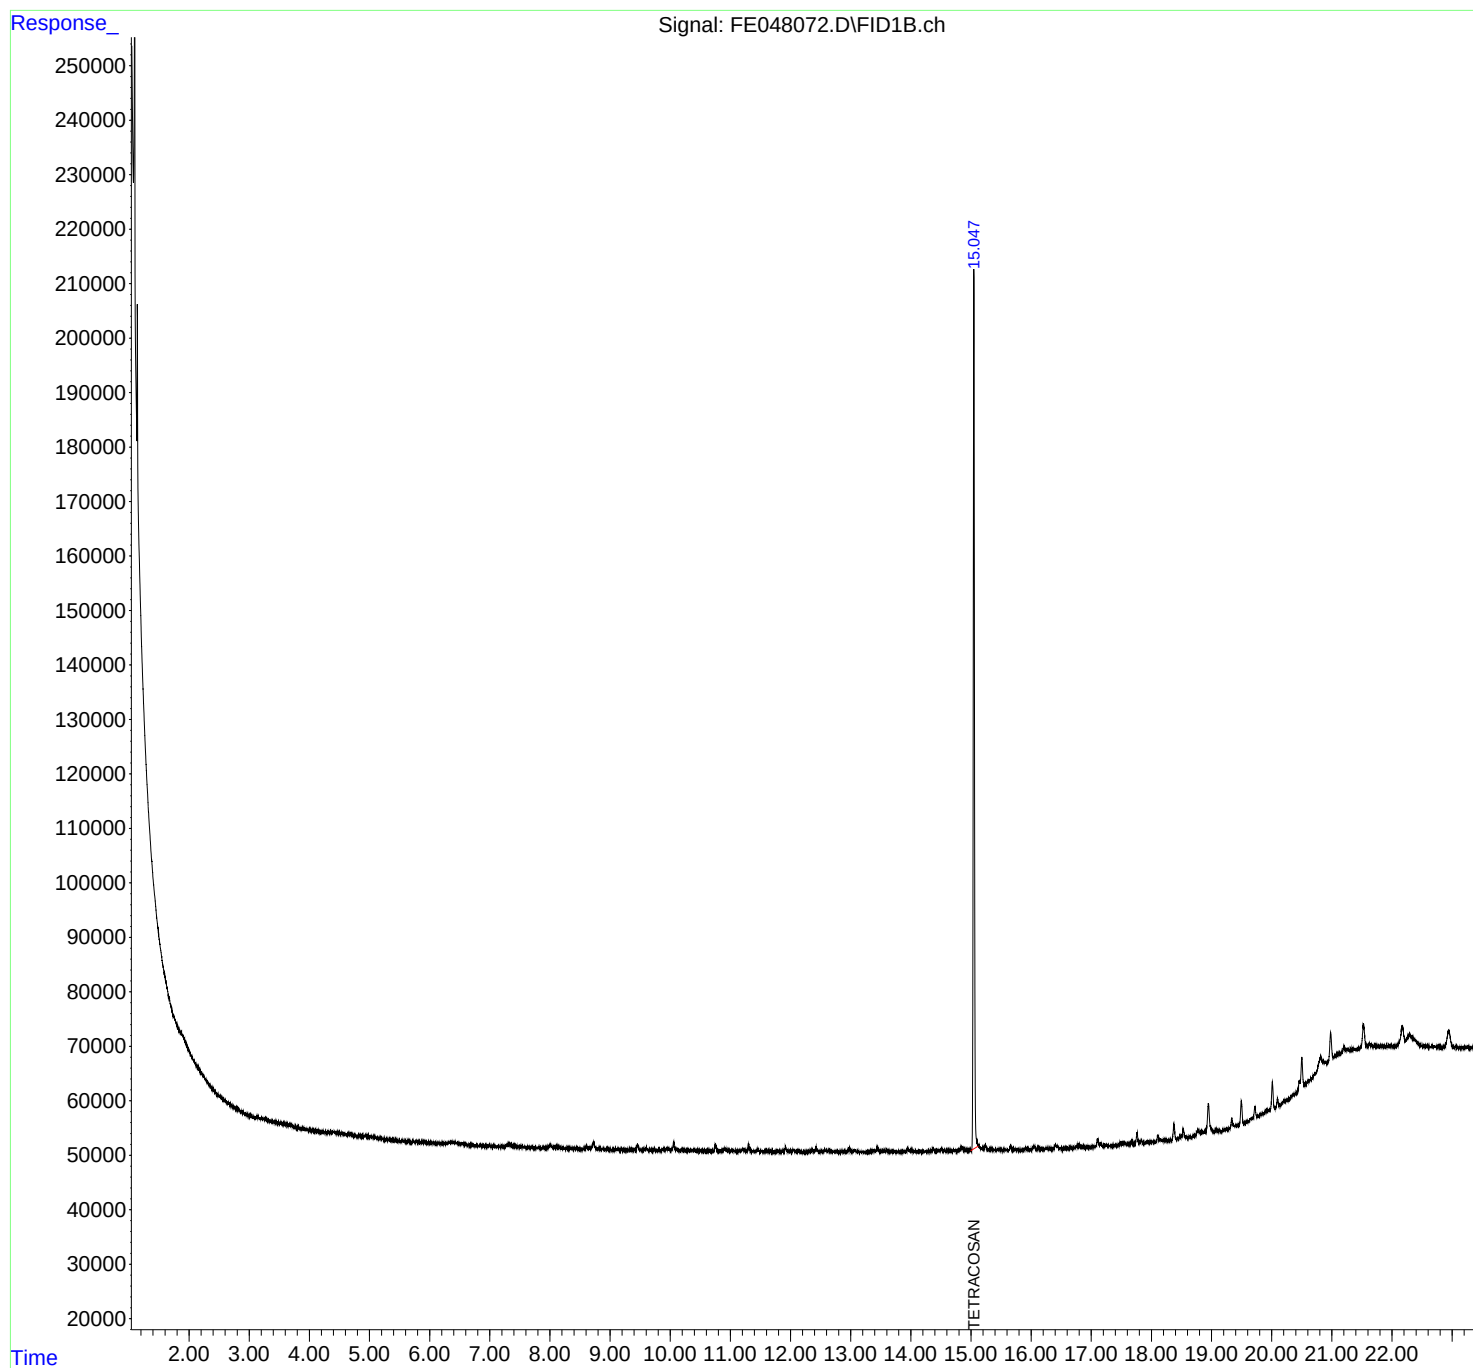

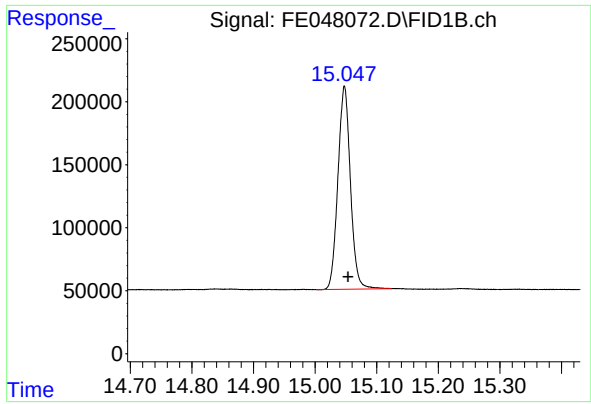

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.048 min
Delta R.T.: -0.006 min
Response: 2277050
Conc: 19.75 ug/ml

Instrument :
FID_E
ClientSampleId :
PB160785BL