

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051024AL\
 Data File : FE048111.D
 Signal(s) : FID1B.ch
 Acq On : 11 May 2024 05:12
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 11 06:32:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042724.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 29 03:29:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.943	118124	0.855 ug/ml
20) T n-Hexatriacontane (C36)	20.498	101800	0.752 ug/ml
22) T n-Tetracontane (C40)	22.169	94456	0.678 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051024AL\
Data File : FE048111.D
Signal(s) : FID1B.ch
Acq On : 11 May 2024 05:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 06:32:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042724.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 03:29:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

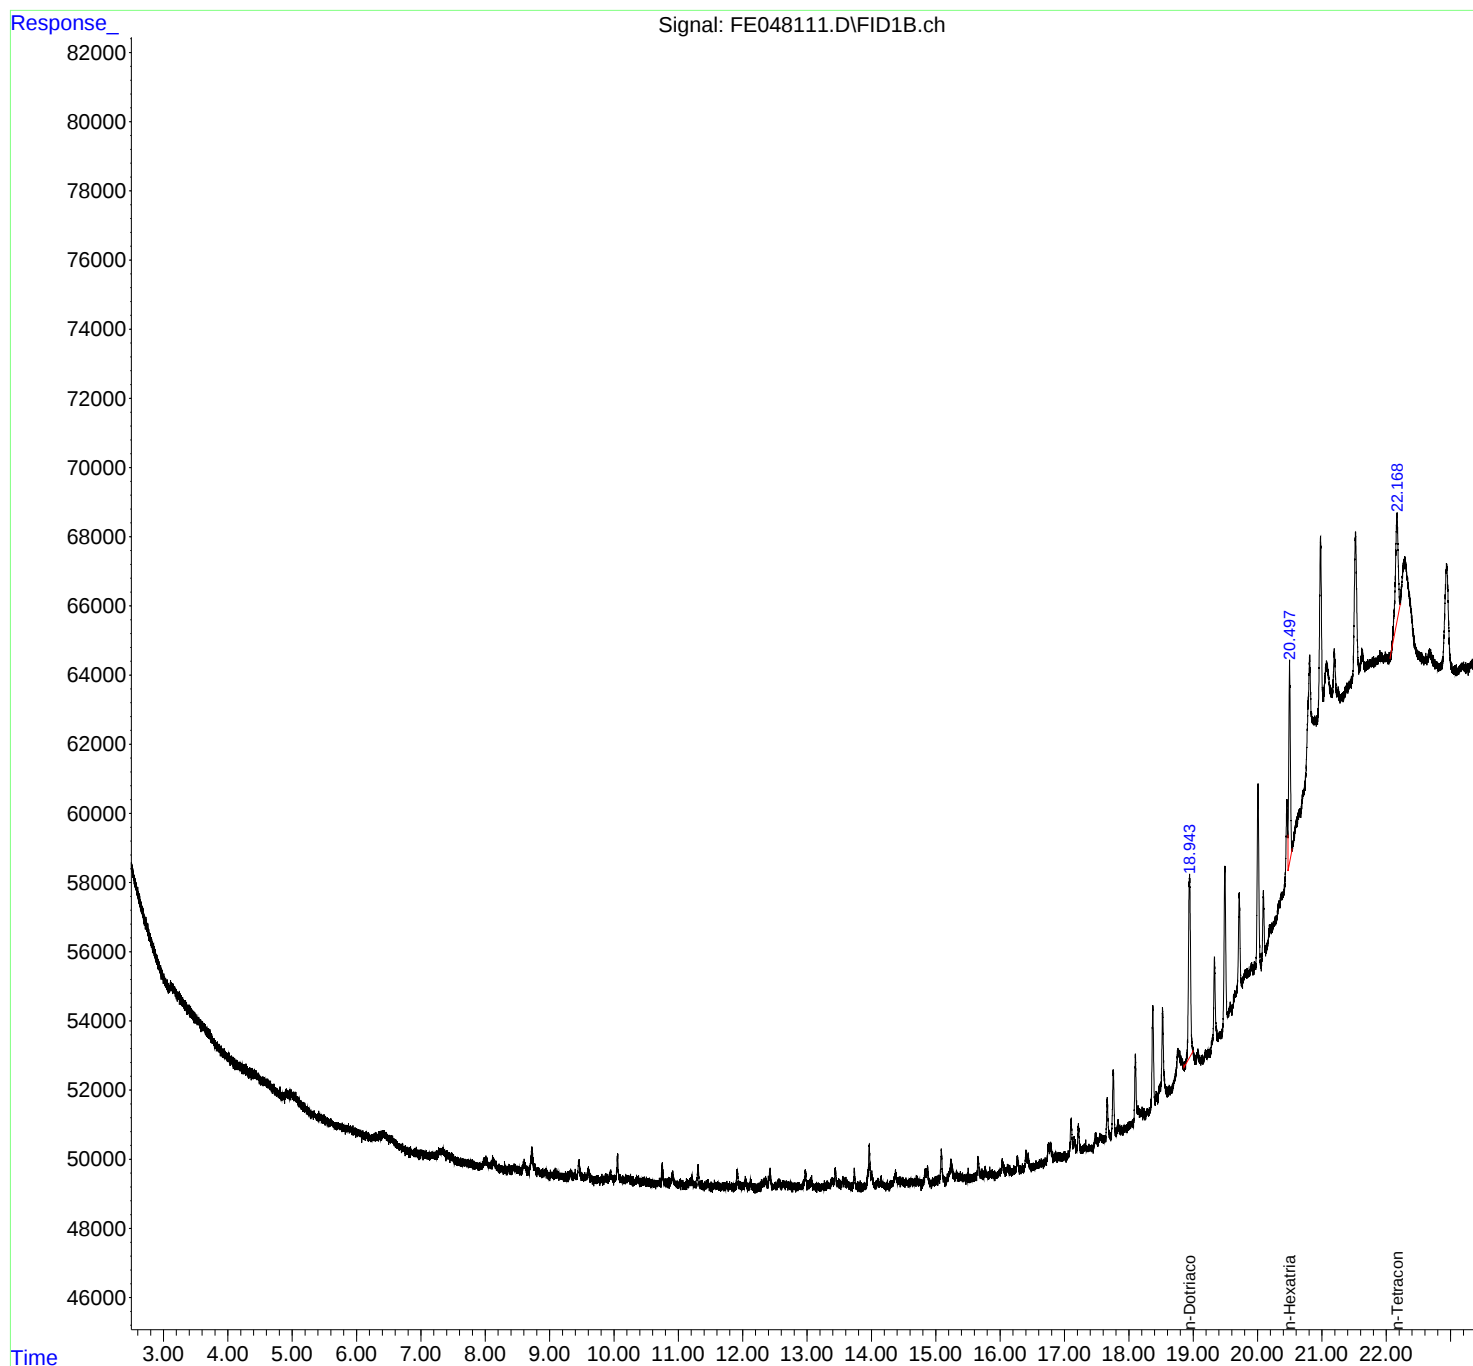


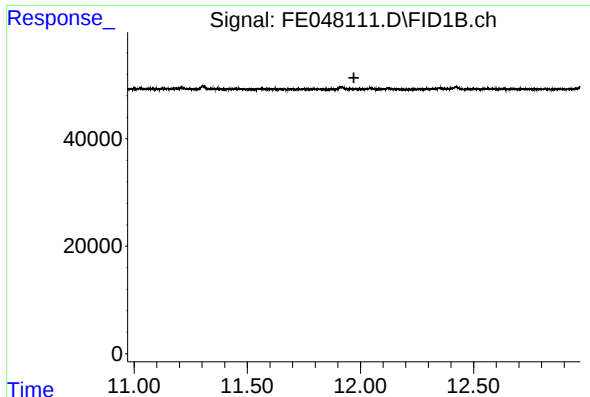

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.971 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

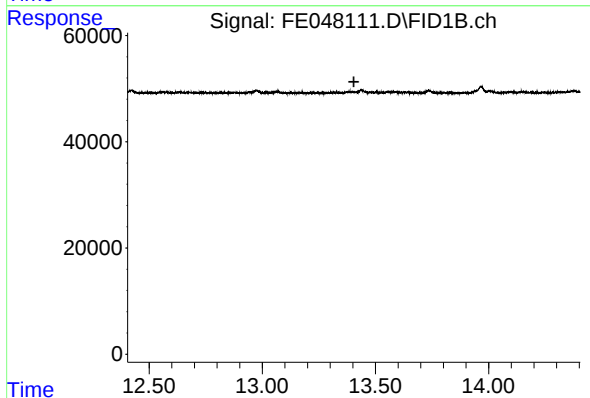


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.405 min
Response: 0
Conc: N.D.

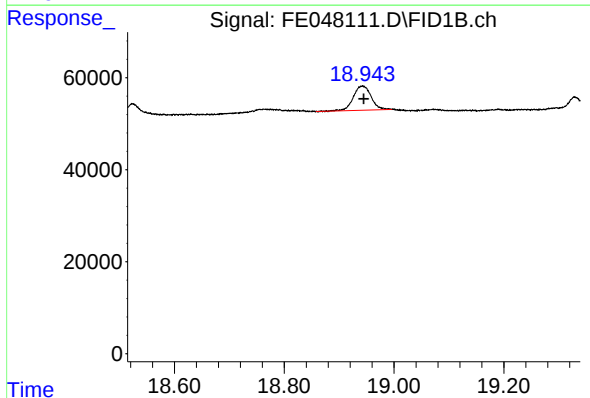


#18 n-Dotriacontane (C32)

R.T.: 18.943 min
Delta R.T.: -0.002 min
Response: 118124
Conc: 0.86 ug/ml

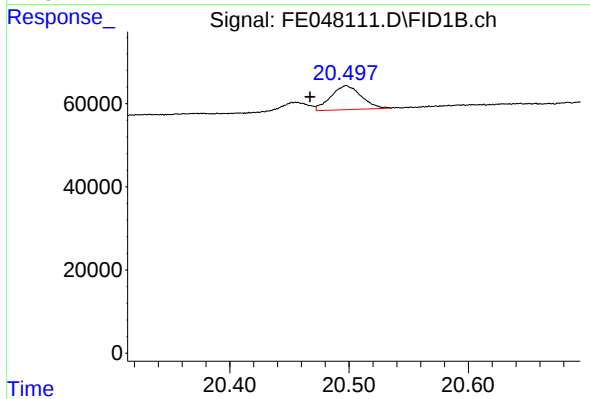

#20 n-Hexatriacontane (C36)

R.T.: 20.498 min
Delta R.T.: 0.030 min
Response: 101800
Conc: 0.75 ug/ml

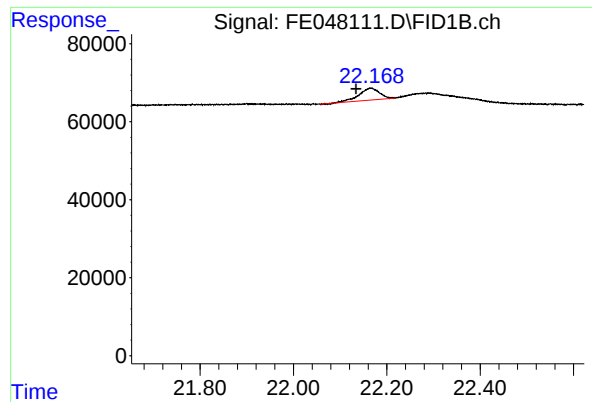

#22 n-Tetracontane (C40)

R.T.: 22.169 min
Delta R.T.: 0.035 min
Response: 94456
Conc: 0.68 ug/ml

Instrument :

FID_E

ClientSampleId :