

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051122\  
Data File : FE035638.D  
Signal(s) : FID1B.CH  
Acq On : 11 May 2022 21:16  
Operator : YP\AJ  
Sample : N2762-07  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 12 01:10:39 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE051122.M  
Quant Title :  
QLast Update : Wed May 11 13:51:27 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.040  | 2060154  | 16.704 ug/ml |
| Target Compounds              |         |          |              |
| 7) N-EICOSANE                 | 12.002f | 82435    | 0.582 ug/ml  |
| 14) N-DOTRIACONTANE           | 17.915  | 234310   | 1.876 ug/ml  |
| 15) N-TETRATRIACONTANE        | 18.769f | 134721   | 1.363 ug/ml  |
| -----                         |         |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051122\  
Data File : FE035638.D  
Signal(s) : FID1B.CH  
Acq On : 11 May 2022 21:16  
Operator : YP\AJ  
Sample : N2762-07  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 12 01:10:39 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE051122.M  
Quant Title :  
QLast Update : Wed May 11 13:51:27 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

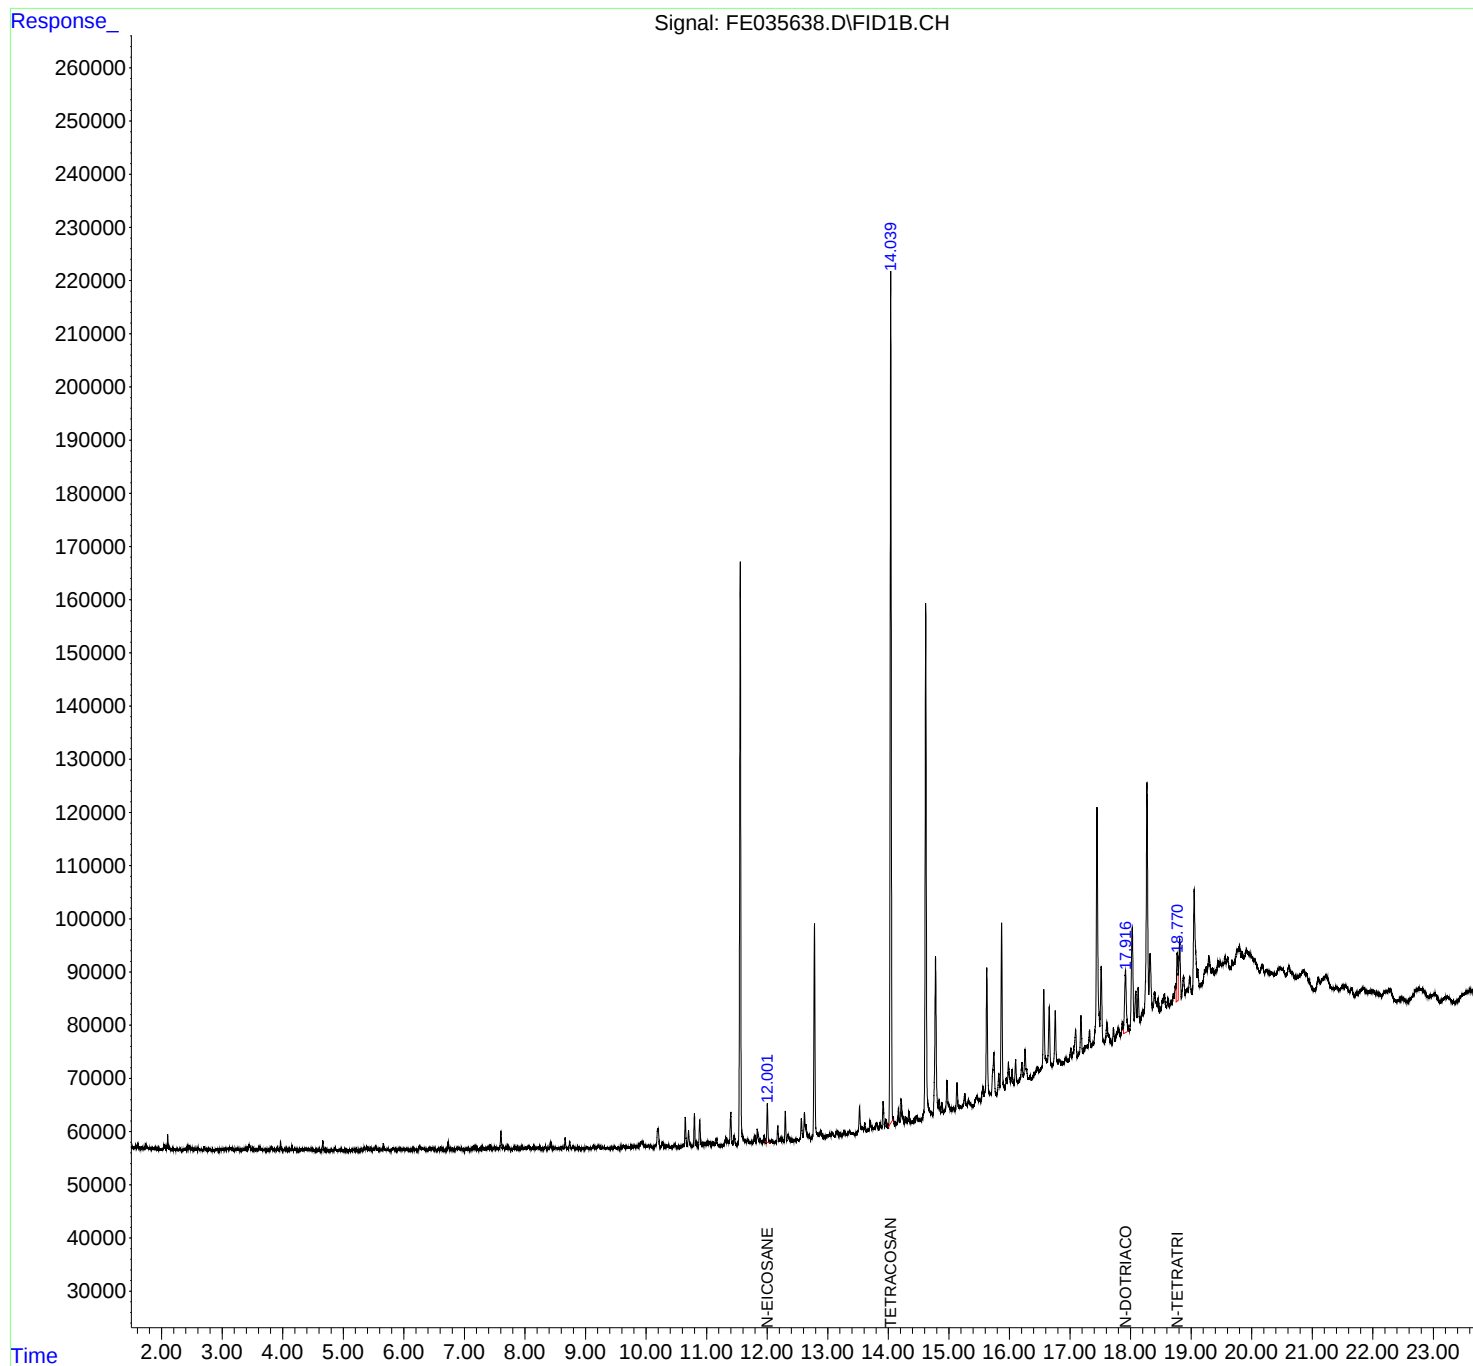

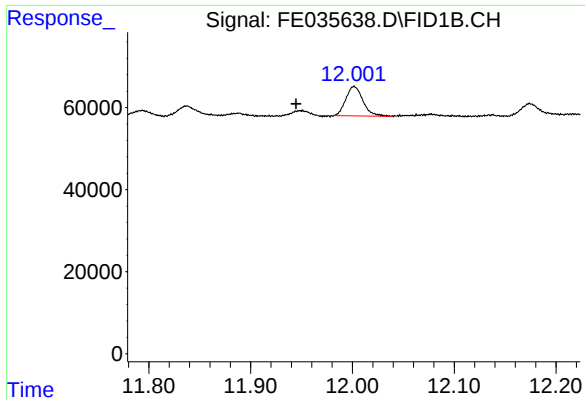


#7 N-EICOSANE

R.T.: 12.002 min  
Delta R.T.: 0.057 min  
Response: 82435  
Conc: 0.58 ug/ml

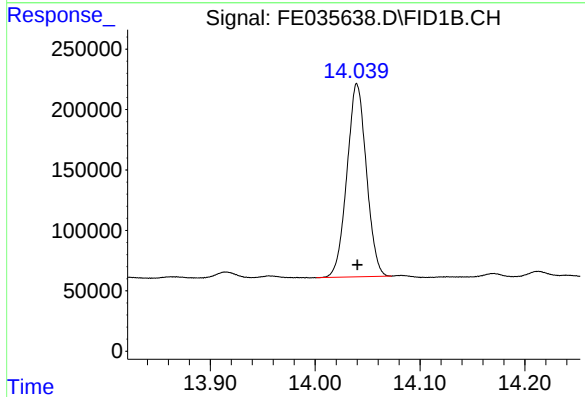


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.040 min  
Delta R.T.: 0.000 min  
Response: 2060154  
Conc: 16.70 ug/ml

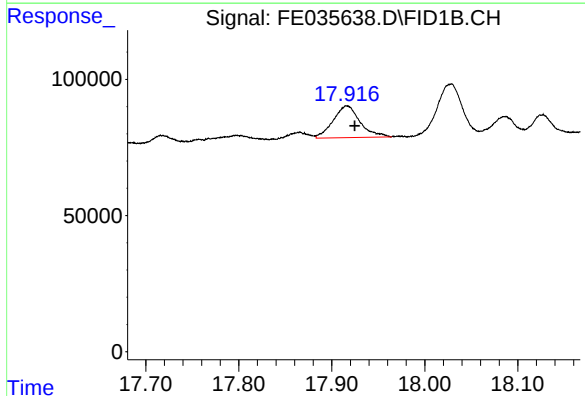

#14 N-DOTRIACONTANE

R.T.: 17.915 min  
Delta R.T.: -0.010 min  
Response: 234310  
Conc: 1.88 ug/ml

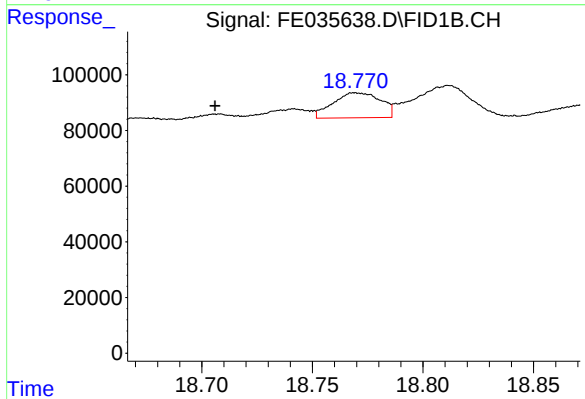

#15 N-TETRATRIACONTANE

R.T.: 18.769 min  
Delta R.T.: 0.063 min  
Response: 134721  
Conc: 1.36 ug/ml