

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051122\
 Data File : FE035626.D
 Signal(s) : FID1B.CH
 Acq On : 11 May 2022 15:02
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: May 12 01:08:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051122.M
 Quant Title :
 QLast Update : Wed May 11 13:51:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.041	5933272	48.107 ug/ml
Target Compounds			
2) N-DECANE	3.822	6691782	47.764 ug/ml
3) N-DODECANE	5.816	6725878	47.704 ug/ml
4) N-TETRADECANE	7.606	6799265	47.627 ug/ml
5) N-HEXADECANE	9.203	6817789	47.680 ug/ml
6) N-OCTADECANE	10.642	6974767	47.835 ug/ml
7) N-EICOSANE	11.949	6798940	48.000 ug/ml
8) N-DOCOSANE	13.144	6748026	48.094 ug/ml
10) N-TETRACOSANE	14.246	6750214	48.007 ug/ml
11) N-HEXACOSANE	15.263	6705114	47.952 ug/ml
12) N-OCTACOSANE	16.212	6615327	47.708 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051122\
Data File : FE035626.D
Signal(s) : FID1B.CH
Acq On : 11 May 2022 15:02
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: May 12 01:08:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051122.M
Quant Title :
QLast Update : Wed May 11 13:51:27 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

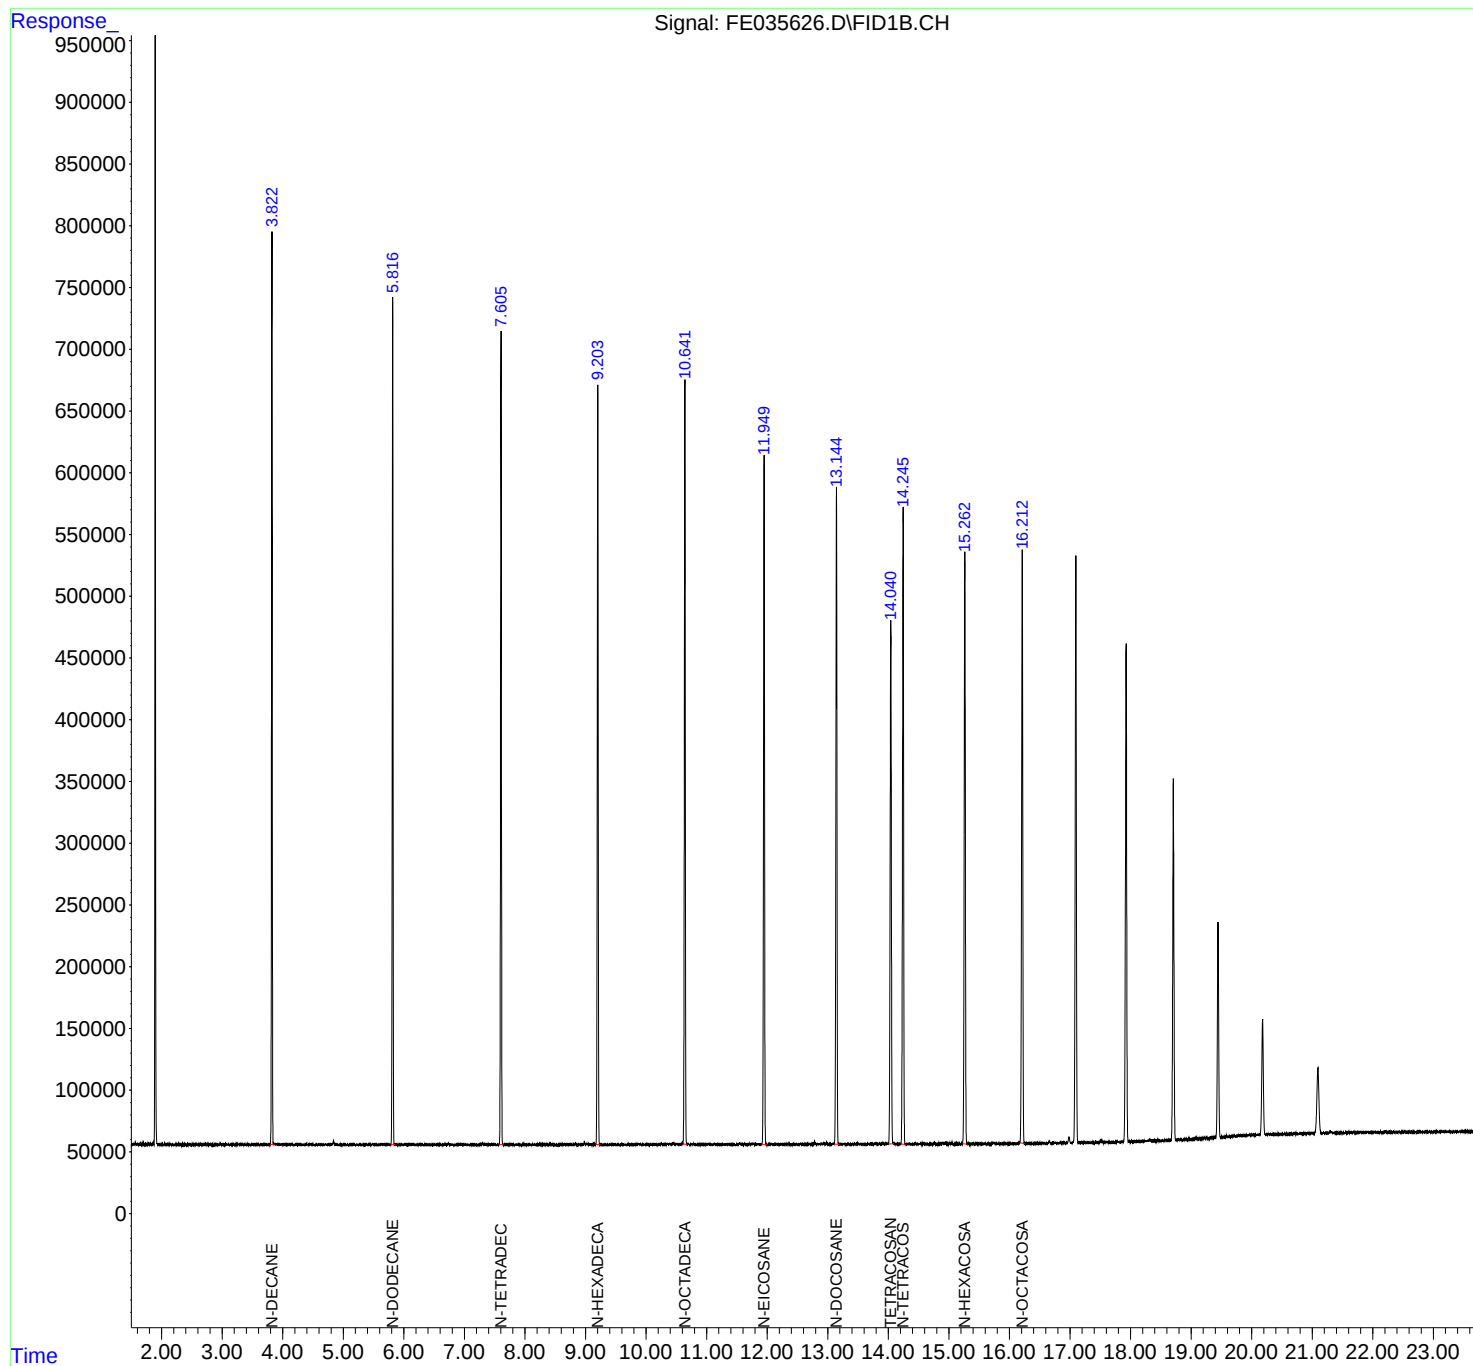

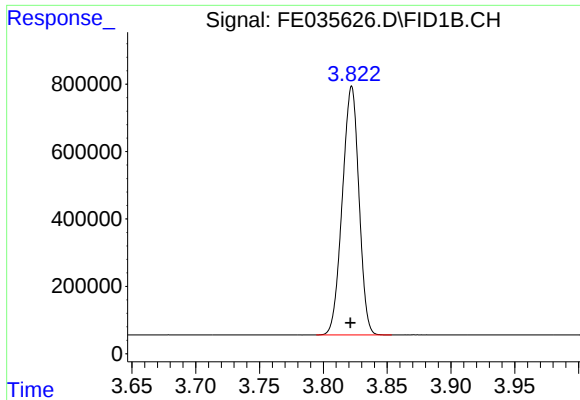


#2 N-DECANE

R.T.: 3.822 min
Delta R.T.: 0.001 min
Response: 6691782
Conc: 47.76 ug/ml

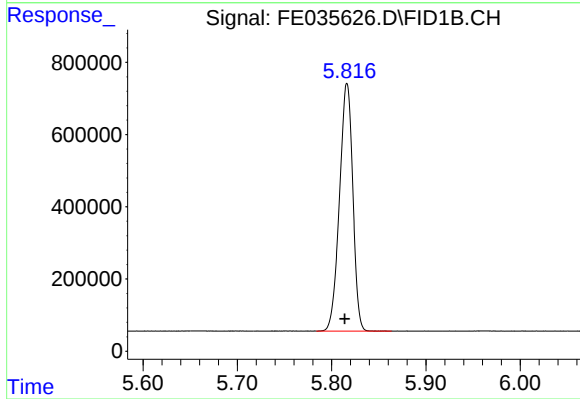


#3 N-DODECANE

R.T.: 5.816 min
Delta R.T.: 0.002 min
Response: 6725878
Conc: 47.70 ug/ml

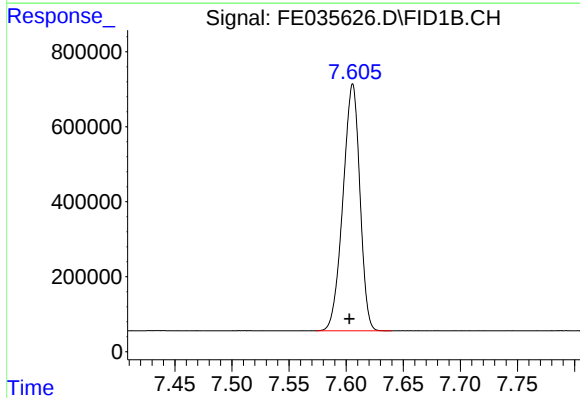


#4 N-TETRADECANE

R.T.: 7.606 min
Delta R.T.: 0.003 min
Response: 6799265
Conc: 47.63 ug/ml

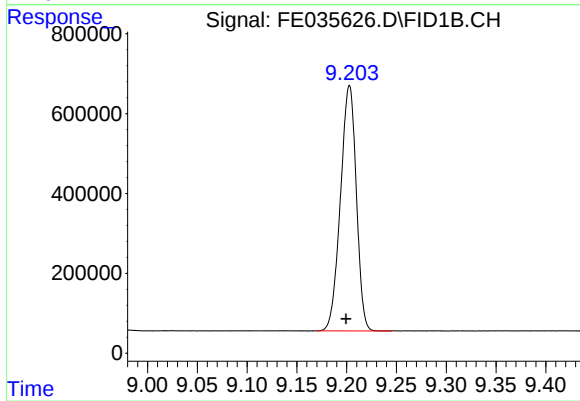


#5 N-HEXADECANE

R.T.: 9.203 min
Delta R.T.: 0.004 min
Response: 6817789
Conc: 47.68 ug/ml

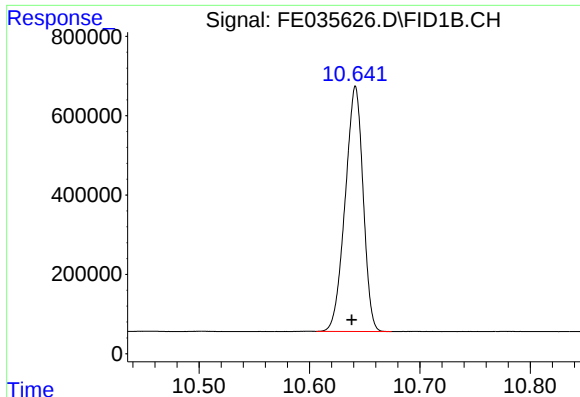


#6 N-OCTADECANE

R.T.: 10.642 min
Delta R.T.: 0.003 min
Response: 6974767
Conc: 47.83 ug/ml

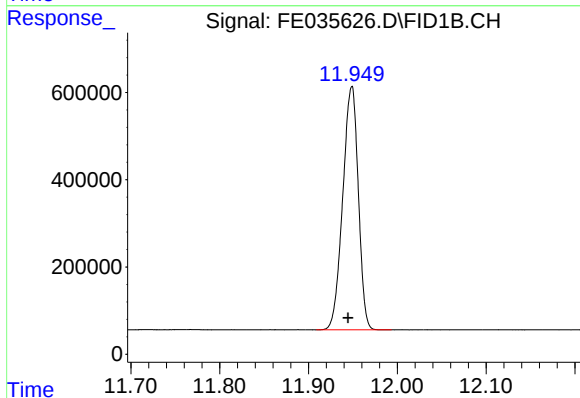


#7 N-EICOSANE

R.T.: 11.949 min
Delta R.T.: 0.004 min
Response: 6798940
Conc: 48.00 ug/ml

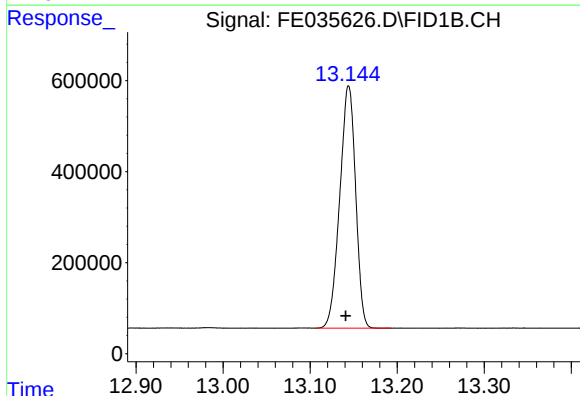


#8 N-DOCOSANE

R.T.: 13.144 min
Delta R.T.: 0.003 min
Response: 6748026
Conc: 48.09 ug/ml

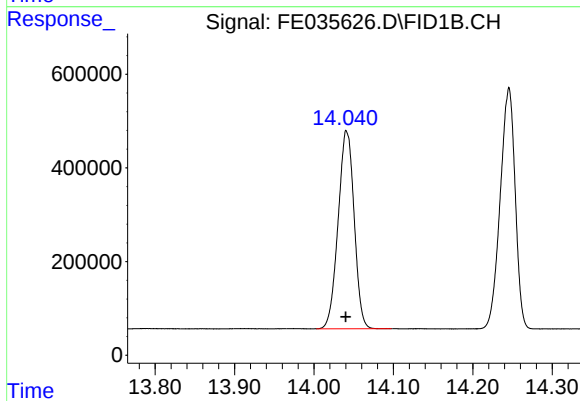


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.041 min
Delta R.T.: 0.000 min
Response: 5933272
Conc: 48.11 ug/ml

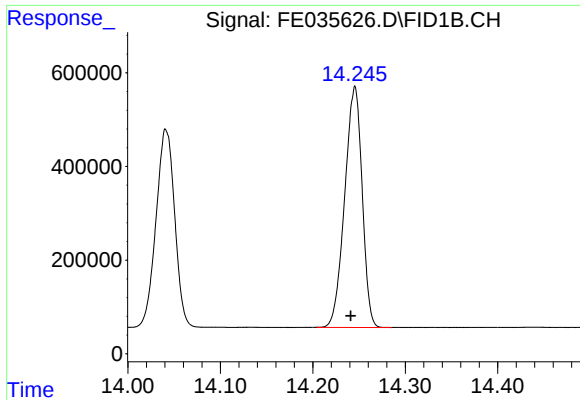


#10 N-TETRACOSANE

R.T.: 14.246 min
Delta R.T.: 0.005 min
Response: 6750214
Conc: 48.01 ug/ml

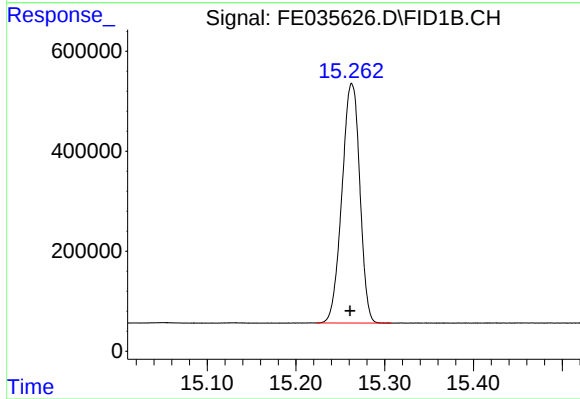

#11 N-HEXACOSANE

R.T.: 15.263 min
Delta R.T.: 0.002 min
Response: 6705114
Conc: 47.95 ug/ml

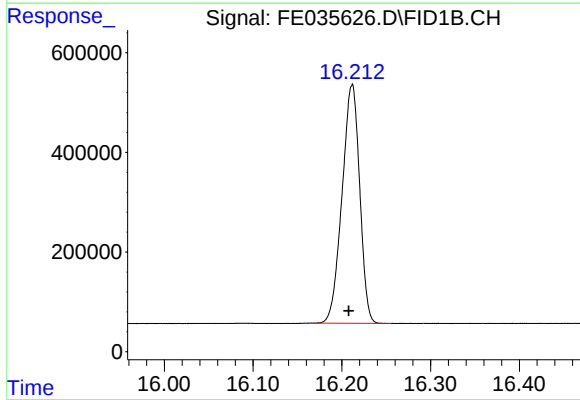

#12 N-OCTACOSANE

R.T.: 16.212 min
Delta R.T.: 0.004 min
Response: 6615327
Conc: 47.71 ug/ml