

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051122\  
 Data File : FE035636.D  
 Signal(s) : FID1B.CH  
 Acq On : 11 May 2022 20:14  
 Operator : YP\AJ  
 Sample : N2762-06MS  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Integration File: Sample.e  
 Quant Time: May 12 01:10:15 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE051122.M  
 Quant Title :  
 QLast Update : Wed May 11 13:51:27 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.040 | 1756953  | 14.245 ug/ml |
| Target Compounds              |        |          |              |
| 2) N-DECANE                   | 3.822  | 2110271  | 15.062 ug/ml |
| 3) N-DODECANE                 | 5.815  | 2165802  | 15.361 ug/ml |
| 4) N-TETRADECANE              | 7.604  | 2241573  | 15.701 ug/ml |
| 5) N-HEXADECANE               | 9.201  | 2240205  | 15.667 ug/ml |
| 6) N-OCTADECANE               | 10.640 | 2272940  | 15.588 ug/ml |
| 7) N-EICOSANE                 | 11.948 | 2248916  | 15.877 ug/ml |
| 8) N-DOCOSANE                 | 13.143 | 2248205  | 16.023 ug/ml |
| 10) N-TETRACOSANE             | 14.243 | 2241566  | 15.942 ug/ml |
| 11) N-HEXACOSANE              | 15.262 | 2226165  | 15.921 ug/ml |
| 12) N-OCTACOSANE              | 16.210 | 2257432  | 16.280 ug/ml |
| -----                         |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051122\  
Data File : FE035636.D  
Signal(s) : FID1B.CH  
Acq On : 11 May 2022 20:14  
Operator : YP\AJ  
Sample : N2762-06MS  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Integration File: Sample.e  
Quant Time: May 12 01:10:15 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE051122.M  
Quant Title :  
QLast Update : Wed May 11 13:51:27 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

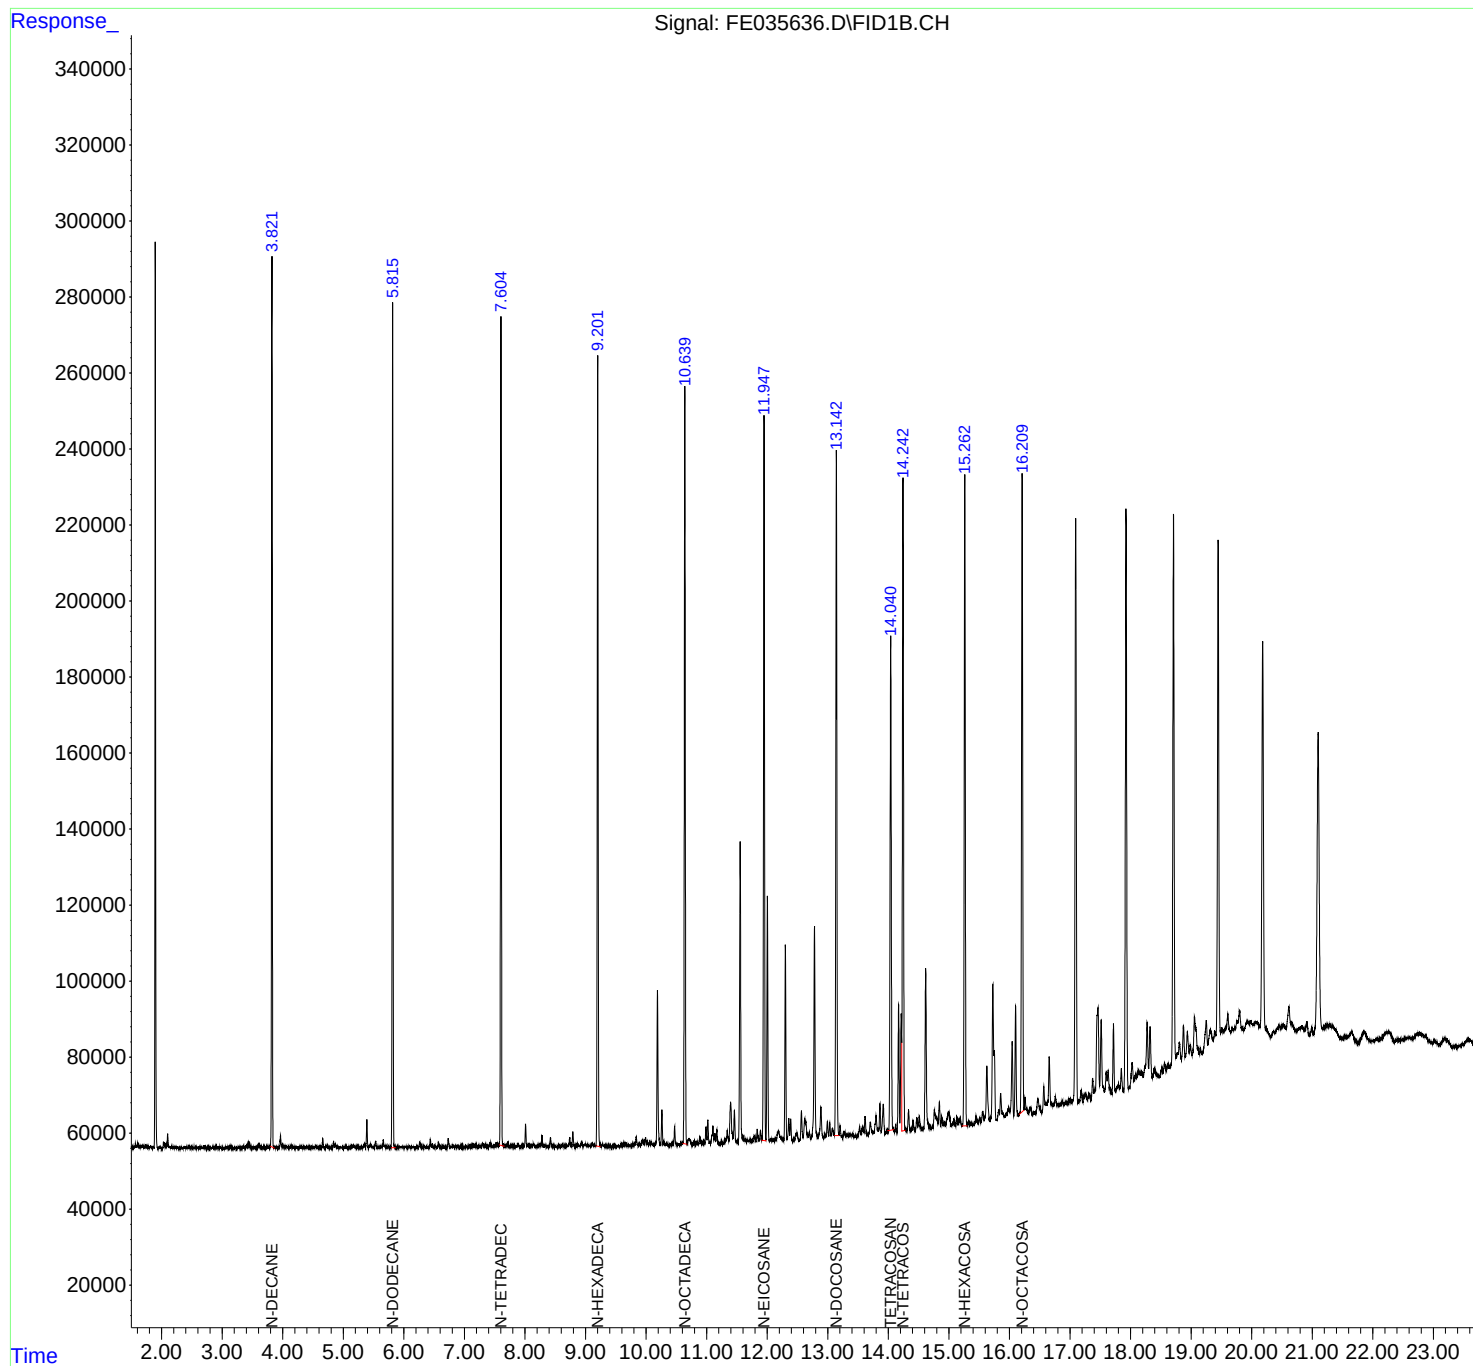

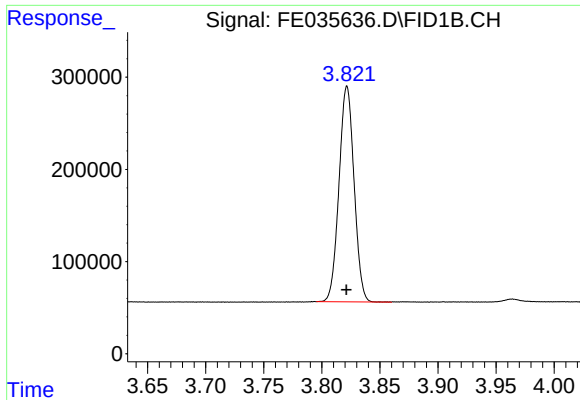


#2 N-DECANE

R.T.: 3.822 min  
Delta R.T.: 0.000 min  
Response: 2110271  
Conc: 15.06 ug/ml

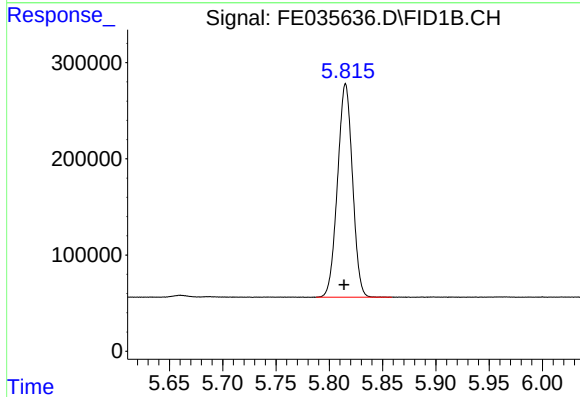


#3 N-DODECANE

R.T.: 5.815 min  
Delta R.T.: 0.001 min  
Response: 2165802  
Conc: 15.36 ug/ml

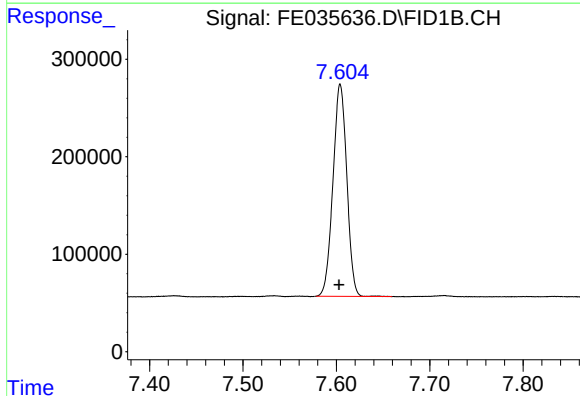


#4 N-TETRADECANE

R.T.: 7.604 min  
Delta R.T.: 0.001 min  
Response: 2241573  
Conc: 15.70 ug/ml

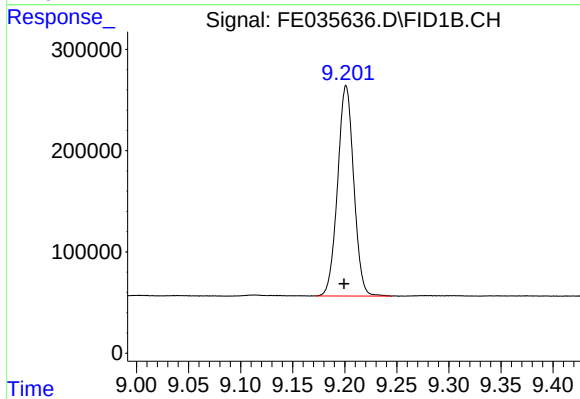


#5 N-HEXADECANE

R.T.: 9.201 min  
Delta R.T.: 0.002 min  
Response: 2240205  
Conc: 15.67 ug/ml

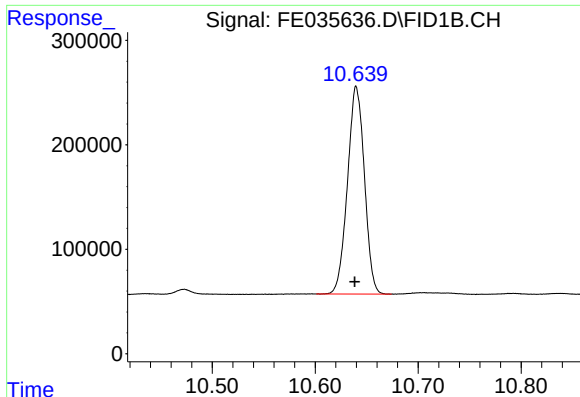


#6 N-OCTADECANE

R.T.: 10.640 min  
Delta R.T.: 0.001 min  
Response: 2272940  
Conc: 15.59 ug/ml

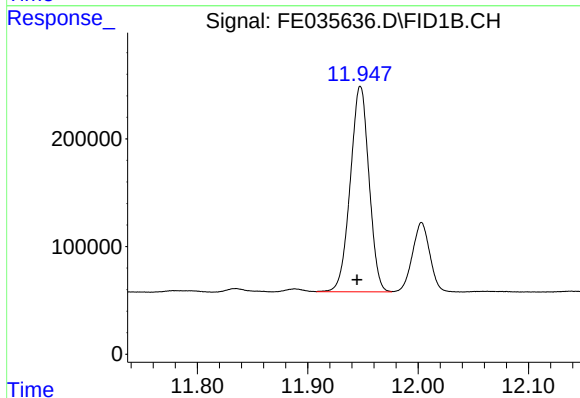


#7 N-EICOSANE

R.T.: 11.948 min  
Delta R.T.: 0.003 min  
Response: 2248916  
Conc: 15.88 ug/ml

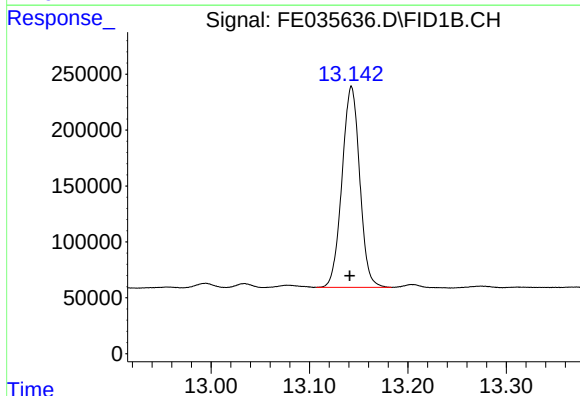


#8 N-DOCOSANE

R.T.: 13.143 min  
Delta R.T.: 0.002 min  
Response: 2248205  
Conc: 16.02 ug/ml

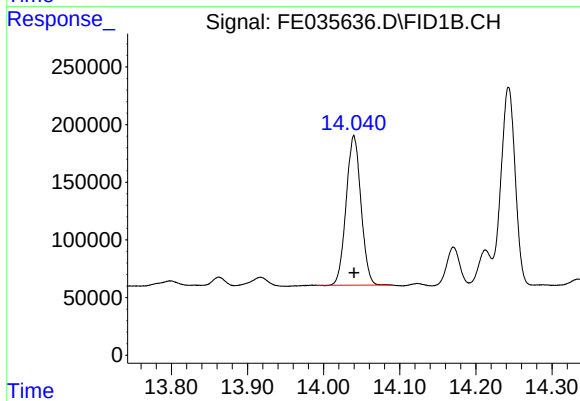


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.040 min  
Delta R.T.: 0.000 min  
Response: 1756953  
Conc: 14.25 ug/ml

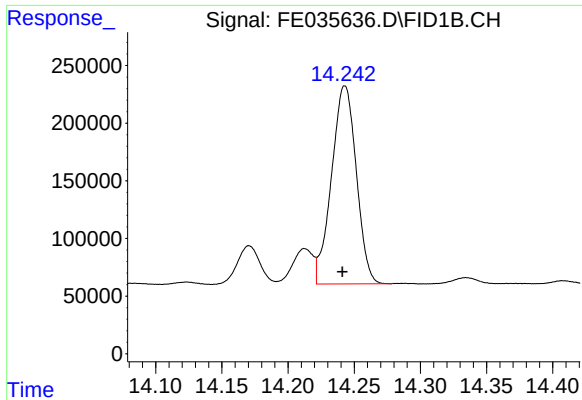


#10 N-TETRACOSANE

R.T.: 14.243 min  
Delta R.T.: 0.002 min  
Response: 2241566  
Conc: 15.94 ug/ml

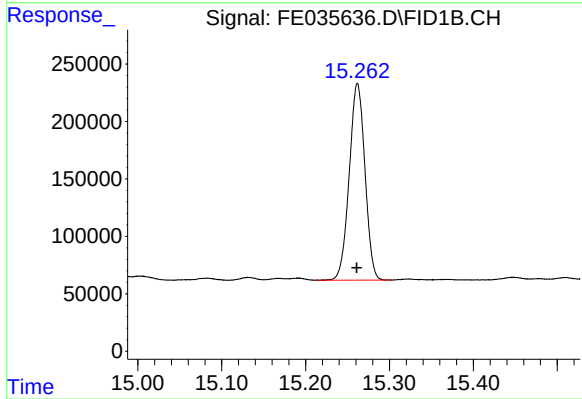

#11 N-HEXACOSANE

R.T.: 15.262 min  
Delta R.T.: 0.000 min  
Response: 2226165  
Conc: 15.92 ug/ml

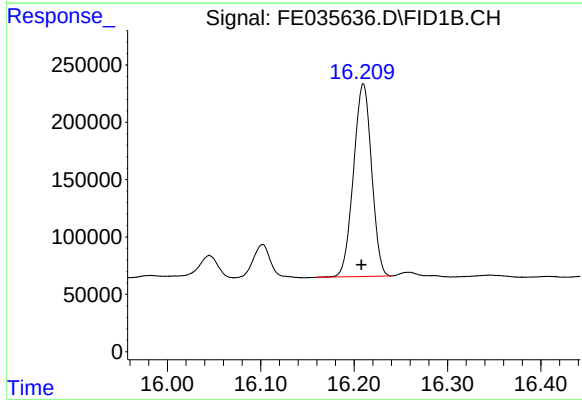

#12 N-OCTACOSANE

R.T.: 16.210 min  
Delta R.T.: 0.002 min  
Response: 2257432  
Conc: 16.28 ug/ml