

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051122\
 Data File : FE035642.D
 Signal(s) : FID1B.CH
 Acq On : 11 May 2022 23:20
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: May 12 01:25:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051122.M
 Quant Title :
 QLast Update : Wed May 11 13:51:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.043	5645019	45.769 ug/ml
Target Compounds			
2) N-DECANE	3.824	6627146	47.302 ug/ml
3) N-DODECANE	5.818	6610669	46.887 ug/ml
4) N-TETRADECANE	7.607	6646519	46.557 ug/ml
5) N-HEXADECANE	9.205	6638545	46.427 ug/ml
6) N-OCTADECANE	10.644	6773311	46.453 ug/ml
7) N-EICOSANE	11.950	6554409	46.273 ug/ml
8) N-DOCOSANE	13.147	6465302	46.079 ug/ml
10) N-TETRACOSANE	14.247	6419052	45.652 ug/ml
11) N-HEXACOSANE	15.265	6310986	45.134 ug/ml
12) N-OCTACOSANE	16.213	6169502	44.493 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051122\
Data File : FE035642.D
Signal(s) : FID1B.CH
Acq On : 11 May 2022 23:20
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: May 12 01:25:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051122.M
Quant Title :
QLast Update : Wed May 11 13:51:27 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

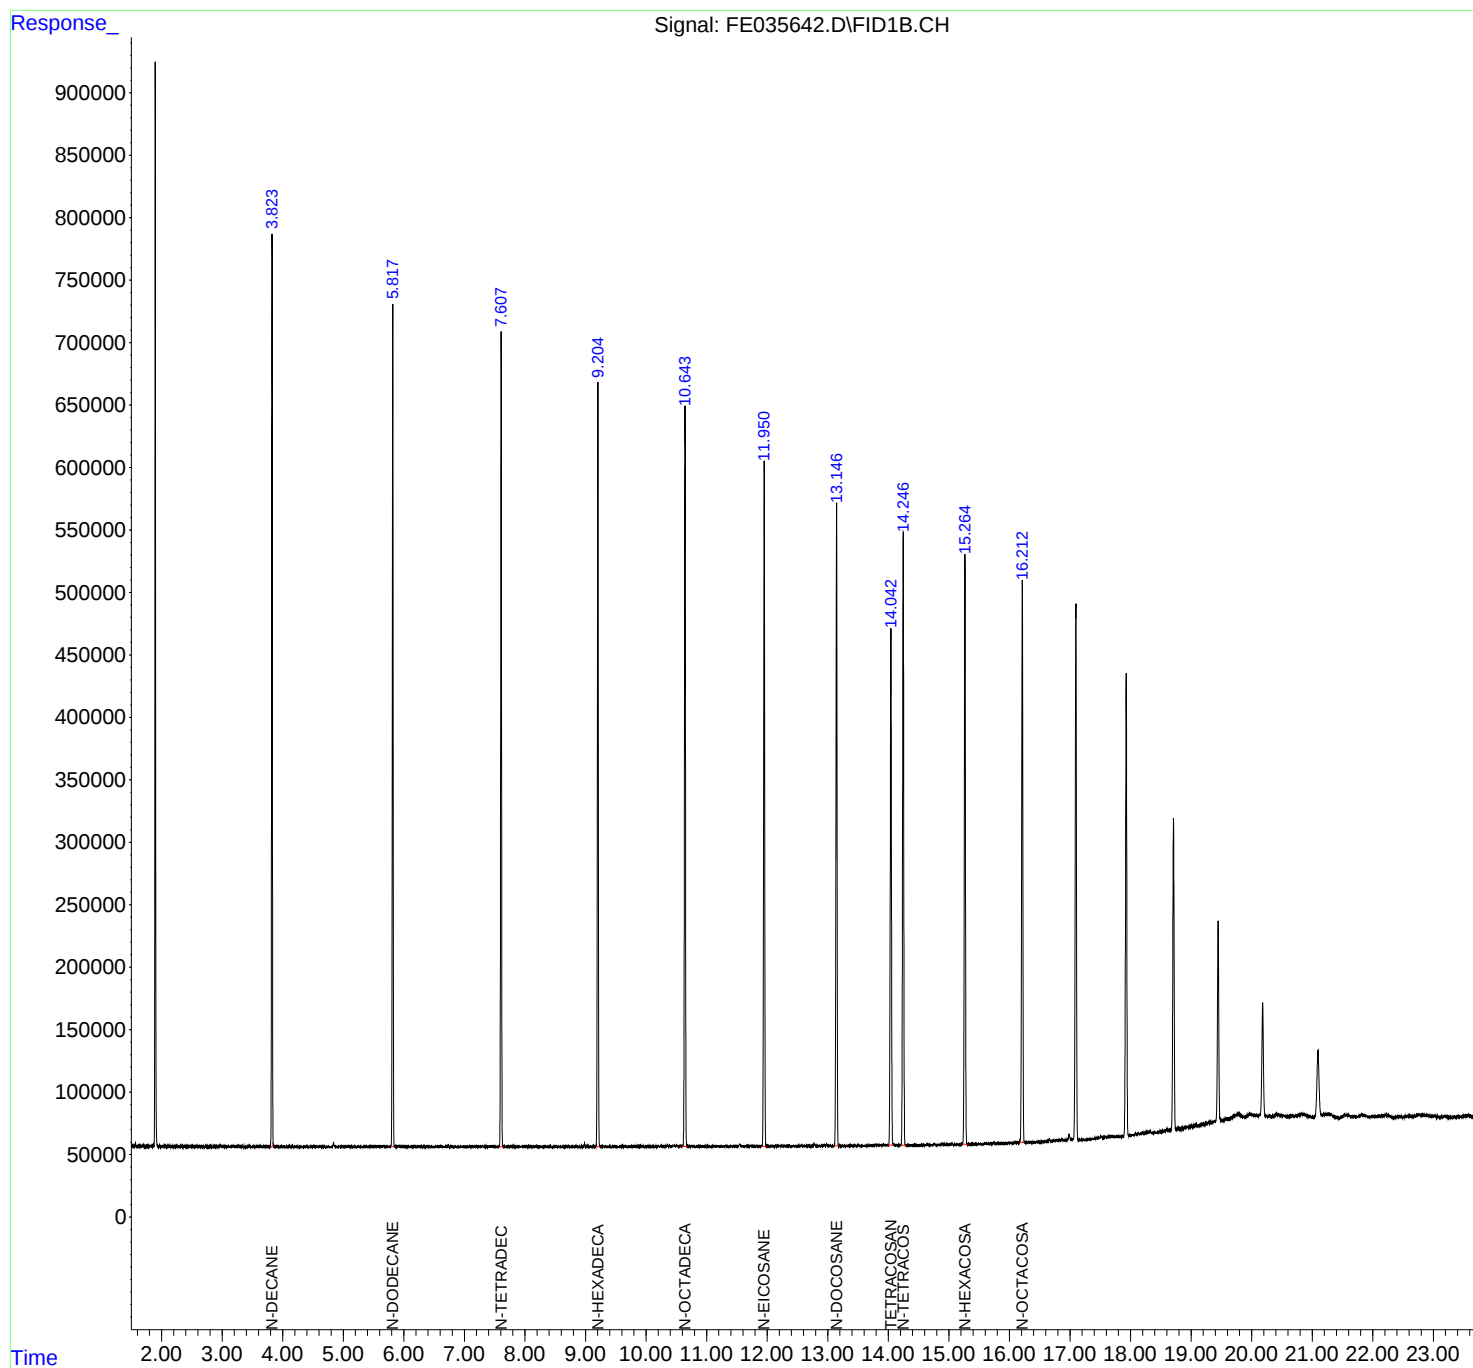

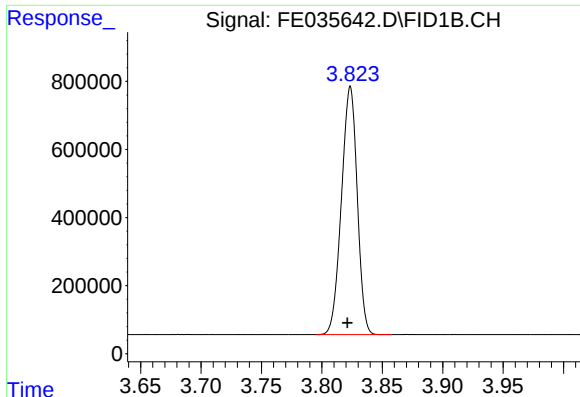


#2 N-DECANE

R.T.: 3.824 min
Delta R.T.: 0.002 min
Response: 6627146
Conc: 47.30 ug/ml

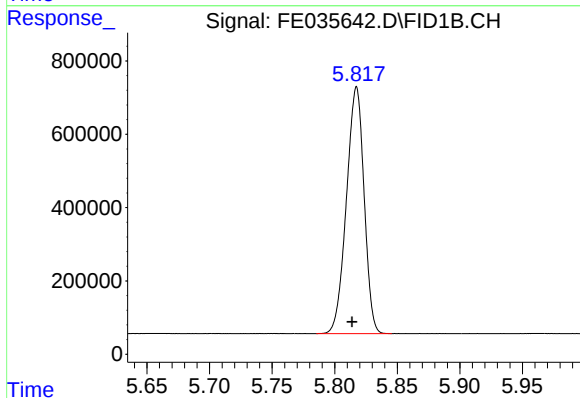


#3 N-DODECANE

R.T.: 5.818 min
Delta R.T.: 0.004 min
Response: 6610669
Conc: 46.89 ug/ml

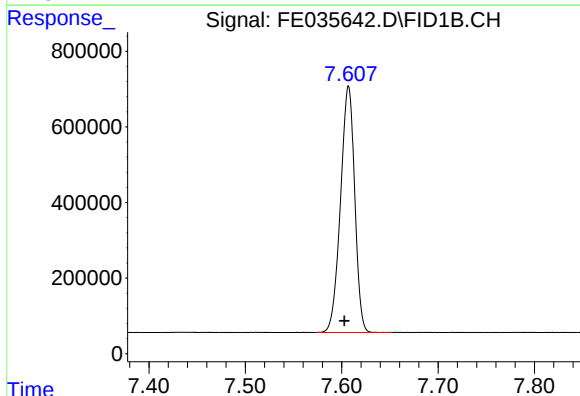


#4 N-TETRADECANE

R.T.: 7.607 min
Delta R.T.: 0.004 min
Response: 6646519
Conc: 46.56 ug/ml

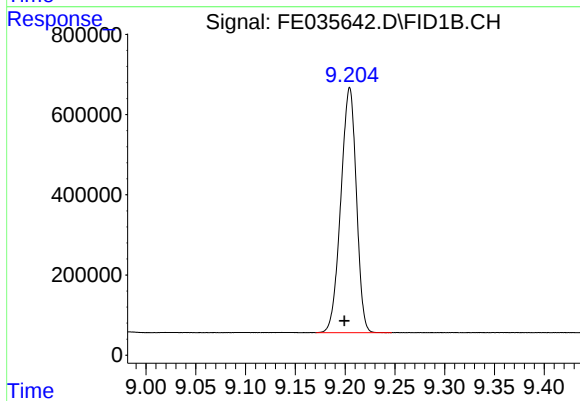


#5 N-HEXADECANE

R.T.: 9.205 min
Delta R.T.: 0.005 min
Response: 6638545
Conc: 46.43 ug/ml

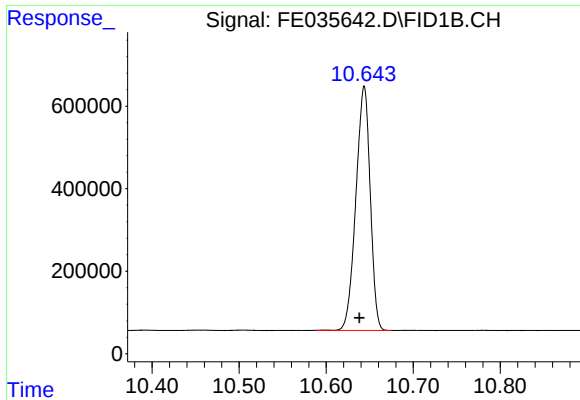


#6 N-OCTADECANE

R.T.: 10.644 min
Delta R.T.: 0.005 min
Response: 6773311
Conc: 46.45 ug/ml

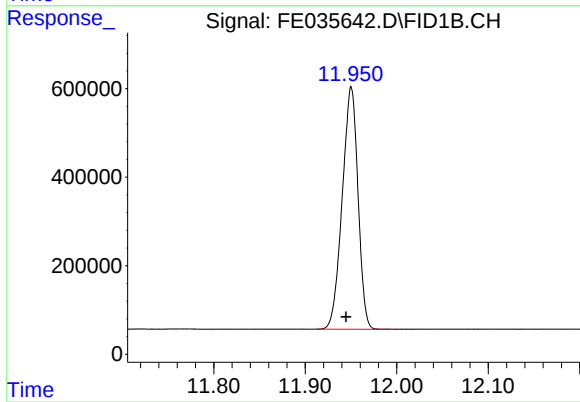


#7 N-EICOSANE

R.T.: 11.950 min
Delta R.T.: 0.006 min
Response: 6554409
Conc: 46.27 ug/ml

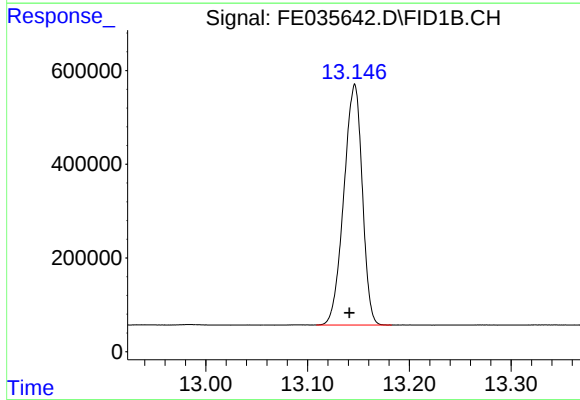


#8 N-DOCOSANE

R.T.: 13.147 min
Delta R.T.: 0.005 min
Response: 6465302
Conc: 46.08 ug/ml

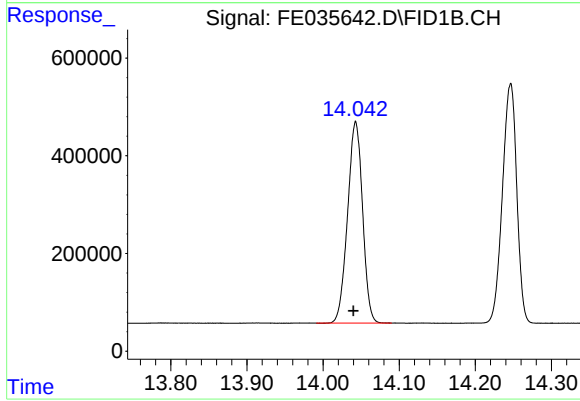


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.043 min
Delta R.T.: 0.003 min
Response: 5645019
Conc: 45.77 ug/ml

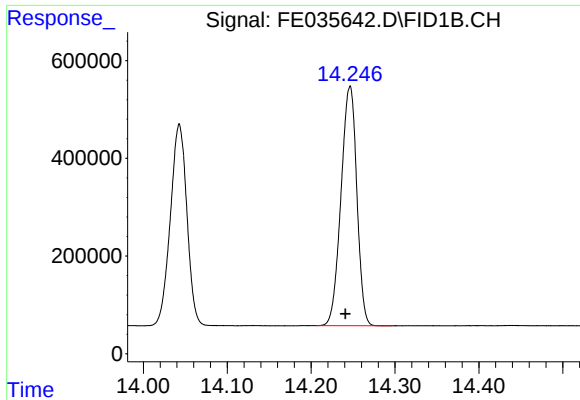


#10 N-TETRACOSANE

R.T.: 14.247 min
Delta R.T.: 0.006 min
Response: 6419052
Conc: 45.65 ug/ml

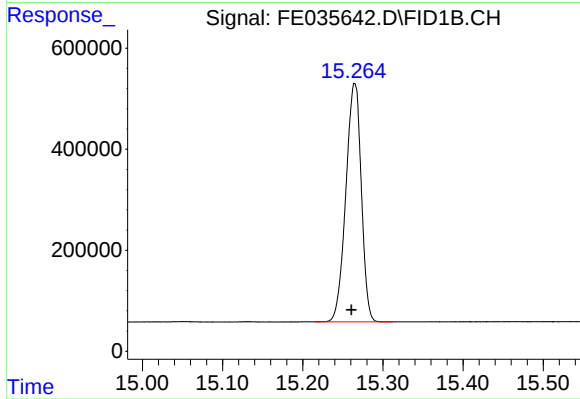

#11 N-HEXACOSANE

R.T.: 15.265 min
Delta R.T.: 0.004 min
Response: 6310986
Conc: 45.13 ug/ml

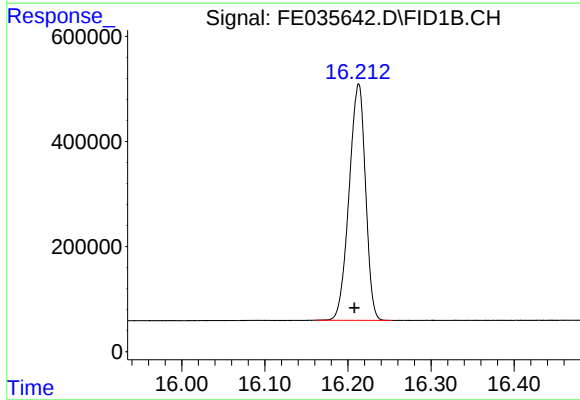

#12 N-OCTACOSANE

R.T.: 16.213 min
Delta R.T.: 0.005 min
Response: 6169502
Conc: 44.49 ug/ml