

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051124\
 Data File : FE048138.D
 Signal(s) : FID1B.ch
 Acq On : 12 May 2024 02:35
 Operator : YP\AJ
 Sample : P2403-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 14 01:48:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050924.M
 Quant Title :
 QLast Update : Fri May 10 23:54:11 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.041	2686112	23.300 ug/ml
Target Compounds			
2) N-DECANE	4.593	169623	1.221 ug/ml
3) N-DODECANE	6.758	161179	1.174 ug/ml
4) N-TETRADECANE	8.586	154478	1.136 ug/ml
5) N-HEXADECANE	10.194	152524	1.137 ug/ml
6) N-OCTADECANE	11.636	156086	1.156 ug/ml
7) N-EICOSANE	12.944	177367	1.298 ug/mlm
8) N-DOCOSANE	14.143	185490	1.409 ug/mlm
10) N-TETRACOSANE	15.244	194329	1.484 ug/mlm
11) N-HEXACOSANE	16.265	199324	1.532 ug/mlm
12) N-OCTACOSANE	17.213	208196	1.611 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051124\
Data File : FE048138.D
Signal(s) : FID1B.ch
Acq On : 12 May 2024 02:35
Operator : YP\AJ
Sample : P2403-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 14 01:48:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050924.M
Quant Title :
QLast Update : Fri May 10 23:54:11 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

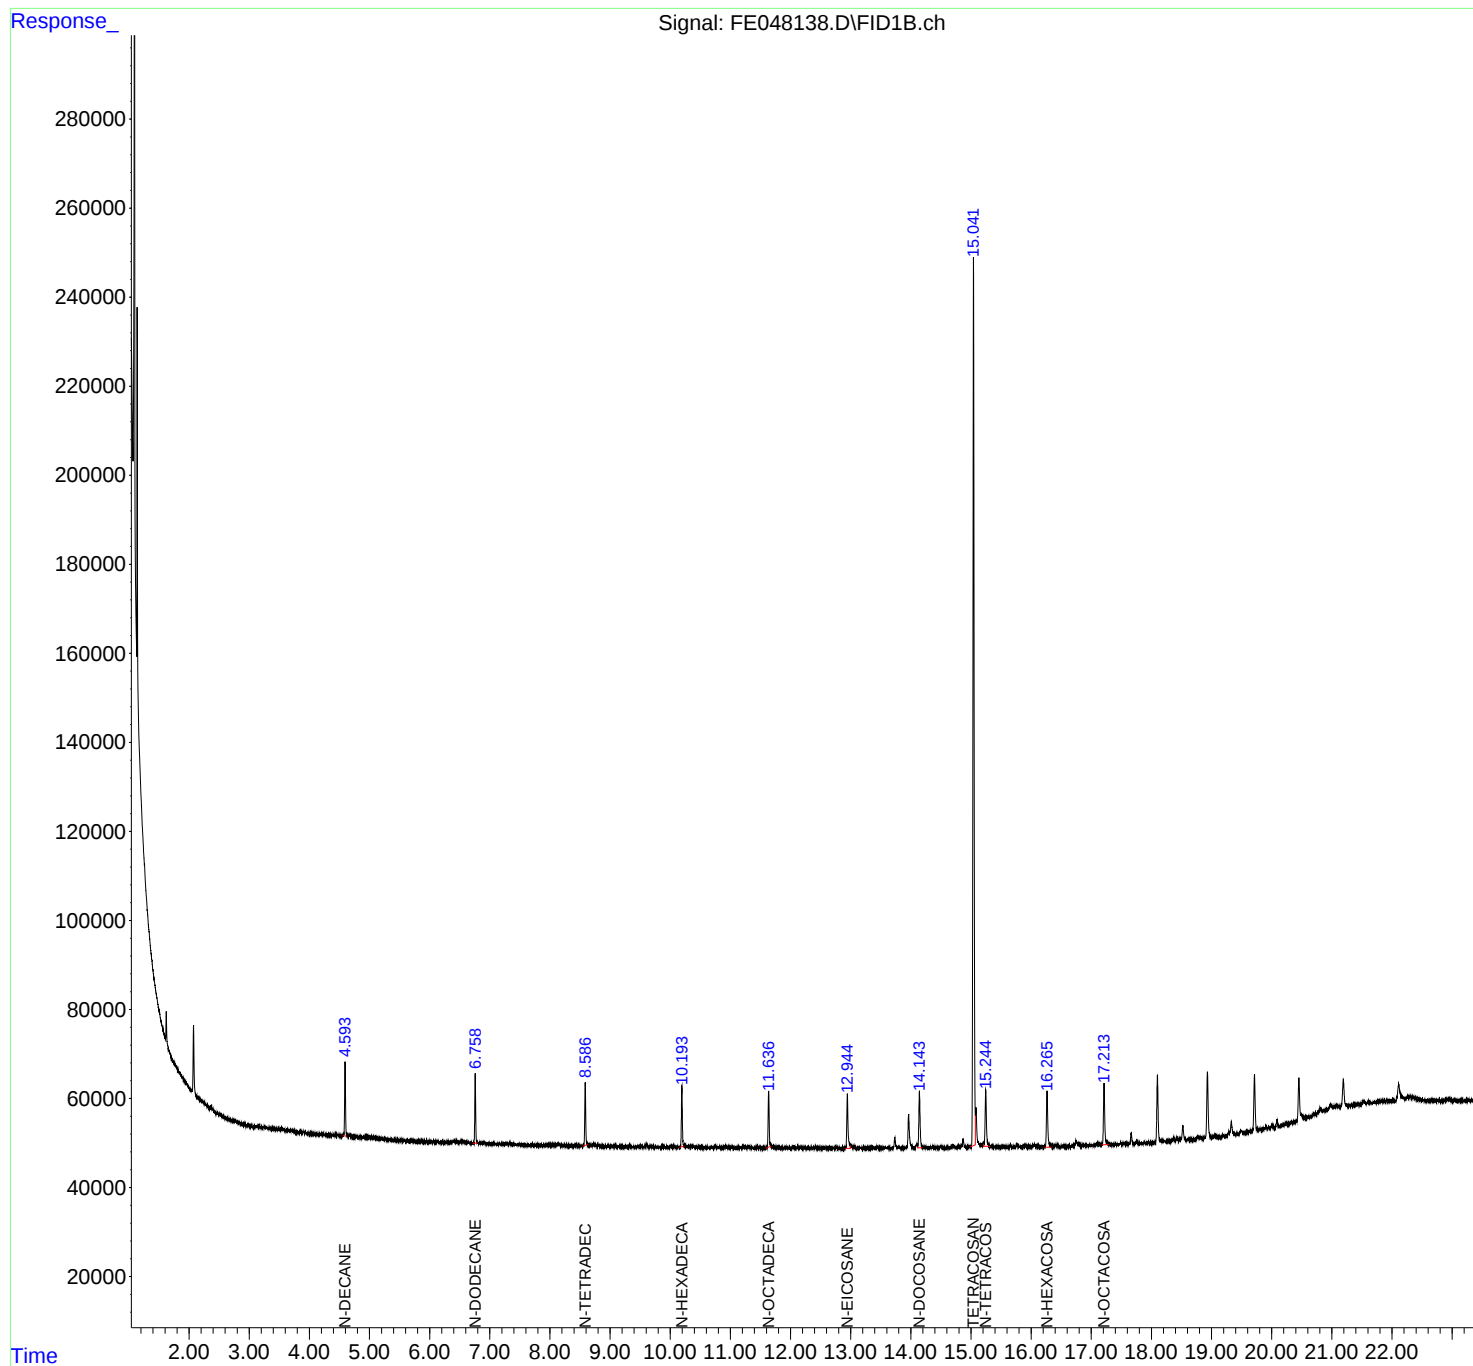

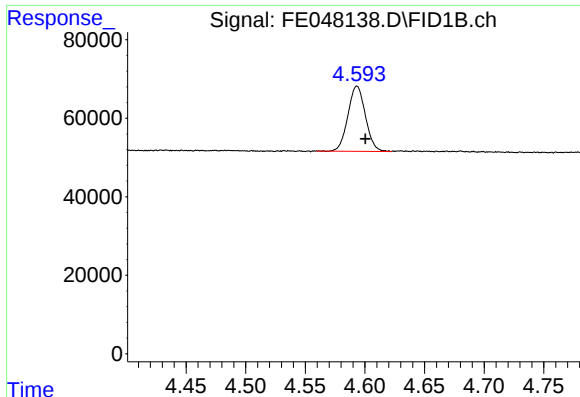


#2 N-DECANE

R.T.: 4.593 min
Delta R.T.: -0.007 min
Response: 169623
Conc: 1.22 ug/ml

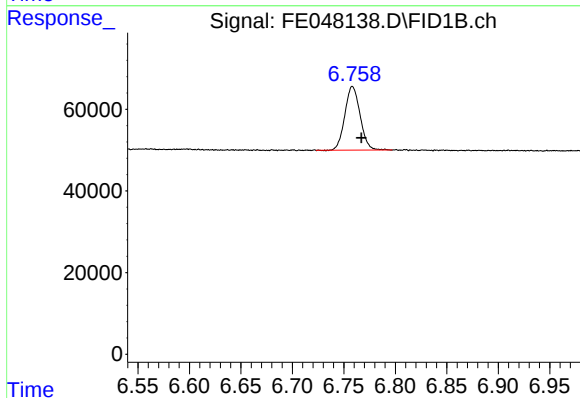


#3 N-DODECANE

R.T.: 6.758 min
Delta R.T.: -0.009 min
Response: 161179
Conc: 1.17 ug/ml

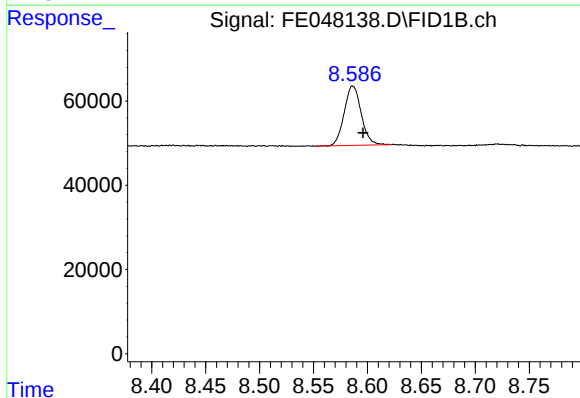


#4 N-TETRADECANE

R.T.: 8.586 min
Delta R.T.: -0.010 min
Response: 154478
Conc: 1.14 ug/ml

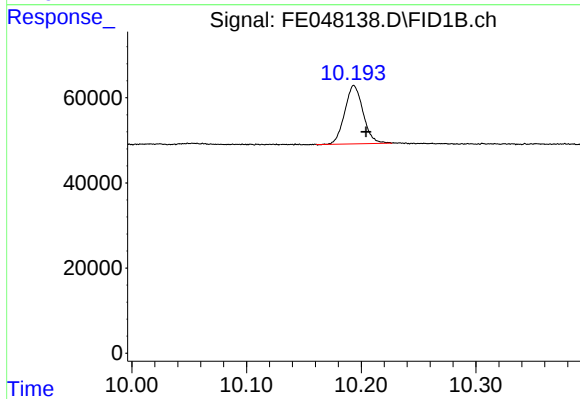


#5 N-HEXADECANE

R.T.: 10.194 min
Delta R.T.: -0.011 min
Response: 152524
Conc: 1.14 ug/ml

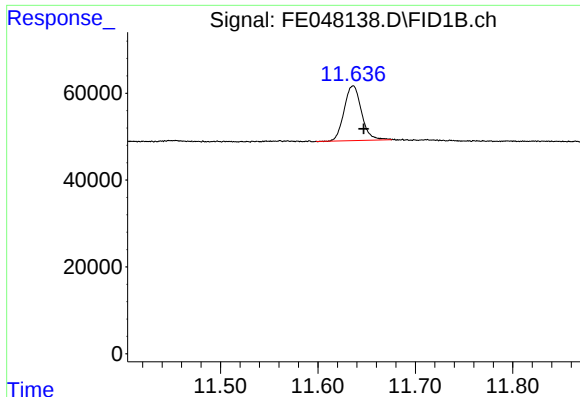


#6 N-OCTADECANE

R.T.: 11.636 min
Delta R.T.: -0.011 min
Response: 156086
Conc: 1.16 ug/ml

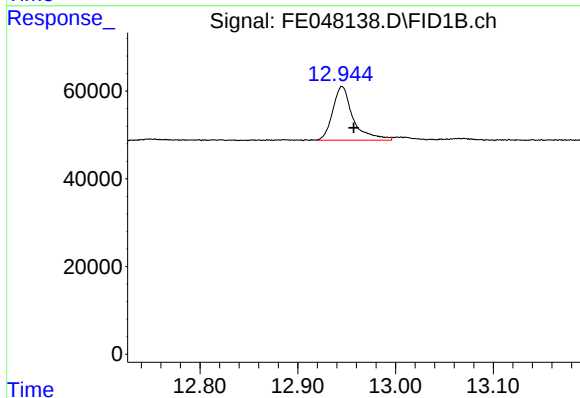


#7 N-EICOSANE

R.T.: 12.944 min
Delta R.T.: -0.013 min
Response: 177367
Conc: 1.30 ug/ml m

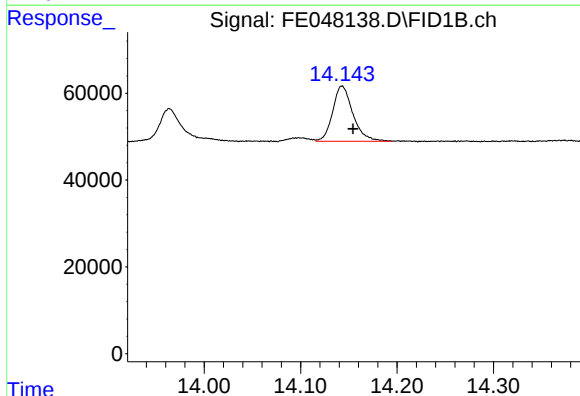


#8 N-DOCOSANE

R.T.: 14.143 min
Delta R.T.: -0.011 min
Response: 185490
Conc: 1.41 ug/ml m

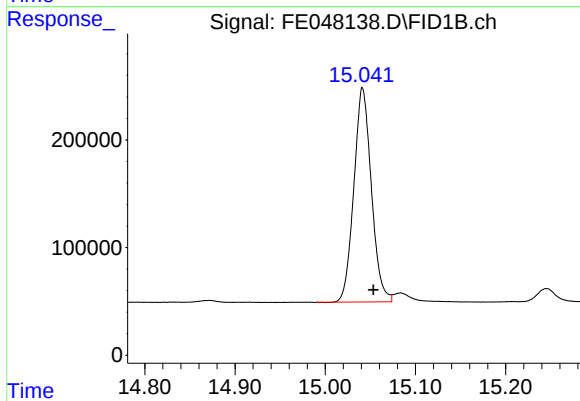


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.041 min
Delta R.T.: -0.012 min
Response: 2686112
Conc: 23.30 ug/ml

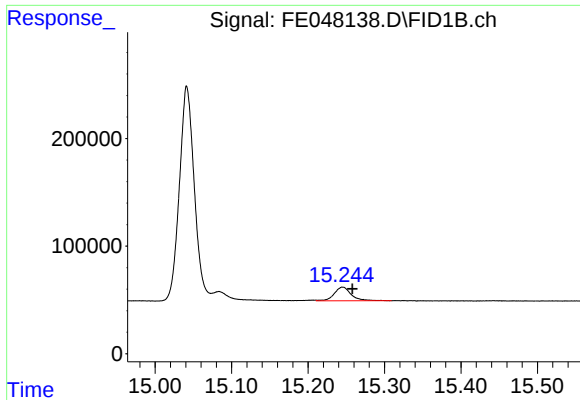


#10 N-TETRACOSANE

R.T.: 15.244 min
Delta R.T.: -0.014 min
Response: 194329
Conc: 1.48 ug/ml m

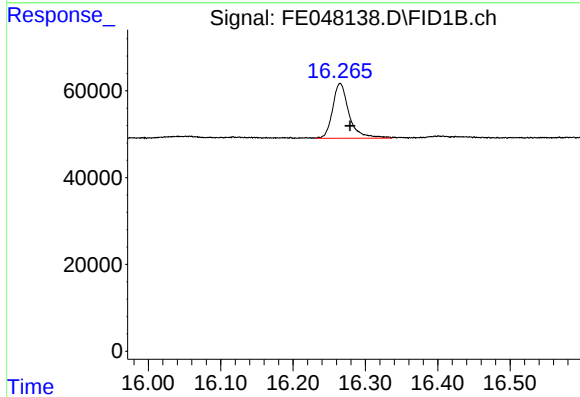

#11 N-HEXACOSANE

R.T.: 16.265 min
Delta R.T.: -0.014 min
Response: 199324
Conc: 1.53 ug/ml m

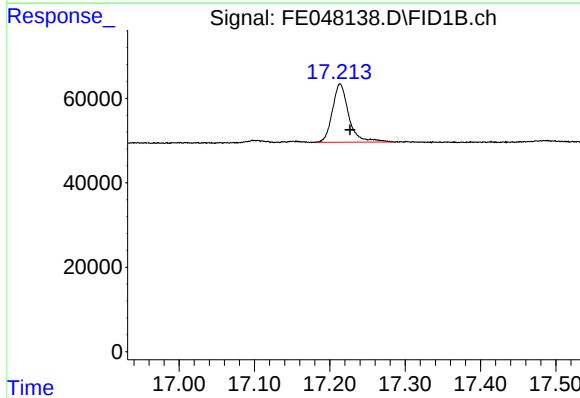

#12 N-OCTACOSANE

R.T.: 17.213 min
Delta R.T.: -0.014 min
Response: 208196
Conc: 1.61 ug/ml m