

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051220\
 Data File : FE031986.D
 Signal(s) : FID1B.CH
 Acq On : 12 May 2020 11:12
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 13 02:15:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050720.M
 Quant Title :
 QLast Update : Thu May 07 13:58:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.365	20361612	52.533 ug/ml
Target Compounds			
2) N-DECANE	4.135	22605872	56.706 ug/ml
3) N-DODECANE	6.136	21990253	54.404 ug/ml
4) N-TETRADECANE	7.926	23976989	57.412 ug/ml
5) N-HEXADECANE	9.523	23578980	55.115 ug/ml
6) N-OCTADECANE	10.963	24332664	54.244 ug/ml
7) N-EICOSANE	12.270	23737019	53.525 ug/ml
8) N-DOCOSANE	13.468	23776449	53.049 ug/ml
10) N-TETRACOSANE	14.572	23821775	53.817 ug/ml
11) N-HEXACOSANE	15.592	22768255	52.039 ug/ml
12) N-OCTACOSANE	16.542	22233047	51.199 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051220\
Data File : FE031986.D
Signal(s) : FID1B.CH
Acq On : 12 May 2020 11:12
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 13 02:15:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050720.M
Quant Title :
QLast Update : Thu May 07 13:58:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

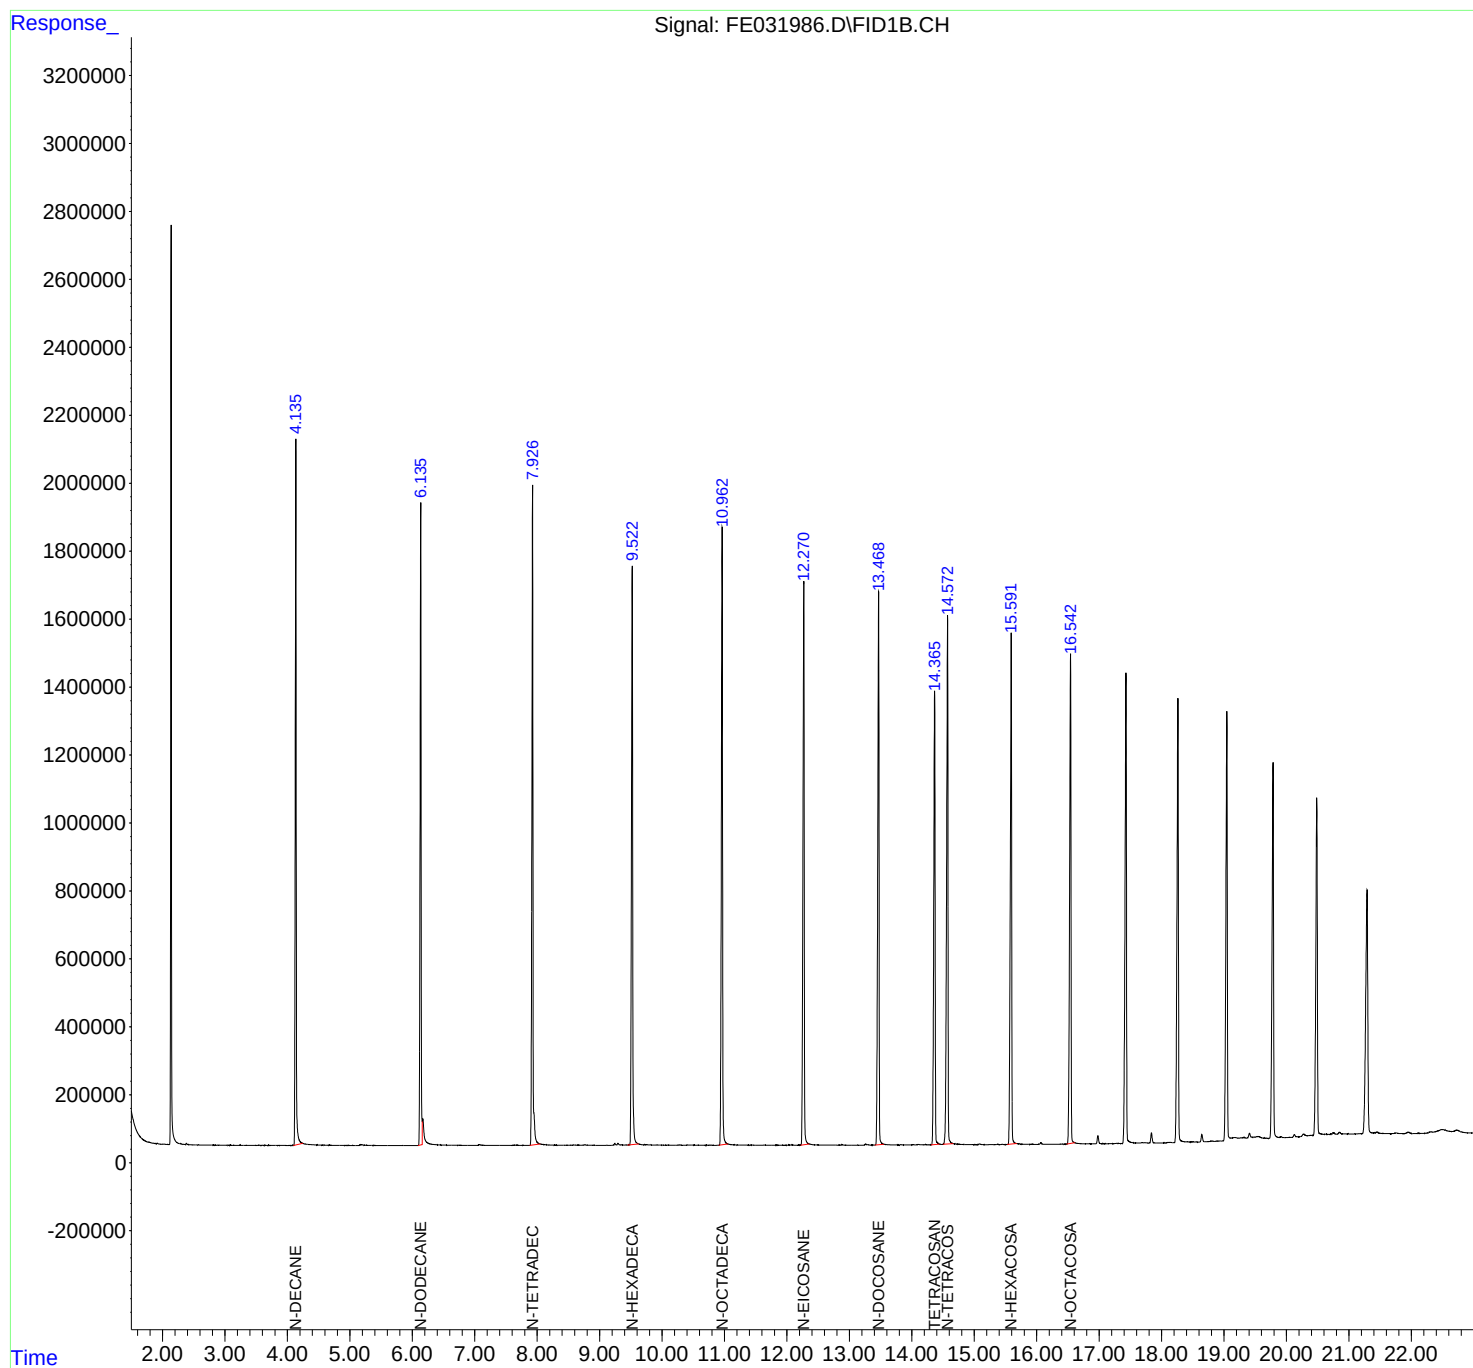

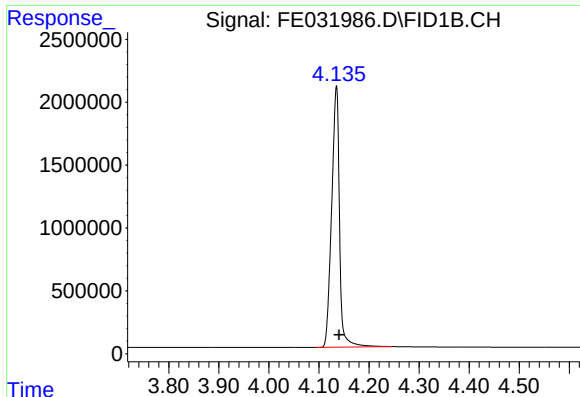


#2 N-DECANE

R.T.: 4.135 min
Delta R.T.: -0.005 min
Response: 22605872
Conc: 56.71 ug/ml

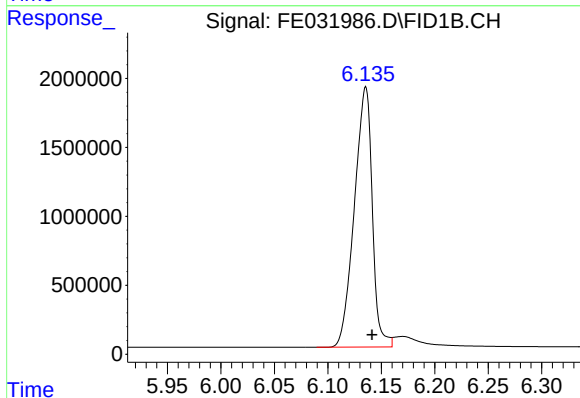


#3 N-DODECANE

R.T.: 6.136 min
Delta R.T.: -0.006 min
Response: 21990253
Conc: 54.40 ug/ml

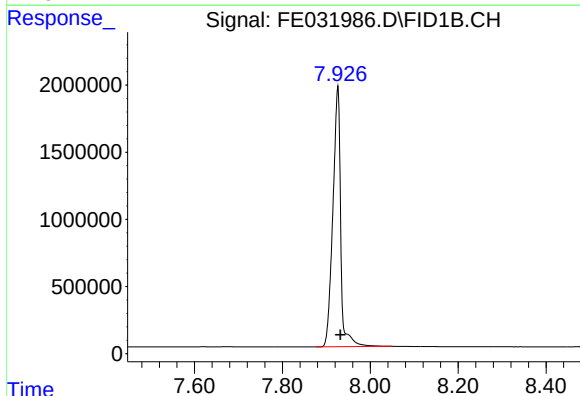


#4 N-TETRADECANE

R.T.: 7.926 min
Delta R.T.: -0.005 min
Response: 23976989
Conc: 57.41 ug/ml

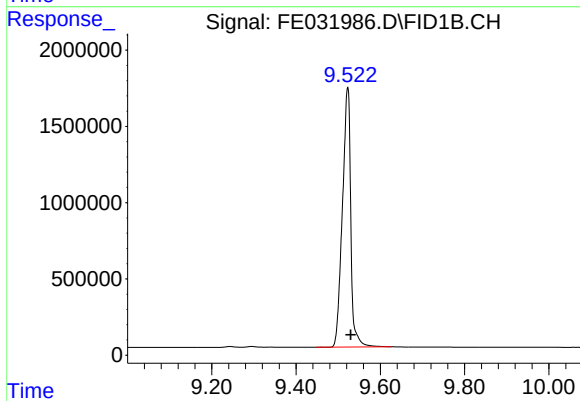


#5 N-HEXADECANE

R.T.: 9.523 min
Delta R.T.: -0.007 min
Response: 23578980
Conc: 55.12 ug/ml

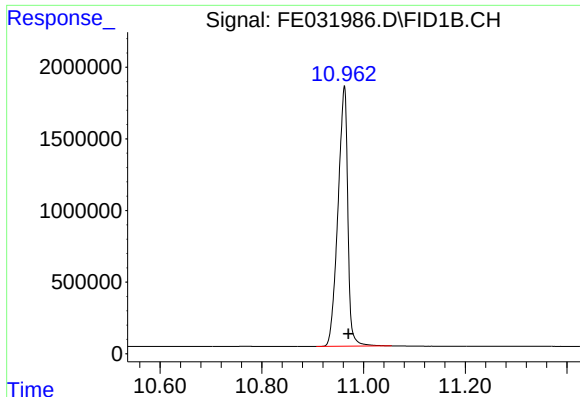


#6 N-OCTADECANE

R.T.: 10.963 min
Delta R.T.: -0.008 min
Response: 24332664
Conc: 54.24 ug/ml

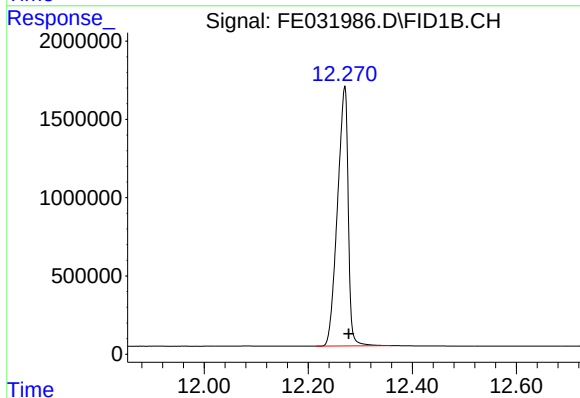


#7 N-EICOSANE

R.T.: 12.270 min
Delta R.T.: -0.007 min
Response: 23737019
Conc: 53.52 ug/ml

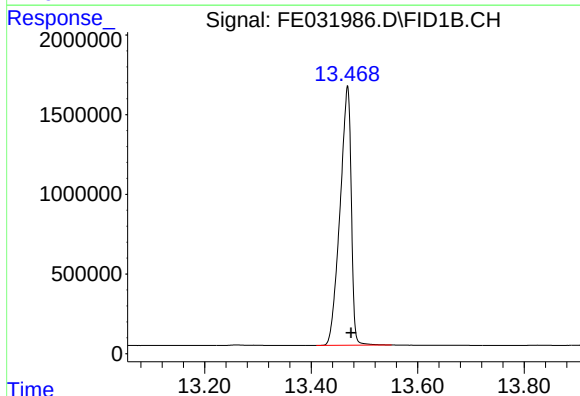


#8 N-DOCOSANE

R.T.: 13.468 min
Delta R.T.: -0.007 min
Response: 23776449
Conc: 53.05 ug/ml

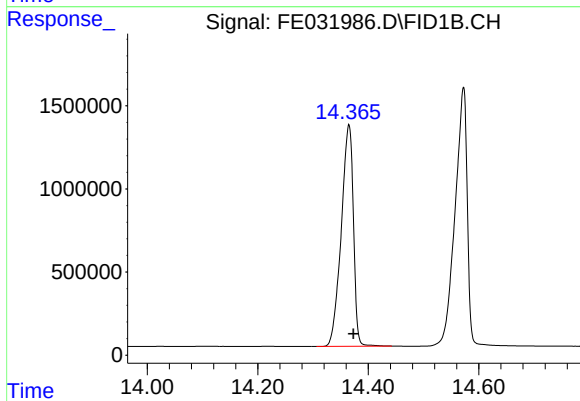


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.365 min
Delta R.T.: -0.008 min
Response: 20361612
Conc: 52.53 ug/ml

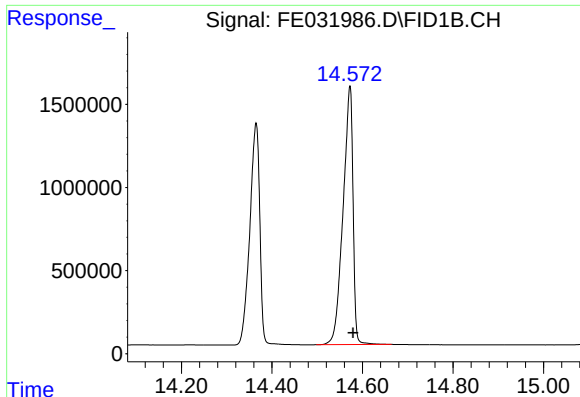


#10 N-TETRACOSANE

R.T.: 14.572 min
Delta R.T.: -0.007 min
Response: 23821775
Conc: 53.82 ug/ml

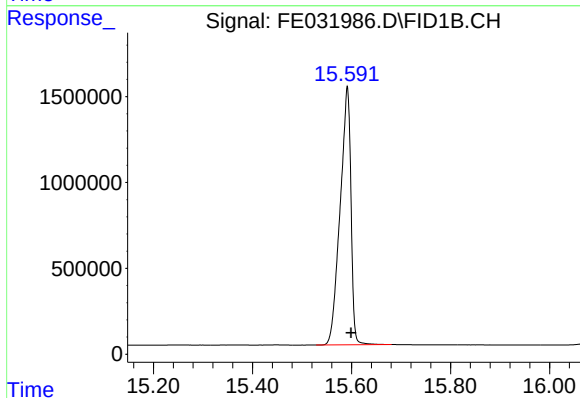

#11 N-HEXACOSANE

R.T.: 15.592 min
Delta R.T.: -0.008 min
Response: 22768255
Conc: 52.04 ug/ml

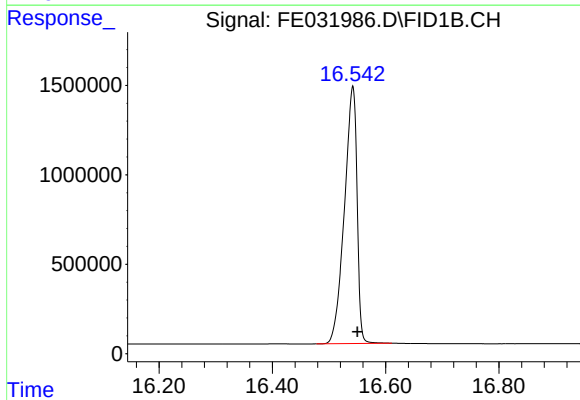

#12 N-OCTACOSANE

R.T.: 16.542 min
Delta R.T.: -0.008 min
Response: 22233047
Conc: 51.20 ug/ml