

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051325AL\
 Data File : FE053782.D
 Signal(s) : FID1B.ch
 Acq On : 13 May 2025 07:28
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 13 11:20:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 041725.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 29 06:49:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.462	118961	0.821 ug/ml
13) T n-Docosane (C22)	14.052	132382	0.917 ug/ml
14) T n-Tetracosane (C24)	15.132f	83248	0.580 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051325AL\
Data File : FE053782.D
Signal(s) : FID1B.ch
Acq On : 13 May 2025 07:28
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 13 11:20:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 041725.M
Quant Title : GC Extractables
QLast Update : Tue Apr 29 06:49:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

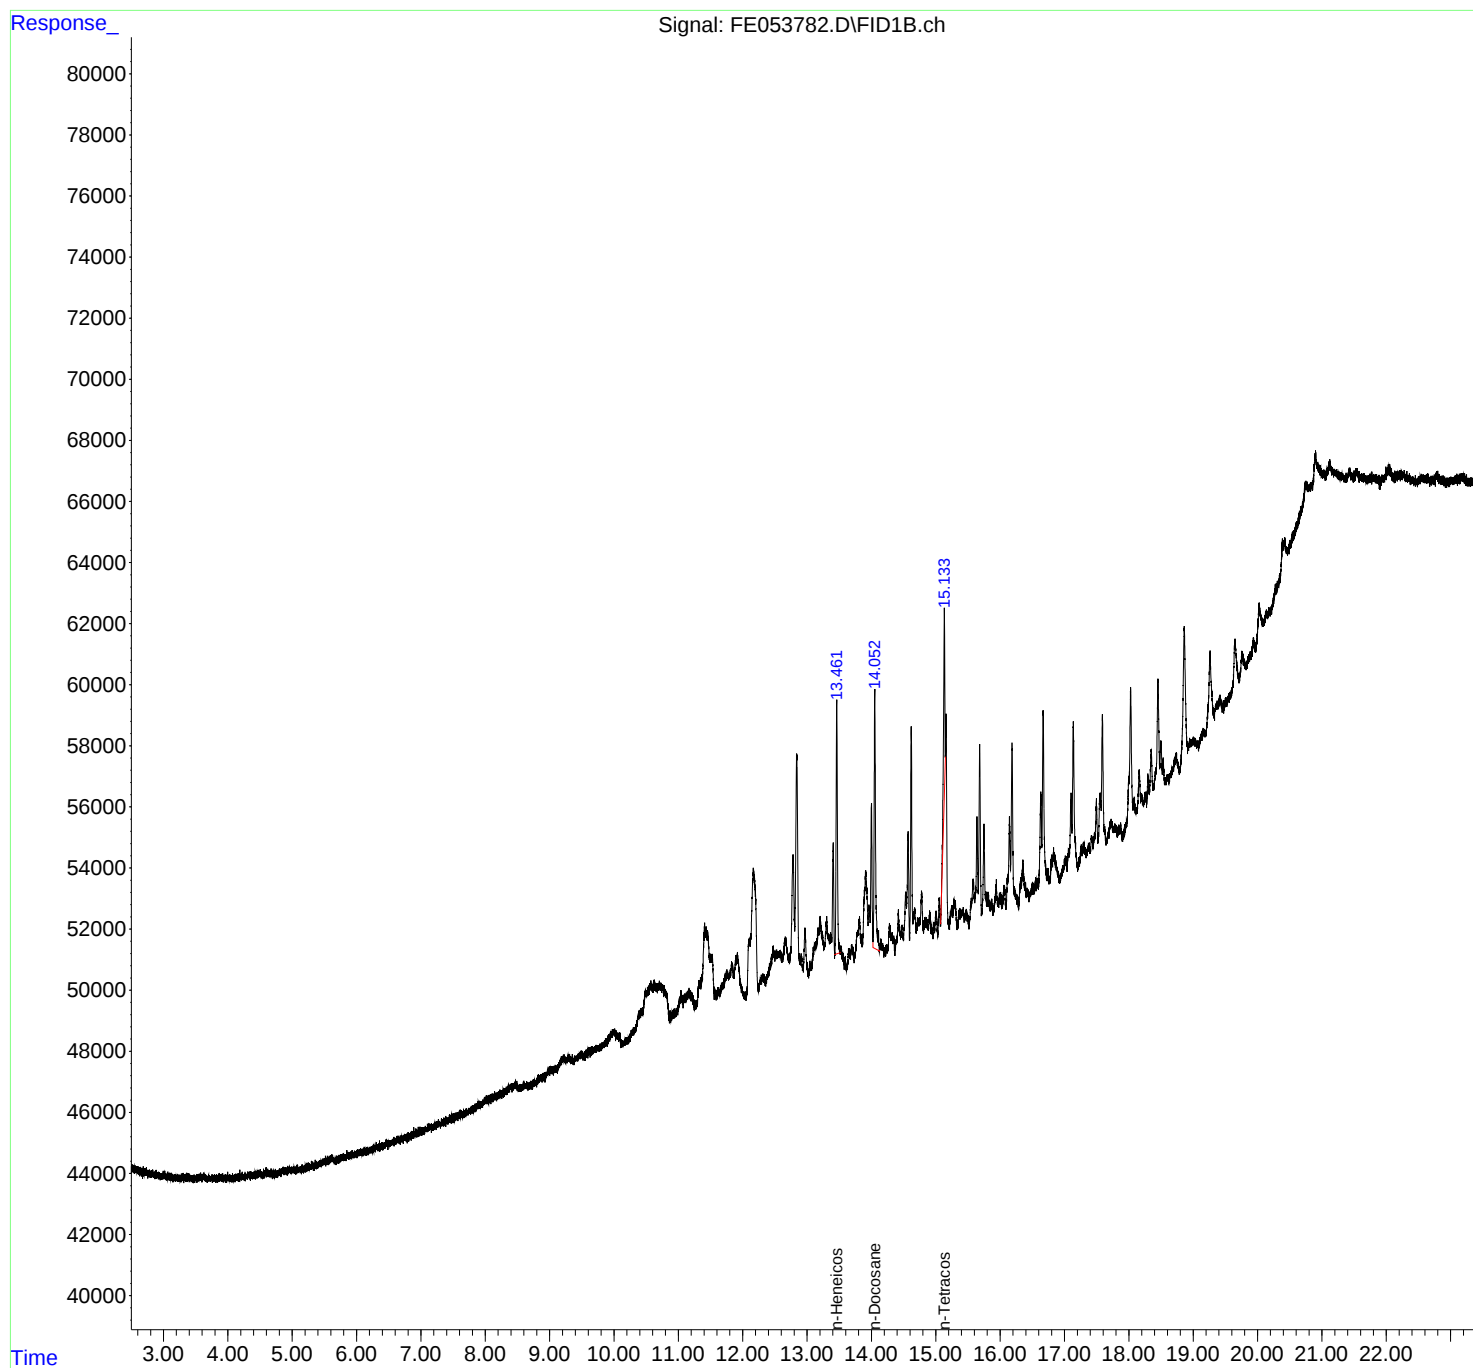


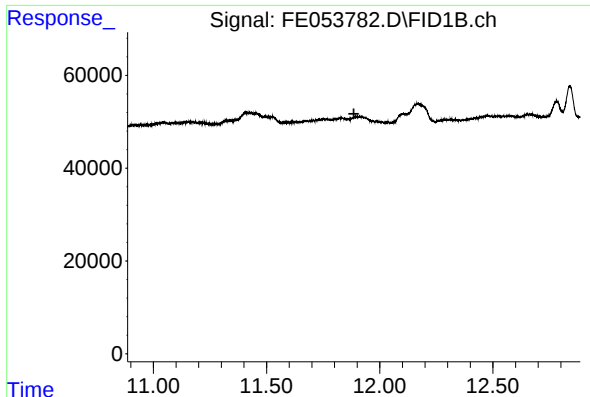

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.886 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

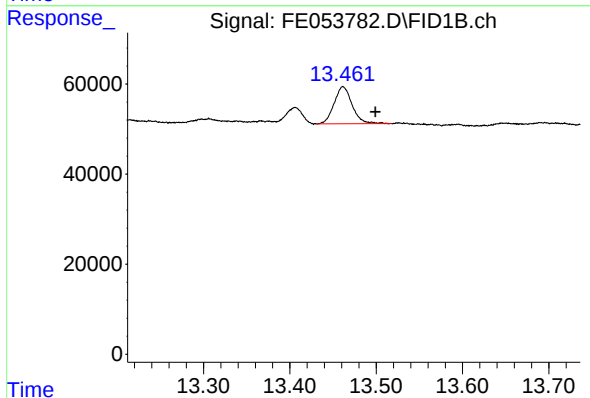


#11 n-Heneicosane (C21)

R.T.: 13.462 min
Delta R.T.: -0.038 min
Response: 118961
Conc: 0.82 ug/ml

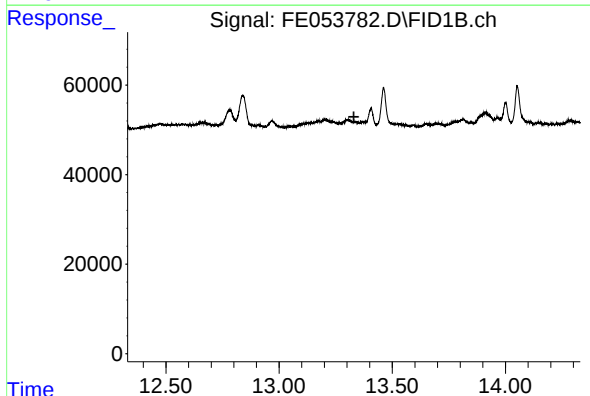


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.330 min
Response: 0
Conc: N.D.

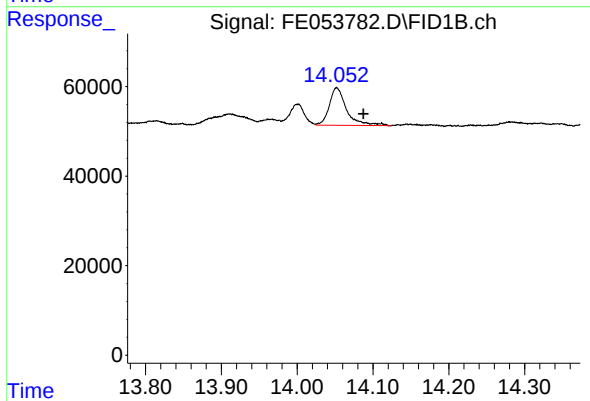

#13 n-Docosane (C22)

R.T.: 14.052 min
Delta R.T.: -0.035 min
Response: 132382
Conc: 0.92 ug/ml

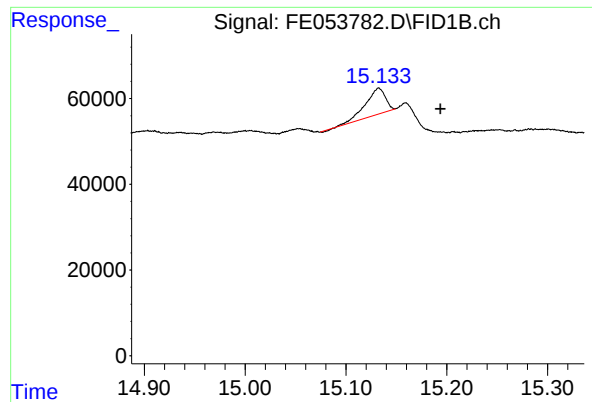

#14 n-Tetracosane (C24)

R.T.: 15.132 min
Delta R.T.: -0.061 min
Response: 83248
Conc: 0.58 ug/ml

Instrument :

FID_E

ClientSampleId :