

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051421\
Data File : FE033798.D
Signal(s) : FID1B.CH
Acq On : 14 May 2021 13:10
Operator : DD\AJ
Sample : PB136384BL
Misc : LOD-WATER-BL
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 14 23:10:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.715	7144819	17.678 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.630	654027	1.469 ug/ml
16)	N-HEXATRIACONTANE	20.185	1695357	4.229 ug/ml
18)	N-TETRACONTANE	21.858	2977121	8.233 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051421\
Data File : FE033798.D
Signal(s) : FID1B.CH
Acq On : 14 May 2021 13:10
Operator : DD\AJ
Sample : PB136384BL
Misc : LOD-WATER-BL
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 14 23:10:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

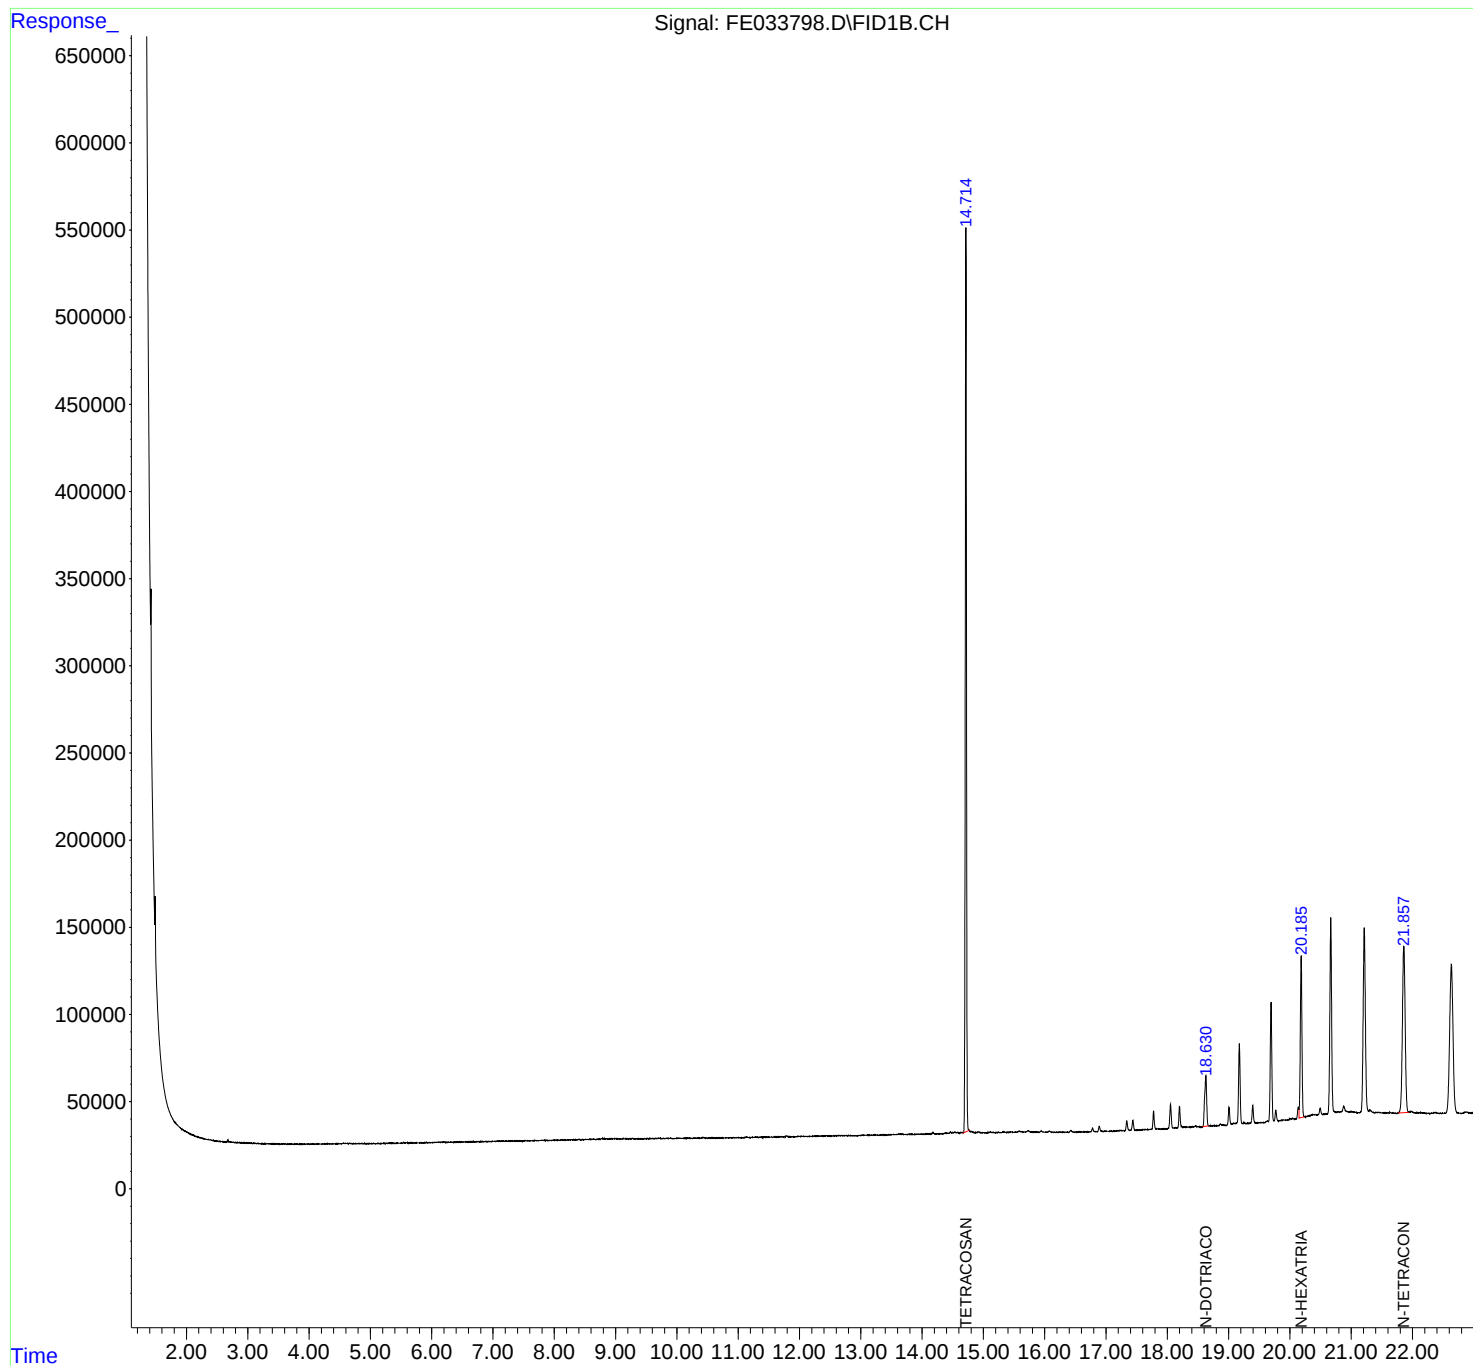

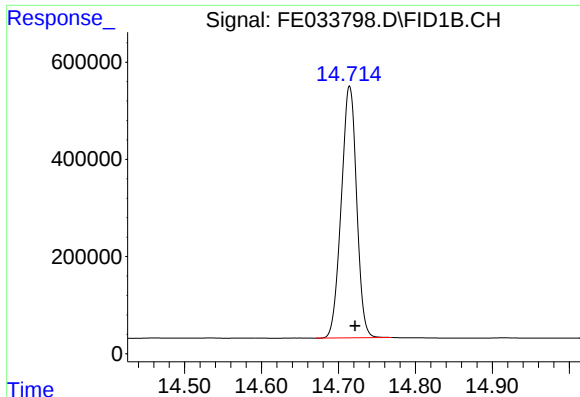


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: -0.007 min
Response: 7144819
Conc: 17.68 ug/ml

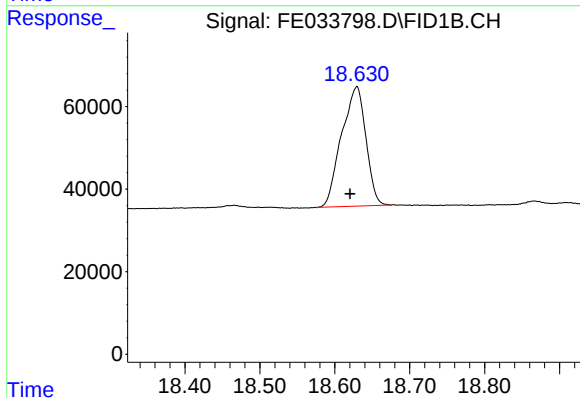


#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.009 min
Response: 654027
Conc: 1.47 ug/ml

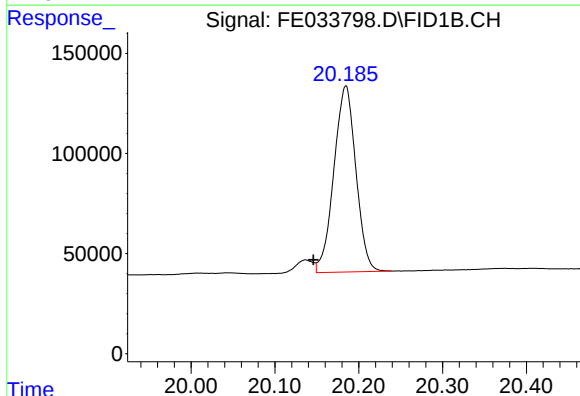

#16 N-HEXATRIACONTANE

R.T.: 20.185 min
Delta R.T.: 0.039 min
Response: 1695357
Conc: 4.23 ug/ml

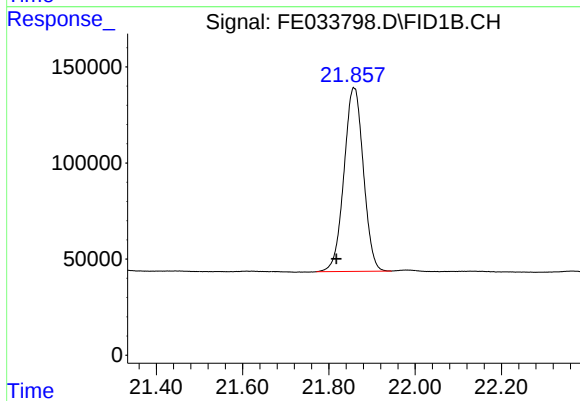

#18 N-TETRACONTANE

R.T.: 21.858 min
Delta R.T.: 0.041 min
Response: 2977121
Conc: 8.23 ug/ml