

Data Path : P:\HPCHEM1\FID E\Data\FE051618\
 Data File : FE027292.D
 Signal(s) : FID1B.CH
 Acq On : 17 May 2018 4:51
 Operator : UA/AJ
 Sample : J2925-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 17 08:05:28 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.281	2540993	17.256 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.860f	1595241	8.441 ug/ml
7)	N-EICOSANE	13.167	322492	1.693 ug/ml
8)	N-DOCOSANE	14.375	220978	1.239 ug/ml
10)	N-TETRACOSANE	15.499	1739672	10.329 ug/ml
11)	N-HEXACOSANE	16.514	191973	1.162 ug/ml
12)	N-OCTACOSANE	17.480	2298364	13.908 ug/ml
13)	N-TRIACONTANE	18.374	1096275	6.516 ug/ml
14)	N-DOTRIACONTANE	19.208	1853272	10.787 ug/ml
15)	N-TETRATRIACONTANE	20.001	909148	5.073 ug/ml
16)	N-HEXATRIACONTANE	20.767	1484198	8.435 ug/ml
17)	N-OCTATRIACONTANE	21.678	753767	4.589 ug/ml
18)	N-TETRACONTANE	22.840	720044	4.336 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE051618\
Data File : FE027292.D
Signal(s) : FID1B.CH
Acq On : 17 May 2018 4:51
Operator : UA/AJ
Sample : J2925-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 17 08:05:28 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

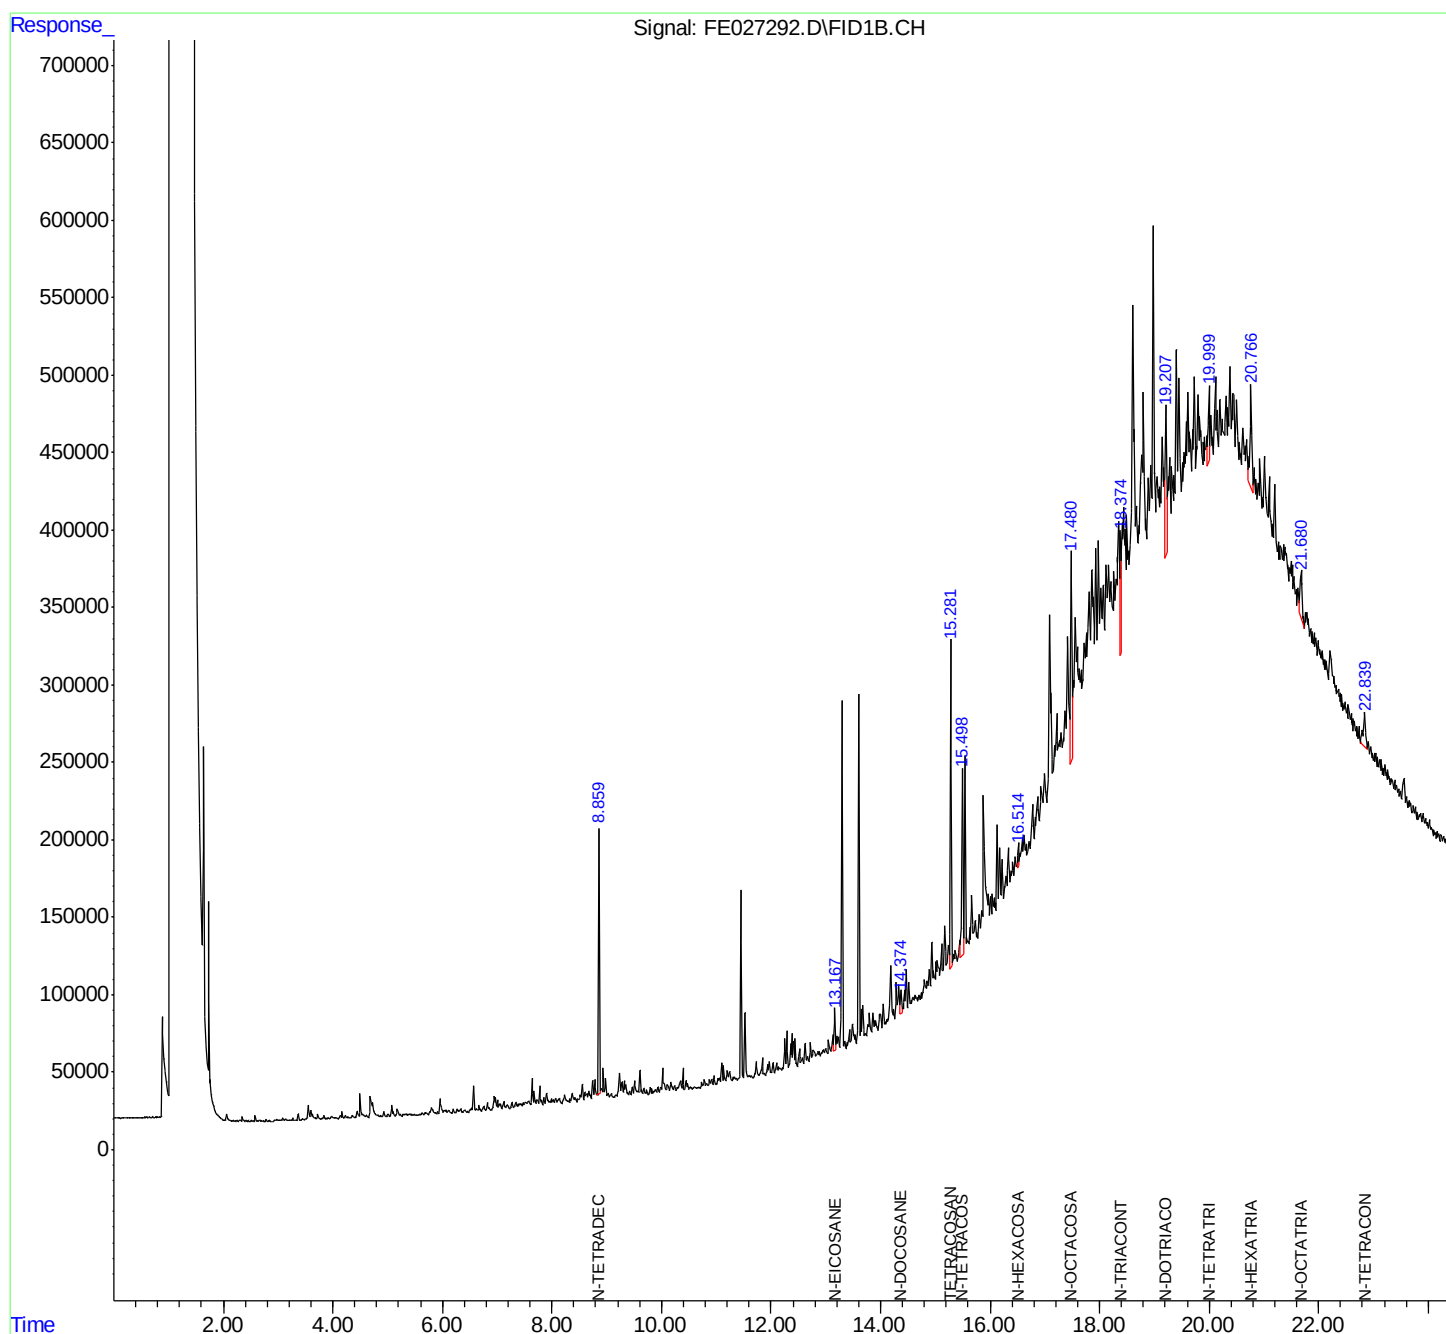


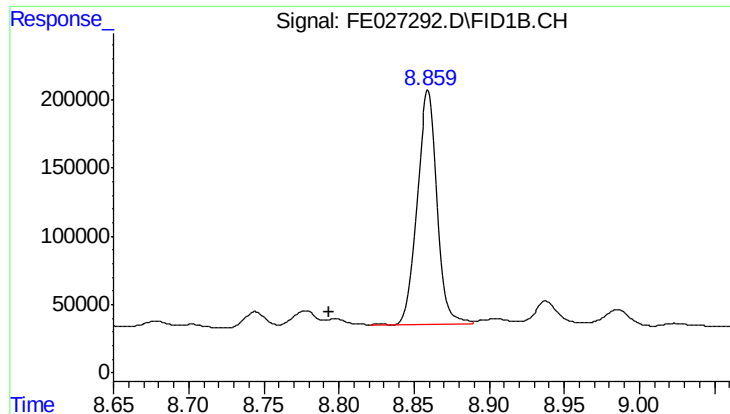

#4 N-TETRADECANE


R.T.: 8.860 min
Delta R.T.: 0.066 min
Response: 1595241
Conc: 8.44 ug/ml

Instrument :
FID_E
ClientSampleId :

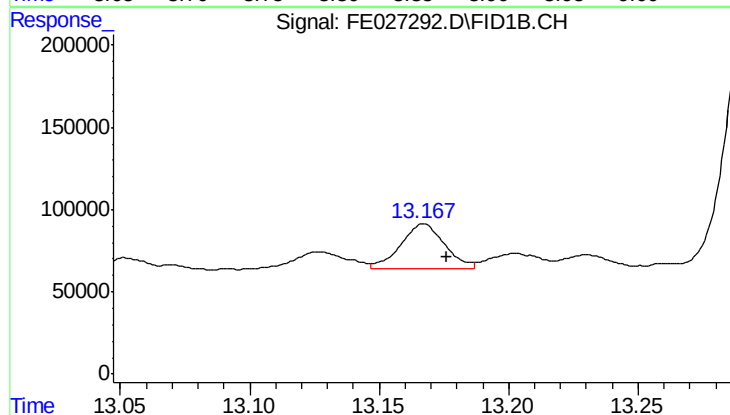


#7 N-EICOSANE

R.T.: 13.167 min
Delta R.T.: -0.009 min
Response: 322492
Conc: 1.69 ug/ml

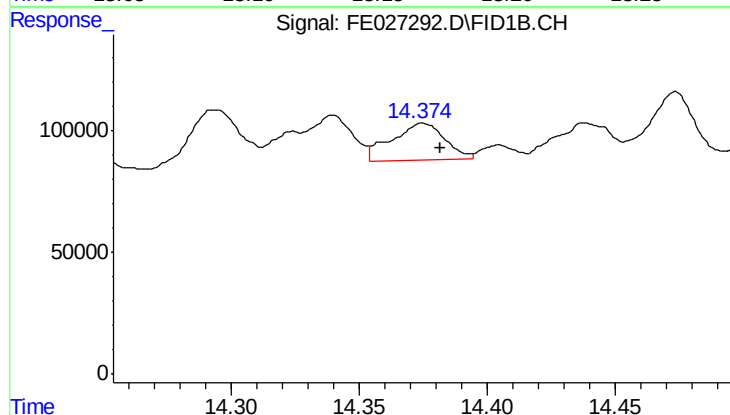


#8 N-DOCOSANE

R.T.: 14.375 min
Delta R.T.: -0.007 min
Response: 220978
Conc: 1.24 ug/ml

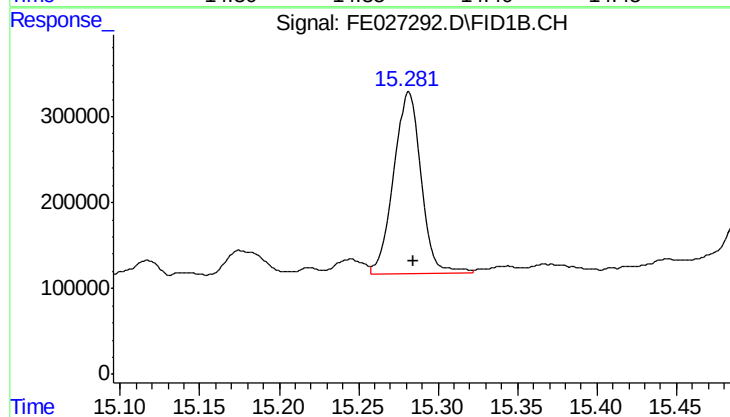

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.281 min
Delta R.T.: -0.003 min
Response: 2540993
Conc: 17.26 ug/ml

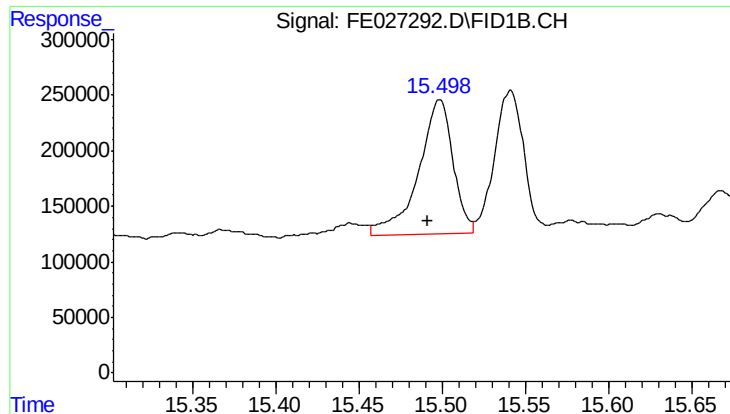

#10 N-TETRACOSANE


R.T.: 15.499 min
Delta R.T.: 0.008 min
Response: 1739672
Conc: 10.33 ug/ml

Instrument :
FID_E
ClientSampleId :

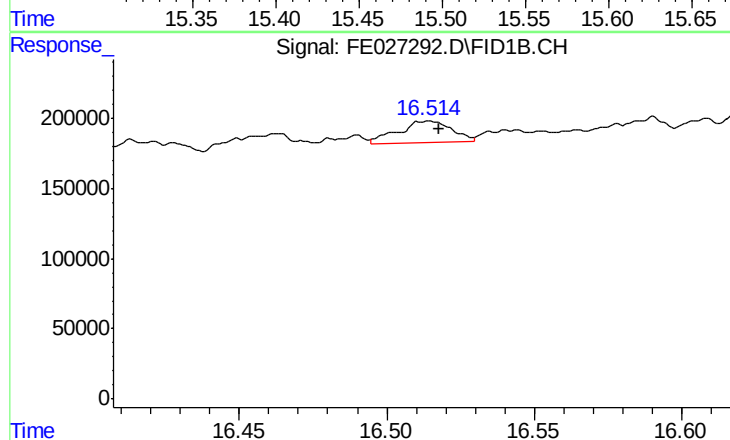


#11 N-HEXACOSANE

R.T.: 16.514 min
Delta R.T.: -0.004 min
Response: 191973
Conc: 1.16 ug/ml

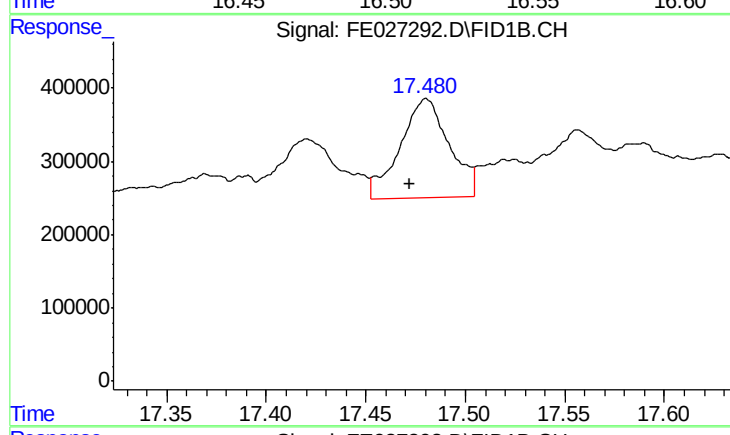


#12 N-OCTACOSANE

R.T.: 17.480 min
Delta R.T.: 0.008 min
Response: 2298364
Conc: 13.91 ug/ml

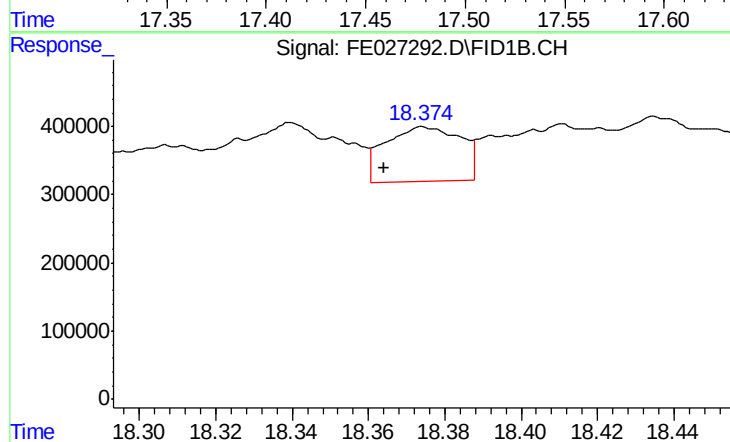

#13 N-TRIACONTANE


R.T.: 18.374 min
Delta R.T.: 0.010 min
Response: 1096275
Conc: 6.52 ug/ml

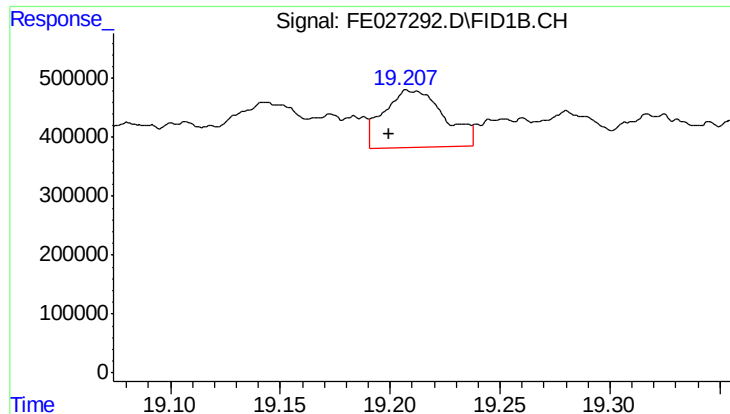

#14 N-DOTRIACONTANE


R.T.: 19.208 min
Delta R.T.: 0.008 min
Response: 1853272
Conc: 10.79 ug/ml

Instrument :
FID_E
ClientSampleId :

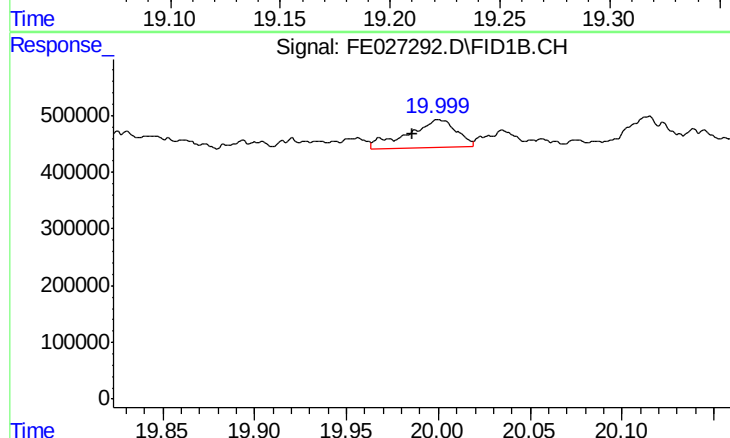


#15 N-TETRATRIACONTANE

R.T.: 20.001 min
Delta R.T.: 0.015 min
Response: 909148
Conc: 5.07 ug/ml

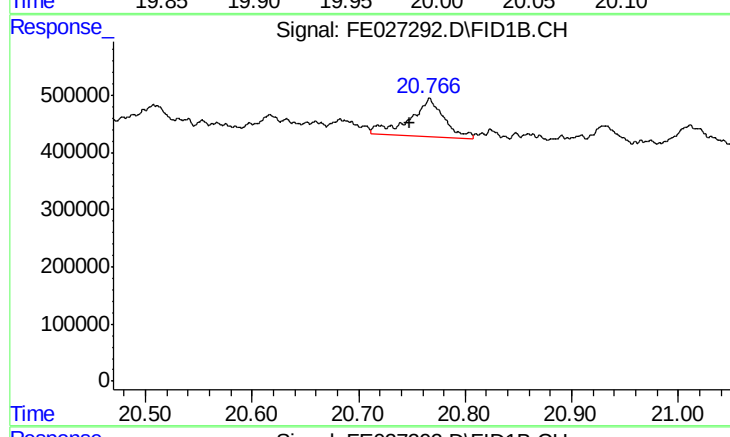


#16 N-HEXATRIACONTANE

R.T.: 20.767 min
Delta R.T.: 0.019 min
Response: 1484198
Conc: 8.43 ug/ml

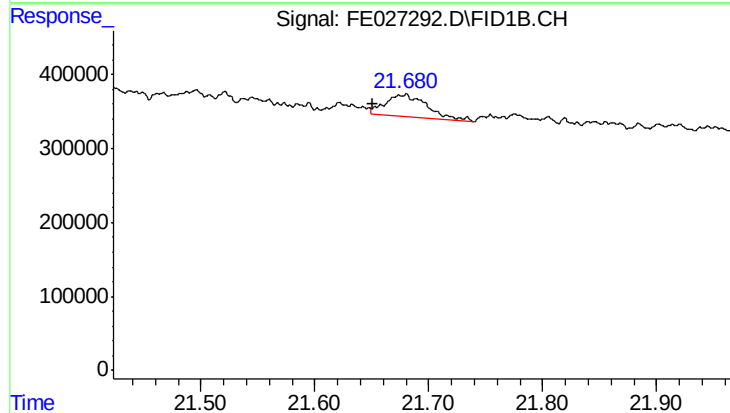

#17 N-OCTATRIACONTANE

R.T.: 21.678 min
Delta R.T.: 0.027 min
Response: 753767
Conc: 4.59 ug/ml

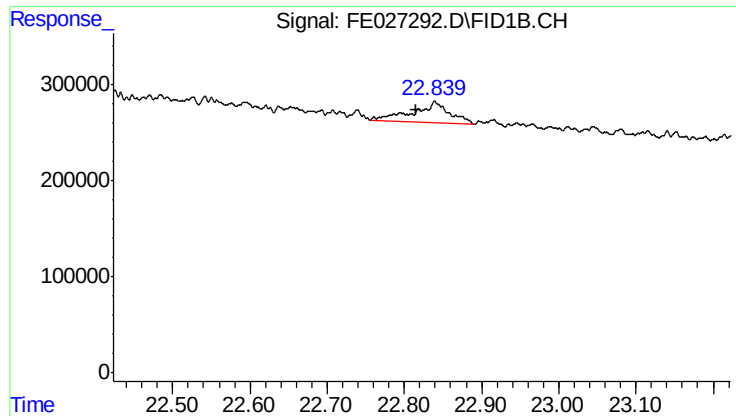

#18 N-TETRACONTANE

R.T.: 22.840 min
Delta R.T.: 0.026 min
Response: 720044
Conc: 4.34 ug/ml

Instrument :
FID_E
ClientSampleId :