

Data Path : P:\HPCHEM1\FID_E\Data\FE051618\
 Data File : FE027283.D
 Signal(s) : FID1B.CH
 Acq On : 16 May 2018 23:47
 Operator : UA/AJ
 Sample : J2933-01MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 EPE-F-7A(105-107)MS

Integration File: autoint1.e
 Quant Time: May 17 02:19:05 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.277	3277953	22.261 ug/ml
Target Compounds			
2) N-DECANE	4.930	2769943	17.005 ug/ml
3) N-DODECANE	6.973	3233232	18.599 ug/ml
4) N-TETRADECANE	8.785	3646515	19.294 ug/ml
5) N-HEXADECANE	10.397	4046940	20.584 ug/ml
6) N-OCTADECANE	11.849	4088206	20.359 ug/ml
7) N-EICOSANE	13.168	3968843	20.841 ug/ml
8) N-DOCOSANE	14.374	3875705	21.727 ug/ml
10) N-TETRACOSANE	15.484	3752349	22.280 ug/ml
11) N-HEXACOSANE	16.510	3625213	21.946 ug/ml
12) N-OCTACOSANE	17.465	3684615	22.297 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051618\
Data File : FE027283.D
Signal(s) : FID1B.CH
Acq On : 16 May 2018 23:47
Operator : UA/AJ
Sample : J2933-01MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
EPE-F-7A(105-107)MS

Integration File: autoint1.e
Quant Time: May 17 02:19:05 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

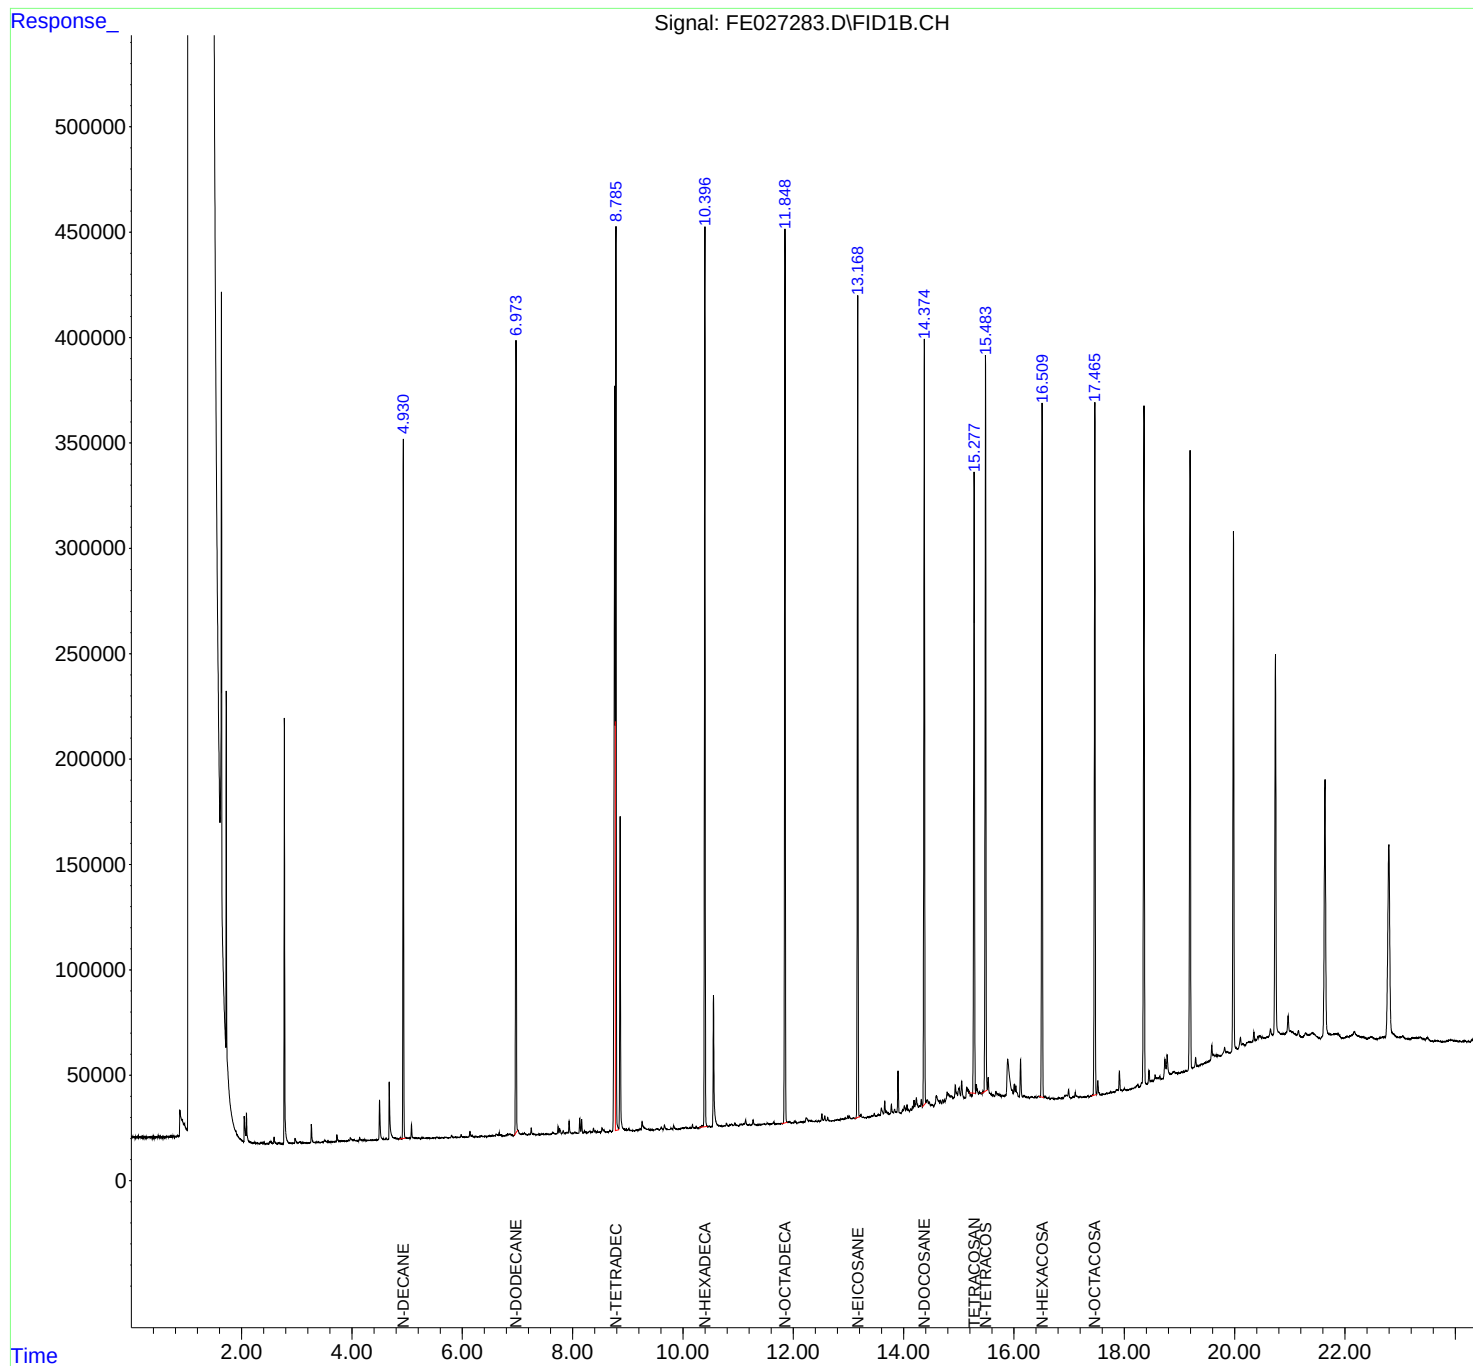


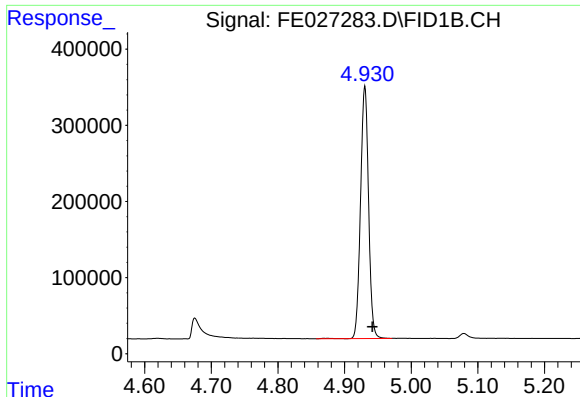

#2 N-DECANE


R.T.: 4.930 min
Delta R.T.: -0.011 min
Response: 2769943
Conc: 17.00 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-7A(105-107)MS

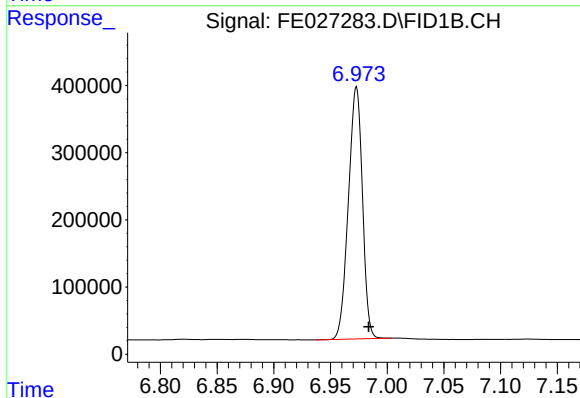


#3 N-DODECANE

R.T.: 6.973 min
Delta R.T.: -0.011 min
Response: 3233232
Conc: 18.60 ug/ml

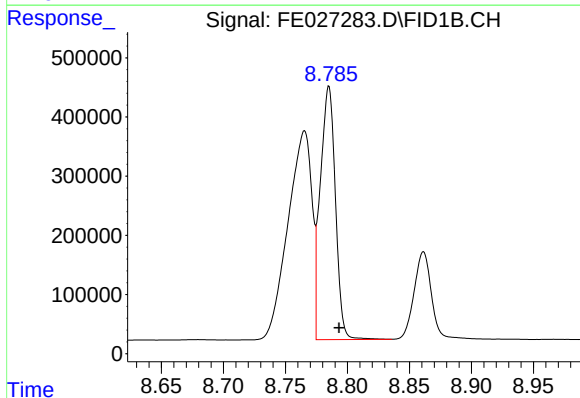


#4 N-TETRADECANE

R.T.: 8.785 min
Delta R.T.: -0.008 min
Response: 3646515
Conc: 19.29 ug/ml

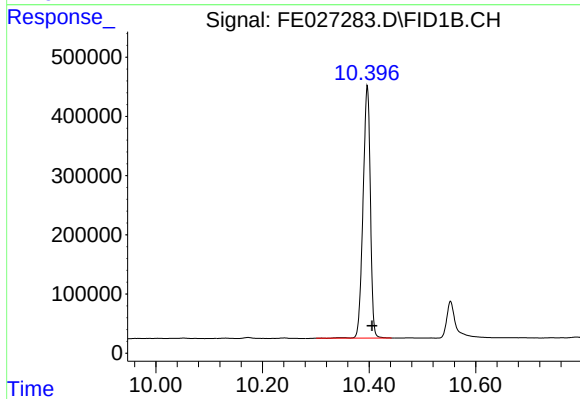

#5 N-HEXADECANE


R.T.: 10.397 min
Delta R.T.: -0.009 min
Response: 4046940
Conc: 20.58 ug/ml

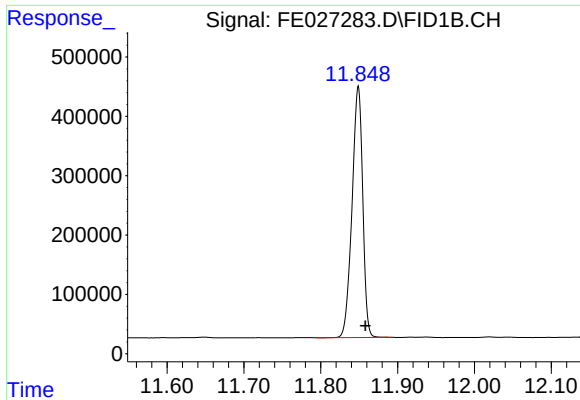

#6 N-OCTADECANE


R.T.: 11.849 min
Delta R.T.: -0.009 min
Response: 4088206
Conc: 20.36 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-7A(105-107)MS

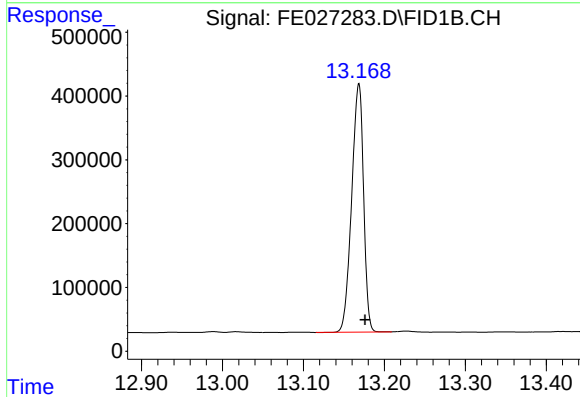


#7 N-EICOSANE

R.T.: 13.168 min
Delta R.T.: -0.008 min
Response: 3968843
Conc: 20.84 ug/ml

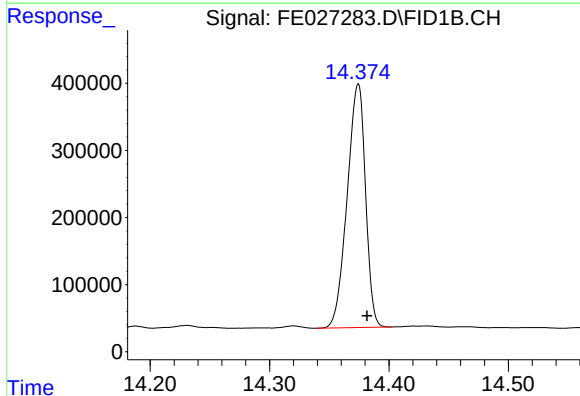


#8 N-DOCOSANE

R.T.: 14.374 min
Delta R.T.: -0.007 min
Response: 3875705
Conc: 21.73 ug/ml

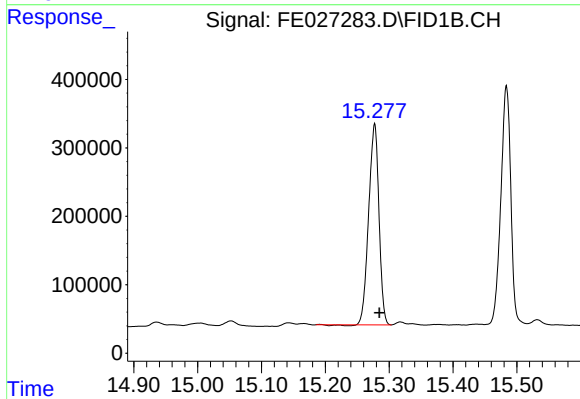

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.277 min
Delta R.T.: -0.007 min
Response: 3277953
Conc: 22.26 ug/ml

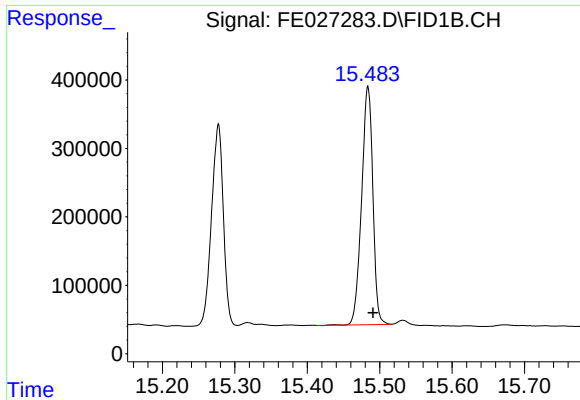

#10 N-TETRACOSANE


R.T.: 15.484 min
Delta R.T.: -0.007 min
Response: 3752349
Conc: 22.28 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-7A(105-107)MS

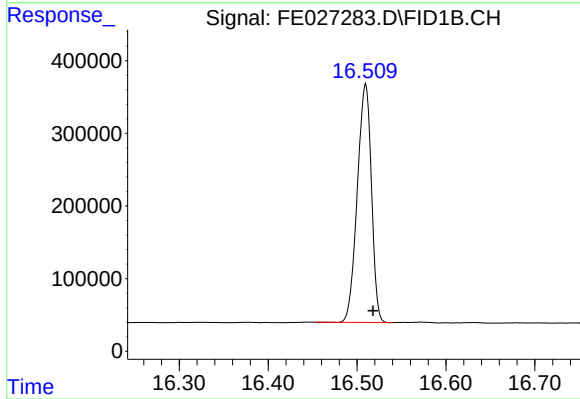

#11 N-HEXACOSANE

R.T.: 16.510 min
Delta R.T.: -0.008 min
Response: 3625213
Conc: 21.95 ug/ml

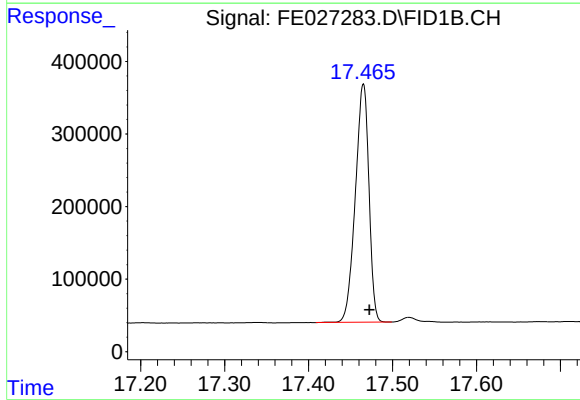

#12 N-OCTACOSANE

R.T.: 17.465 min
Delta R.T.: -0.007 min
Response: 3684615
Conc: 22.30 ug/ml