

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051622\
 Data File : FE035682.D
 Signal(s) : FID1B.CH
 Acq On : 16 May 2022 12:06
 Operator : YP\AJ
 Sample : N2806-01 25X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 16 20:15:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
 Quant Title :
 QLast Update : Fri May 13 15:02:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.035	98402	0.876 ug/ml
Target Compounds			
2) N-DECANE	3.788	51851	0.408 ug/ml
3) N-DODECANE	5.745f	147193	1.151 ug/ml
4) N-TETRADECANE	7.649	90394	0.700 ug/ml
5) N-HEXADECANE	9.156	127953	0.990 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051622\
Data File : FE035682.D
Signal(s) : FID1B.CH
Acq On : 16 May 2022 12:06
Operator : YP\AJ
Sample : N2806-01 25X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 16 20:15:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
Quant Title :
QLast Update : Fri May 13 15:02:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

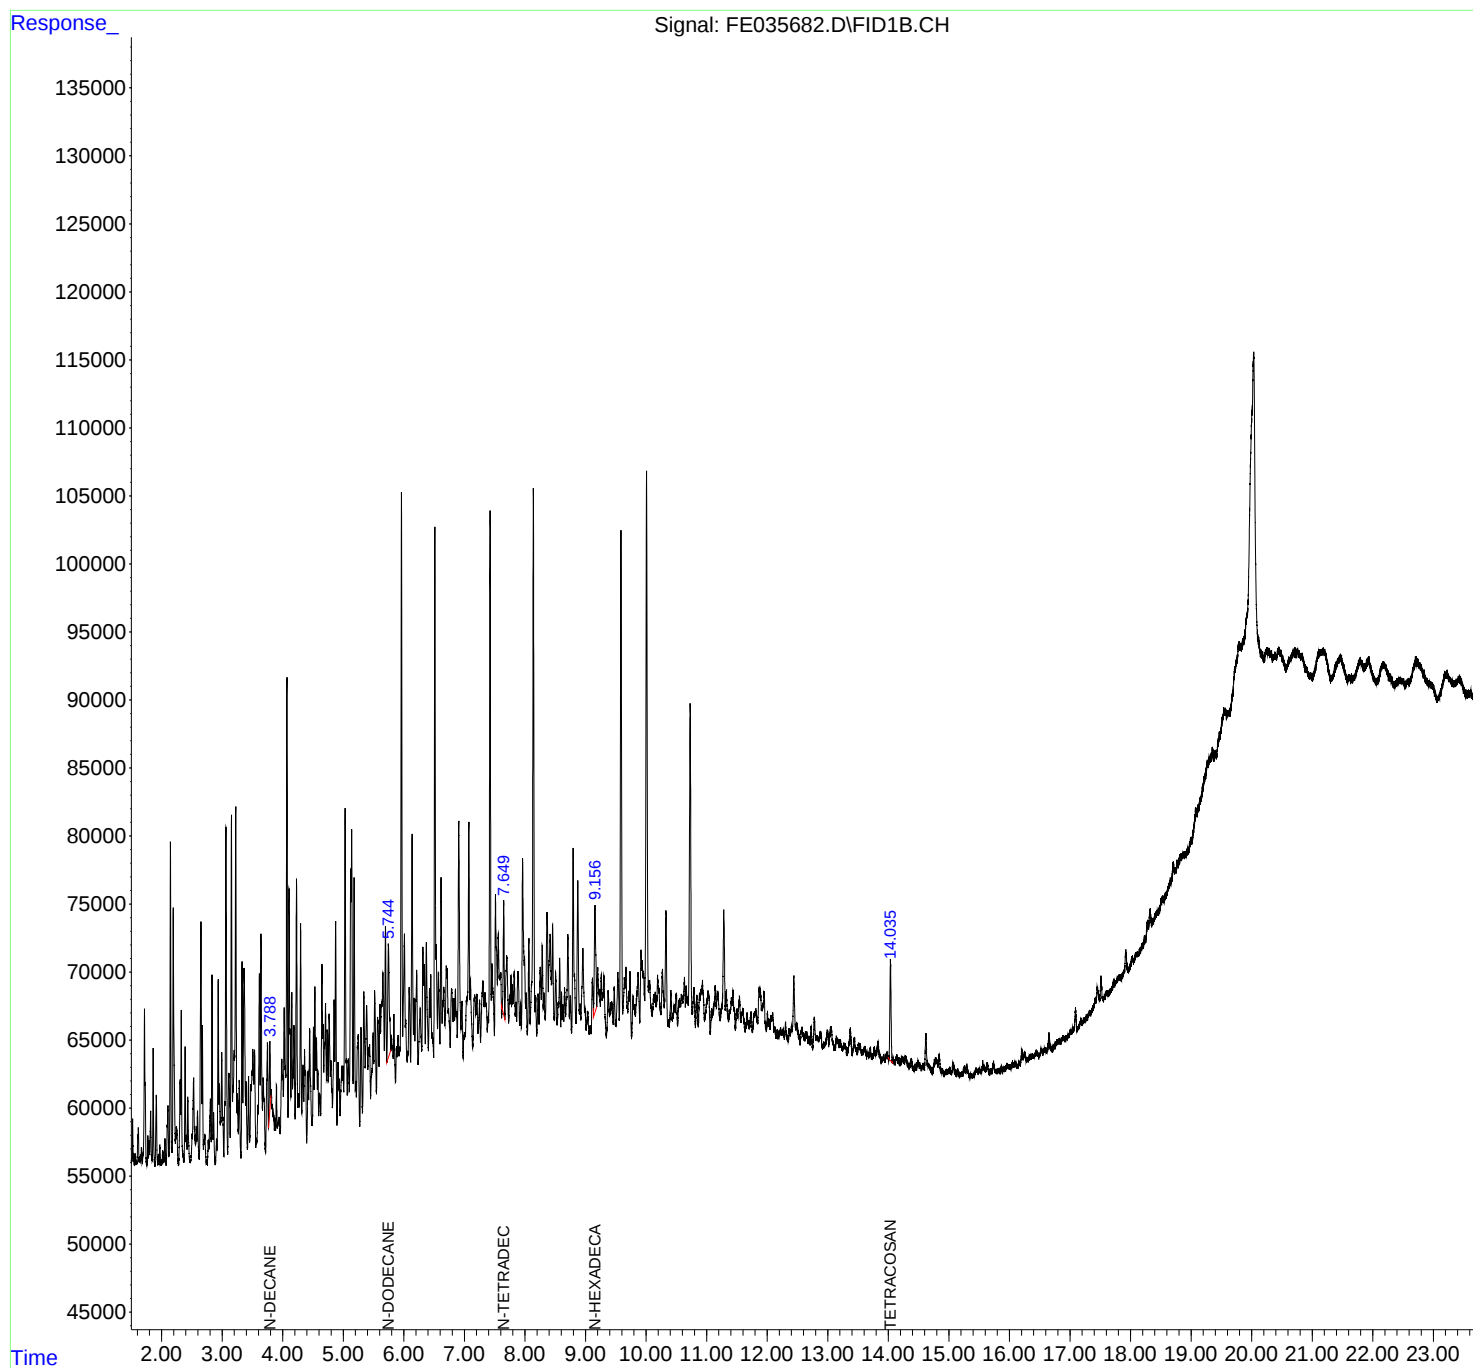


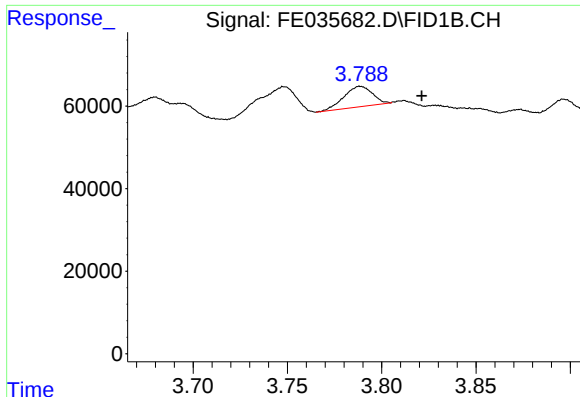

#2 N-DECANE


R.T.: 3.788 min
Delta R.T.: -0.033 min
Response: 51851
Conc: 0.41 ug/ml

Instrument :
FID_E
ClientSampleId :

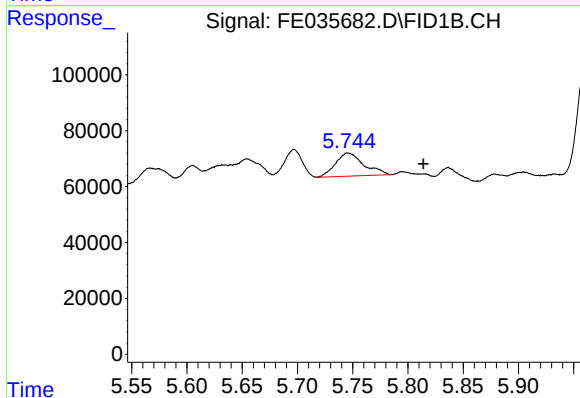


#3 N-DODECANE

R.T.: 5.745 min
Delta R.T.: -0.069 min
Response: 147193
Conc: 1.15 ug/ml

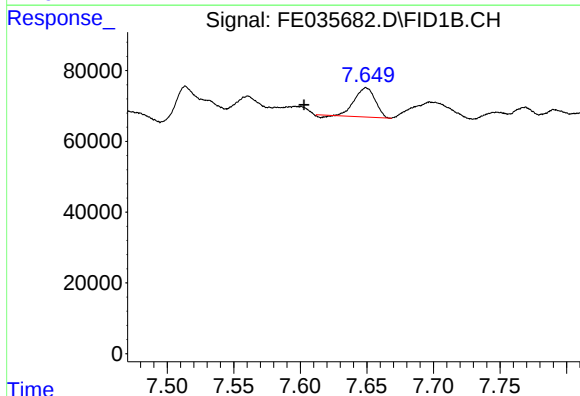


#4 N-TETRADECANE

R.T.: 7.649 min
Delta R.T.: 0.047 min
Response: 90394
Conc: 0.70 ug/ml

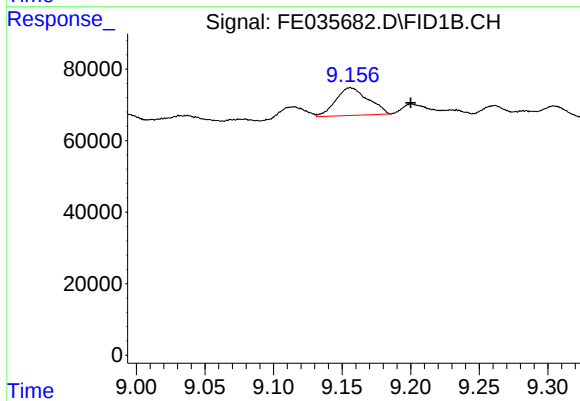

#5 N-HEXADECANE

R.T.: 9.156 min
Delta R.T.: -0.044 min
Response: 127953
Conc: 0.99 ug/ml

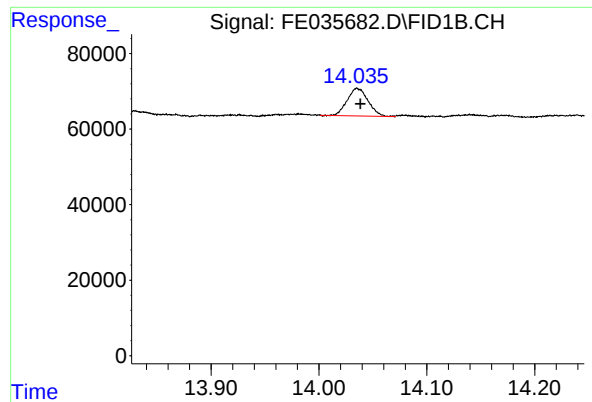

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.035 min
Delta R.T.: -0.003 min
Response: 98402
Conc: 0.88 ug/ml

Instrument :
FID_E
ClientSampleId :