

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051622\
 Data File : FE035701.D
 Signal(s) : FID1B.CH
 Acq On : 16 May 2022 22:07
 Operator : YP\AJ
 Sample : N2832-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 16 23:05:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
 Quant Title :
 QLast Update : Fri May 13 15:02:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.037	1797873	16.013 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051622\
 Data File : FE035701.D
 Signal(s) : FID1B.CH
 Acq On : 16 May 2022 22:07
 Operator : YP\AJ
 Sample : N2832-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 16 23:05:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
 Quant Title :
 QLast Update : Fri May 13 15:02:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

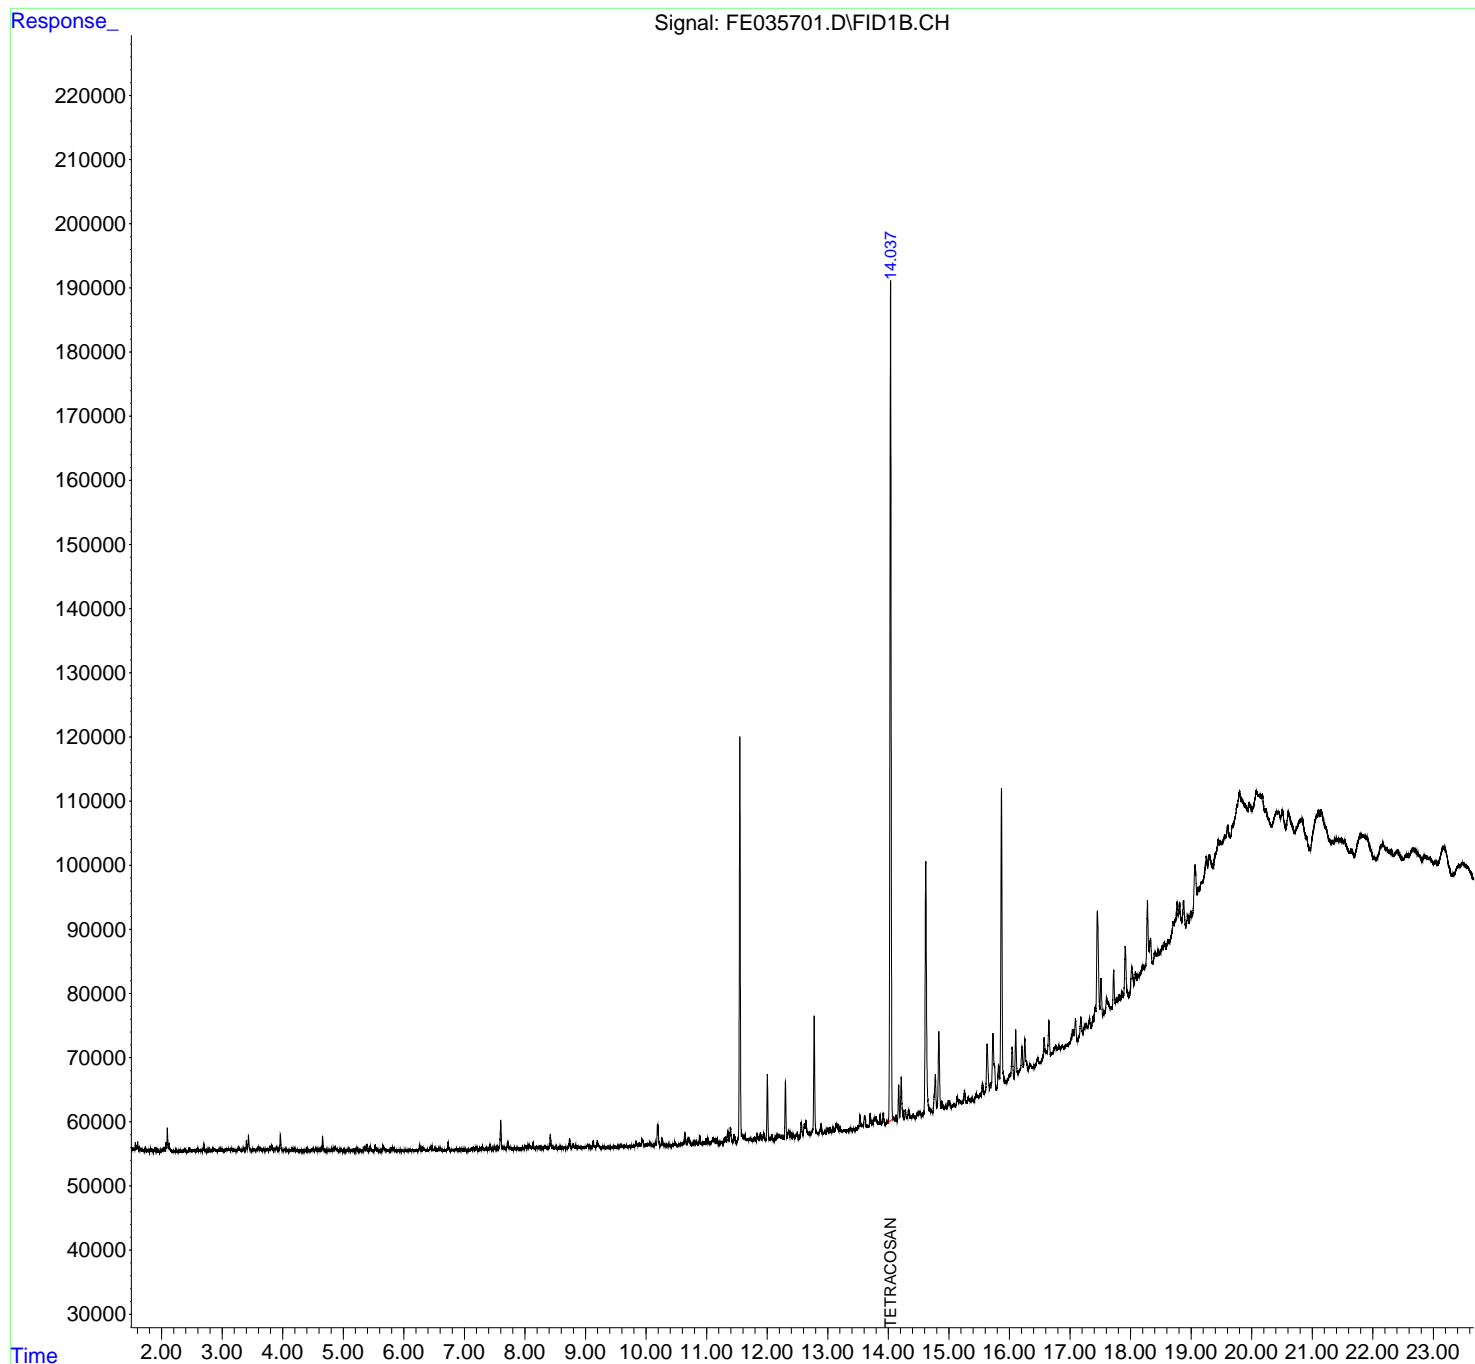

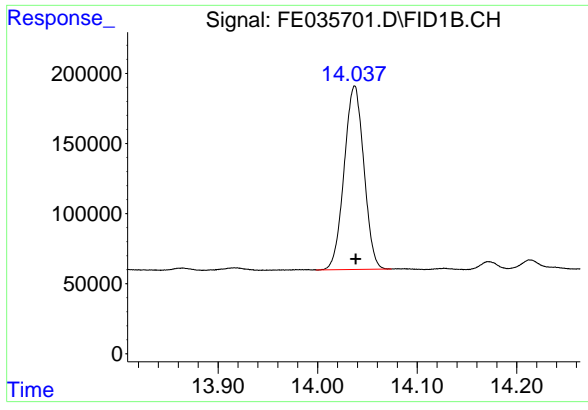

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.037 min
Delta R.T.: -0.001 min
Response: 1797873
Conc: 16.01 ug/ml

Instrument :
FID_E
ClientSampleId :