

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051623AL\
Data File : FE041930.D
Signal(s) : FID1B.ch
Acq On : 16 May 2023 08:52
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 16 11:00:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.122	26285	0.173 ug/ml
19) T	n-Tetratriacontane (C34)	19.741	44670	0.317 ug/ml
20) T	n-Hexatriacontane (C36)	20.544f	42366	0.317 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051623AL\
Data File : FE041930.D
Signal(s) : FID1B.ch
Acq On : 16 May 2023 08:52
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 16 11:00:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

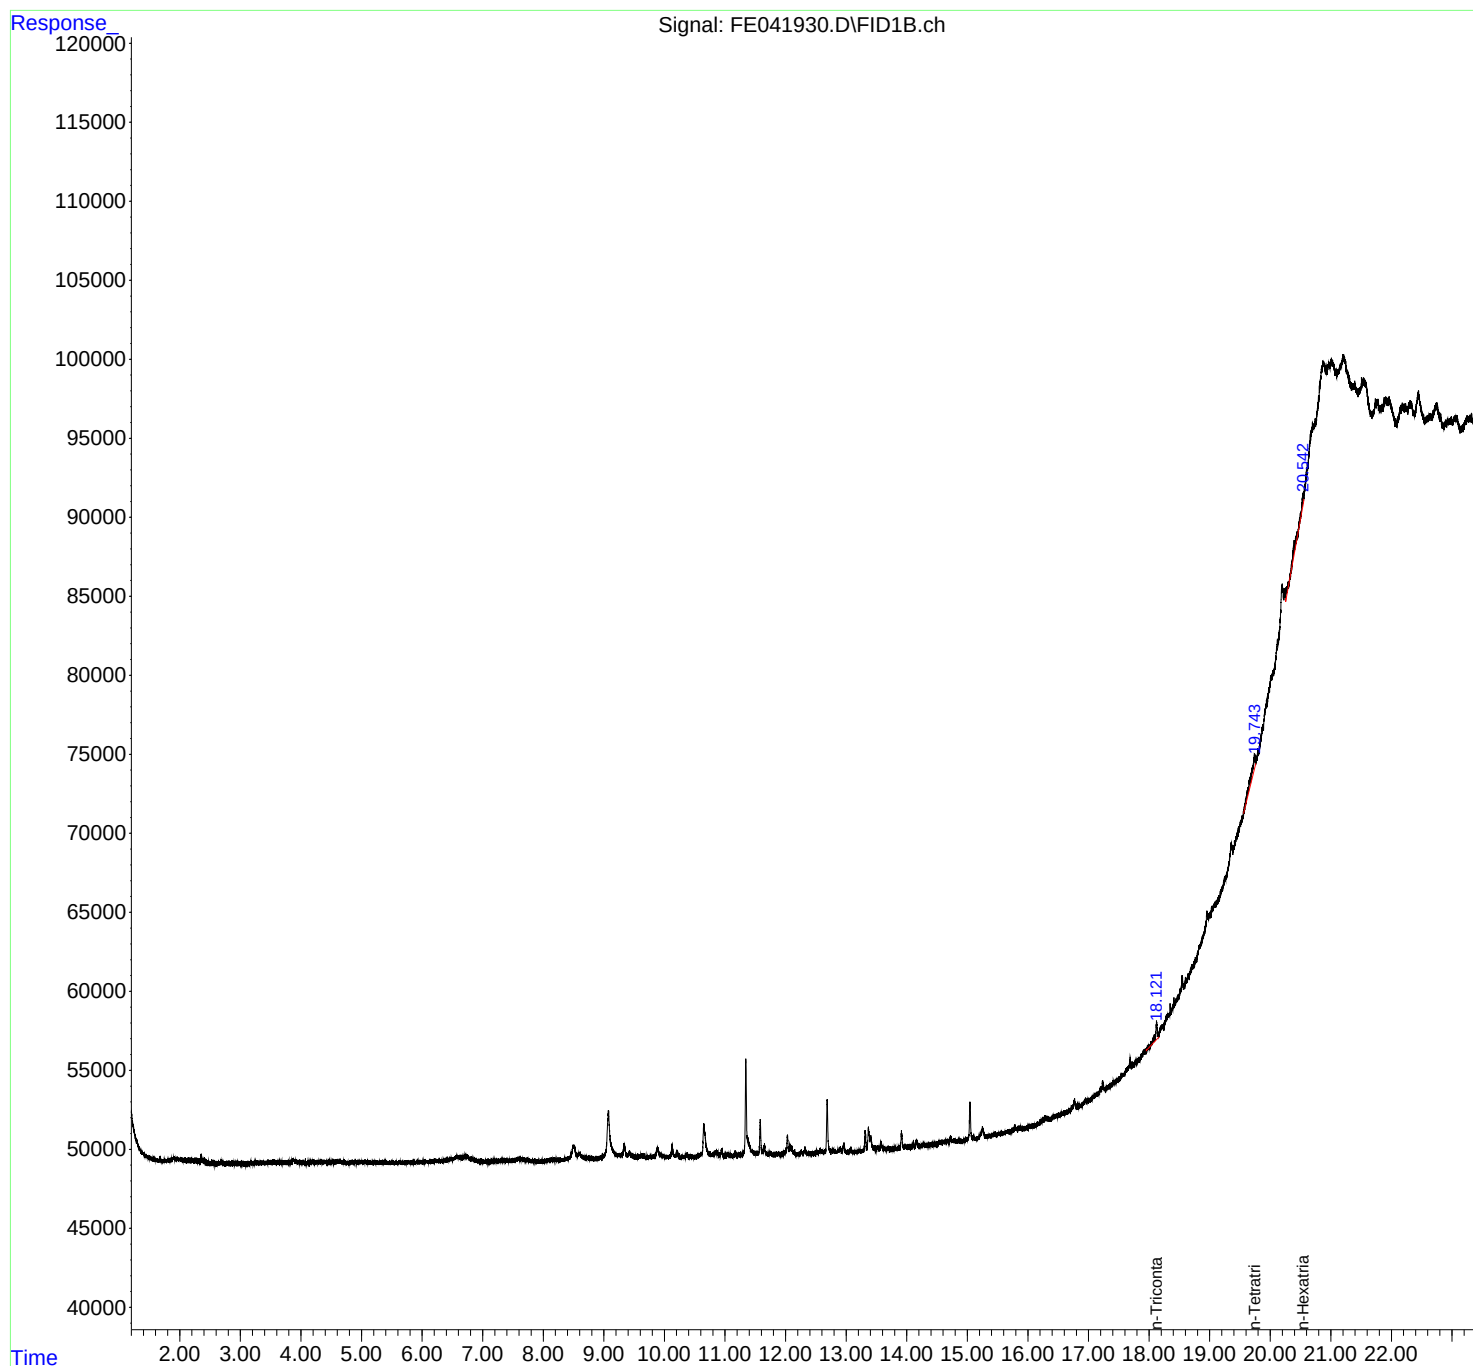


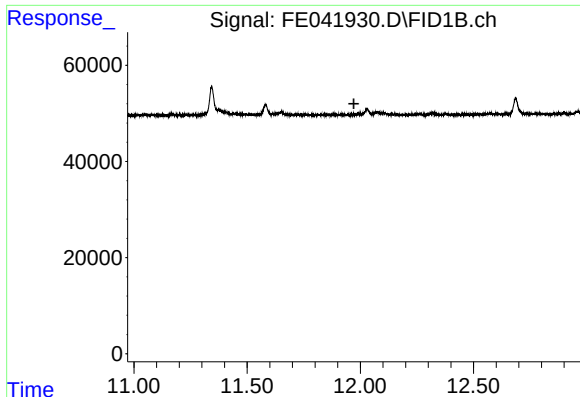

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

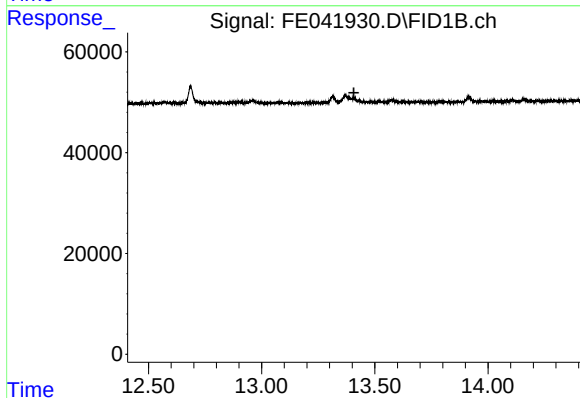


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.408 min
Response: 0
Conc: N.D.

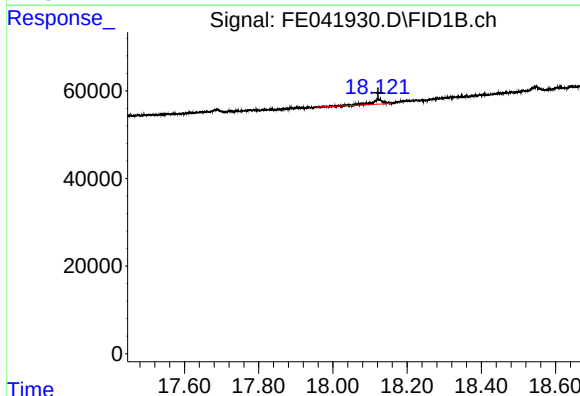


#17 n-Tricontane (C30)

R.T.: 18.122 min
Delta R.T.: 0.000 min
Response: 26285
Conc: 0.17 ug/ml

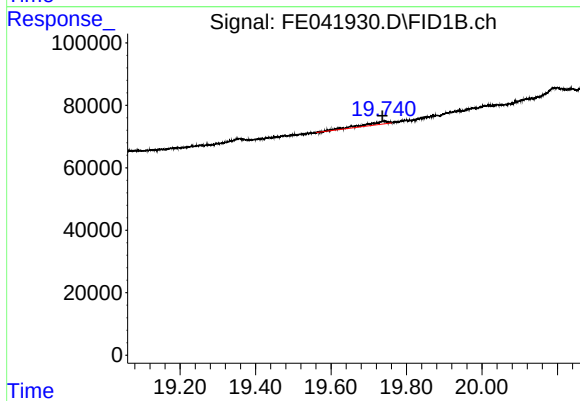

#19 n-Tetratriacontane (C34)

R.T.: 19.741 min
Delta R.T.: 0.005 min
Response: 44670
Conc: 0.32 ug/ml

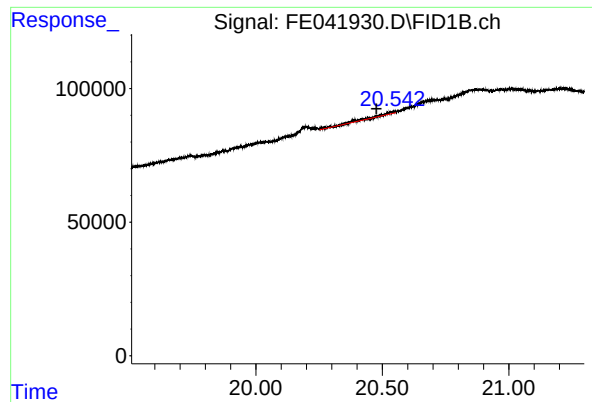

#20 n-Hexatriacontane (C36)

R.T.: 20.544 min
Delta R.T.: 0.068 min
Response: 42366
Conc: 0.32 ug/ml

Instrument :

FID_E

ClientSampleId :