

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051623AL\  
 Data File : FE041935.D  
 Signal(s) : FID1B.ch  
 Acq On : 16 May 2023 11:24  
 Operator : YP\AJ  
 Sample : 02770-01DL 20X  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 CHRT-25990DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 05/17/2023  
 Supervised By :Ankita Jodhani 05/17/2023

Integration File: autoint1.e  
 Quant Time: May 17 02:23:13 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 042123.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Apr 21 07:33:51 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.970 | 579706     | 3.090 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 6.18%        |
| 12) S 1-chlorooctadecane (S... | 13.407 | 250700     | 1.775 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 3.55%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051623AL\  
Data File : FE041935.D  
Signal(s) : FID1B.ch  
Acq On : 16 May 2023 11:24  
Operator : YP\AJ  
Sample : 02770-01DL 20X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
CHRT-25990DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 05/17/2023  
Supervised By :Ankita Jodhani 05/17/2023

Integration File: autoint1.e  
Quant Time: May 17 02:23:13 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 042123.  
Quant Title : GC Extractables  
QLast Update : Fri Apr 21 07:33:51 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

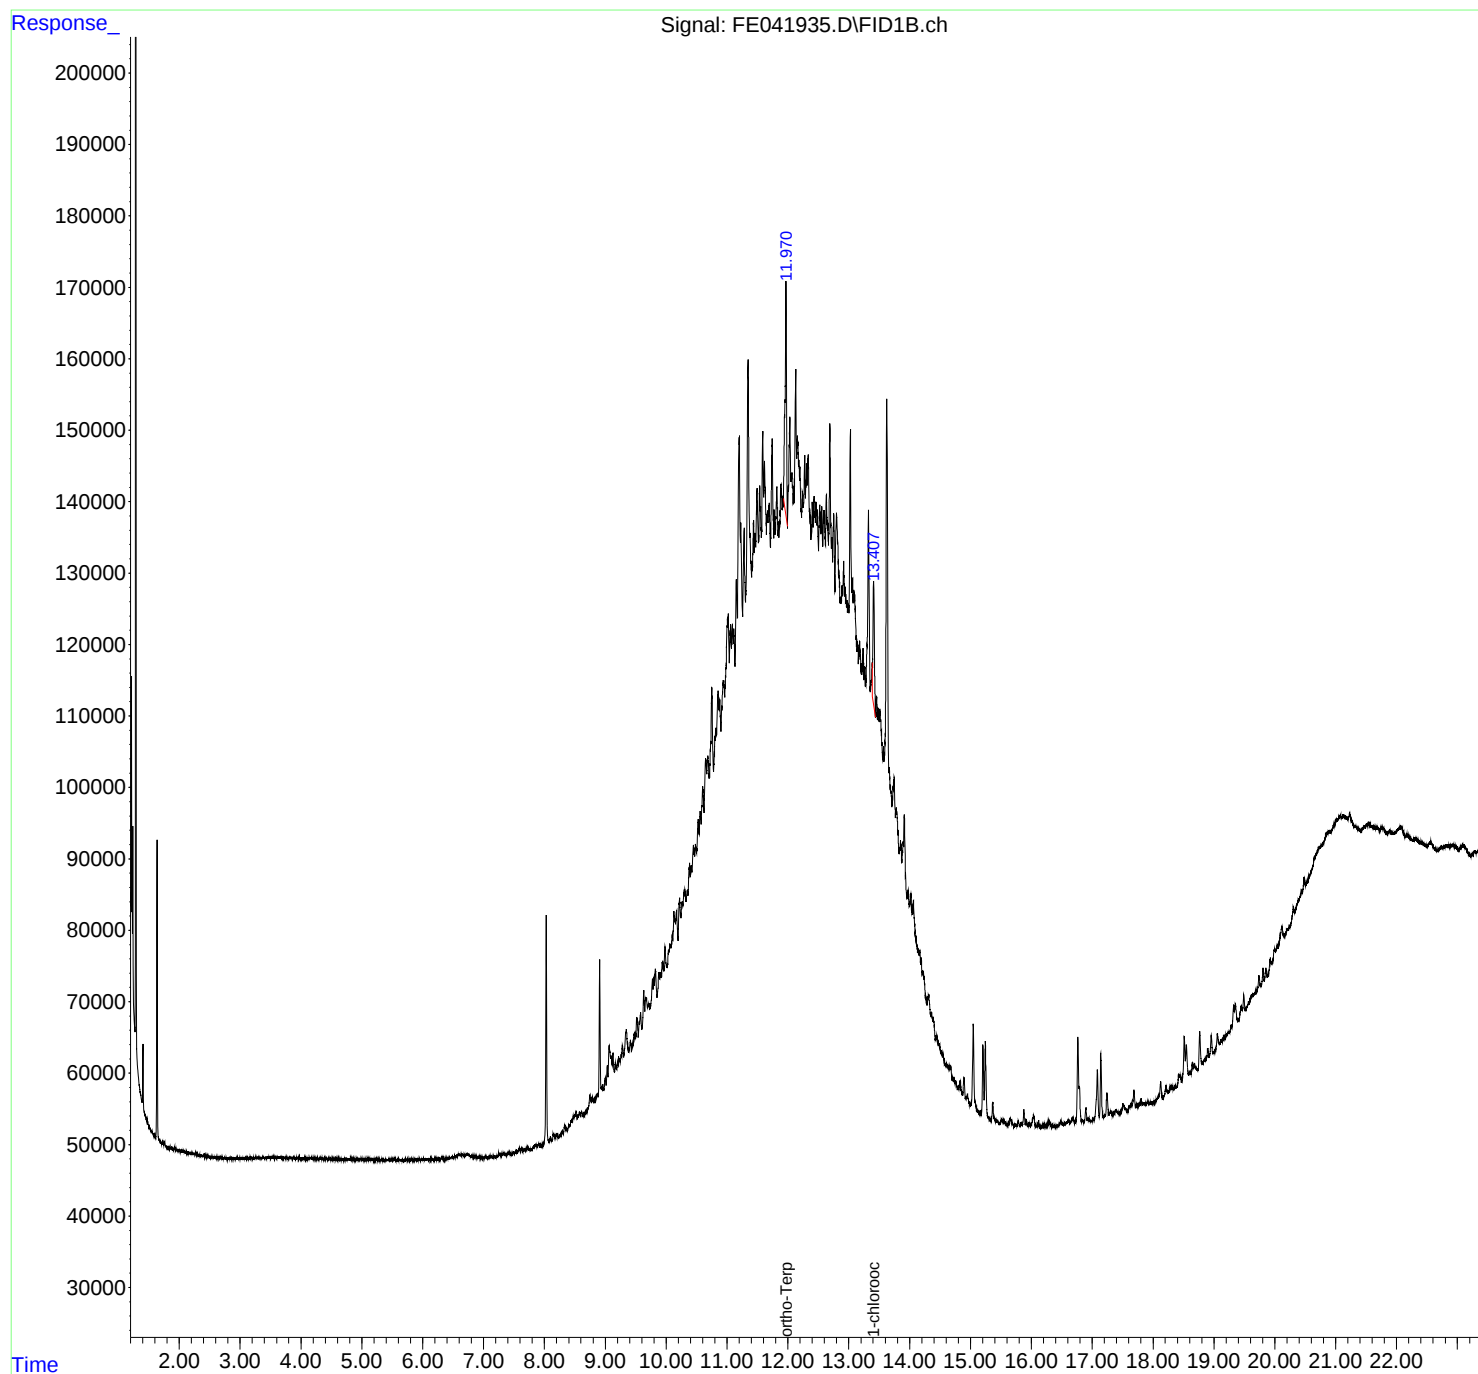

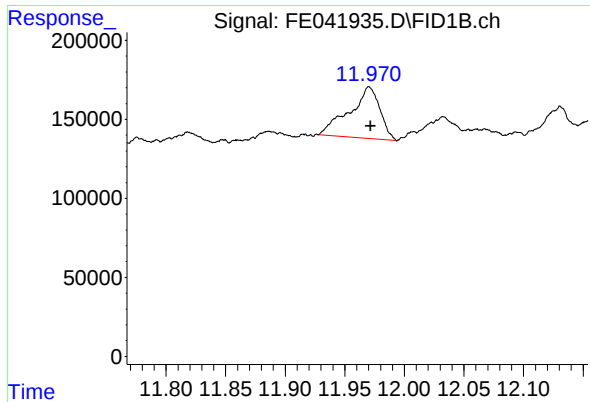


#9 ortho-Terphenyl (SURR)

R.T.: 11.970 min  
Delta R.T.: -0.002 min  
Response: 579706  
Conc: 3.09 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
CHRT-25990DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 05/17/2023  
Supervised By :Ankita Jodhani 05/17/2023

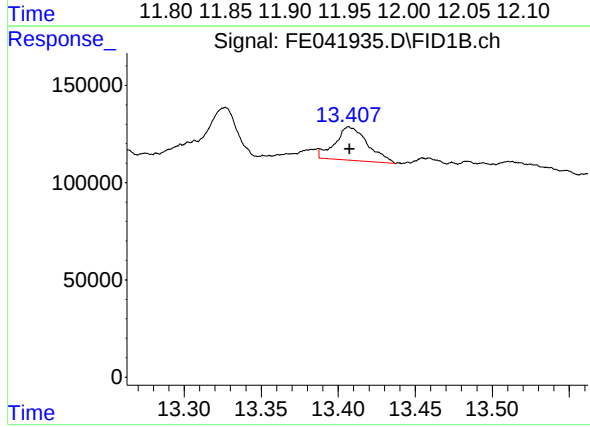

#12 1-chlorooctadecane (SURR)

R.T.: 13.407 min  
Delta R.T.: 0.000 min  
Response: 250700  
Conc: 1.77 ug/ml m