

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051721\
 Data File : FE033806.D
 Signal(s) : FID1B.CH
 Acq On : 17 May 2021 11:24
 Operator : DD\AJ
 Sample : M2262-09
 Misc : MDL-WATER- 1 PPM
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 17 15:39:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.715	8209484	20.312 ug/ml
Target Compounds			
2) N-DECANE	4.458	715766	1.668 ug/ml
3) N-DODECANE	6.467	665066	1.520 ug/ml
4) N-TETRADECANE	8.261	717103	1.592 ug/ml
5) N-HEXADECANE	9.861	708402	1.572 ug/ml
6) N-OCTADECANE	11.302	724552	1.573 ug/ml
7) N-EICOSANE	12.613	751043	1.636 ug/ml
8) N-DOCOSANE	13.810	768168	1.666 ug/ml
10) N-TETRACOSANE	14.914	777311	1.683 ug/ml
11) N-HEXACOSANE	15.935	762400	1.662 ug/ml
12) N-OCTACOSANE	16.885	797468	1.739 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051721\
Data File : FE033806.D
Signal(s) : FID1B.CH
Acq On : 17 May 2021 11:24
Operator : DD\AJ
Sample : M2262-09
Misc : MDL-WATER- 1 PPM
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 17 15:39:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

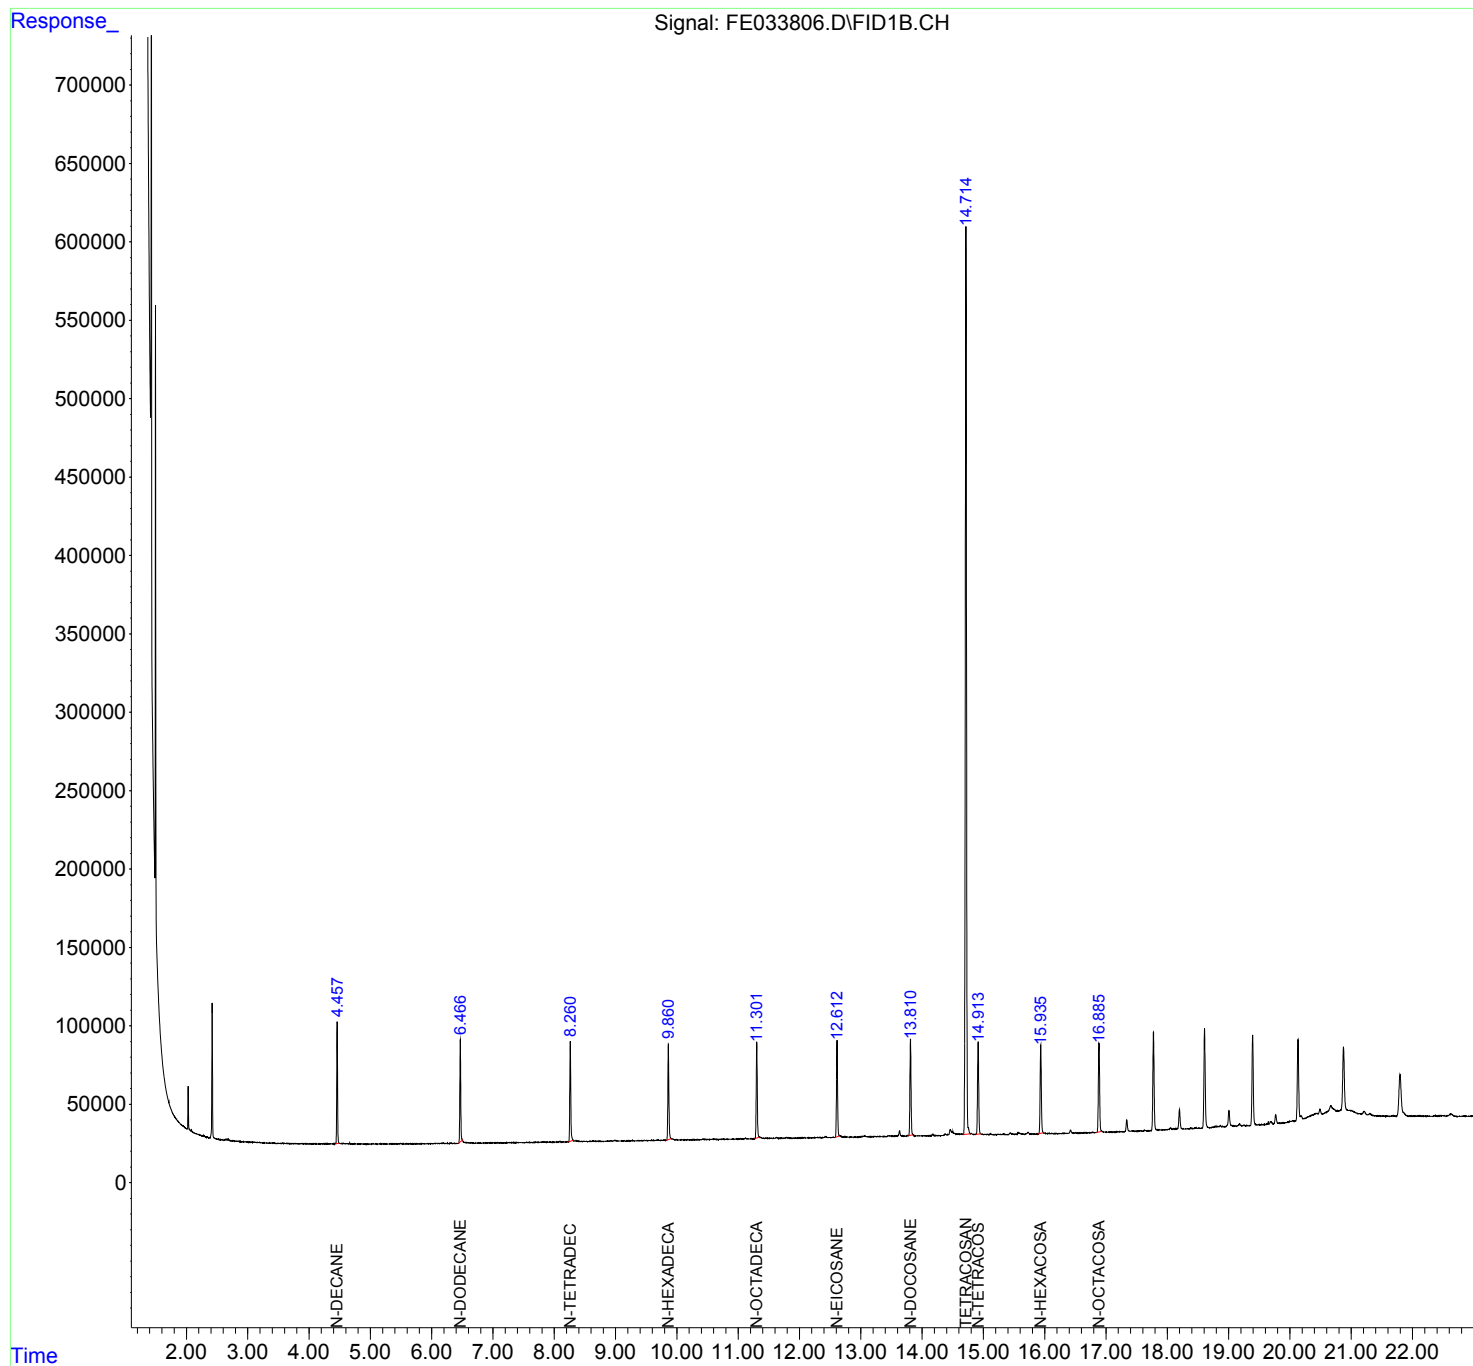

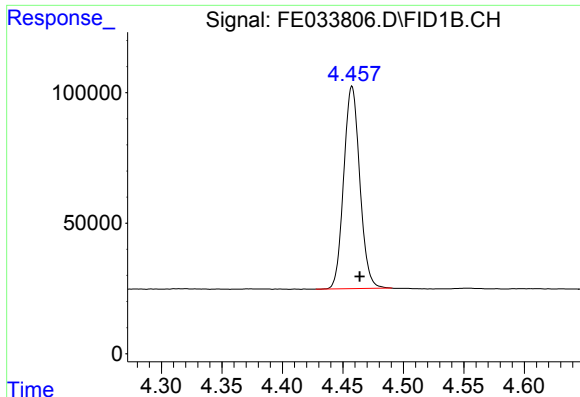


#2 N-DECANE

R.T.: 4.458 min
Delta R.T.: -0.006 min
Response: 715766
Conc: 1.67 ug/ml

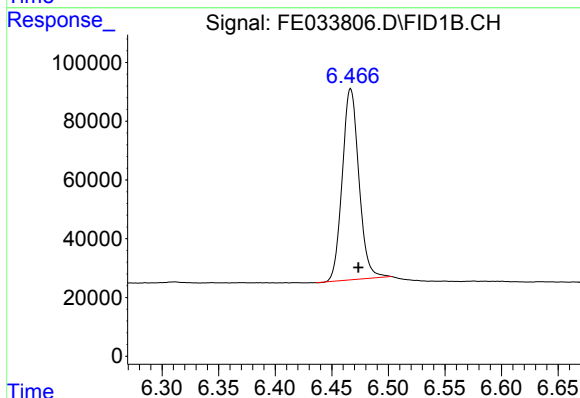


#3 N-DODECANE

R.T.: 6.467 min
Delta R.T.: -0.007 min
Response: 665066
Conc: 1.52 ug/ml

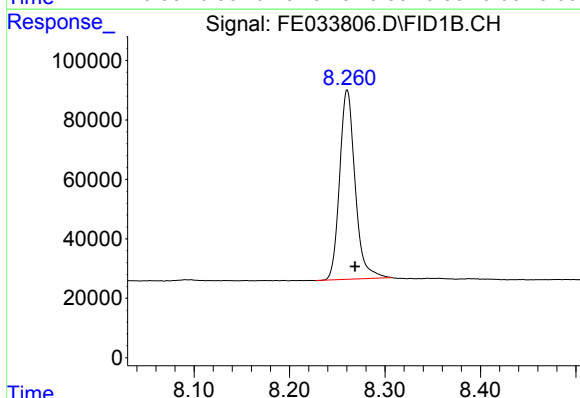


#4 N-TETRADECANE

R.T.: 8.261 min
Delta R.T.: -0.008 min
Response: 717103
Conc: 1.59 ug/ml

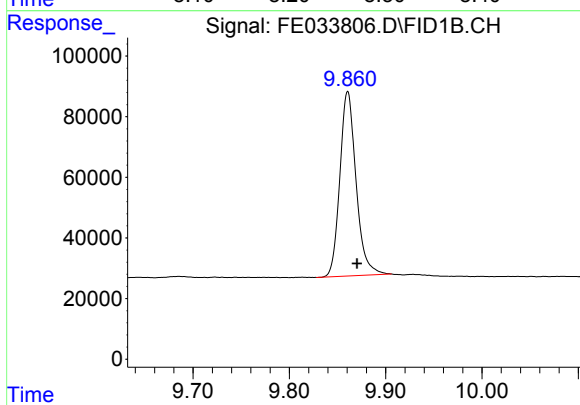


#5 N-HEXADECANE

R.T.: 9.861 min
Delta R.T.: -0.009 min
Response: 708402
Conc: 1.57 ug/ml

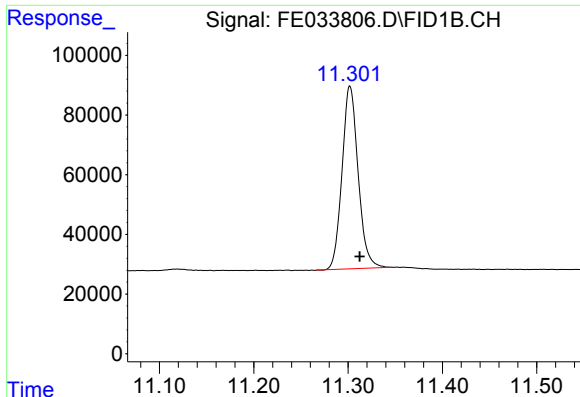


#6 N-OCTADECANE

R.T.: 11.302 min
Delta R.T.: -0.010 min
Response: 724552
Conc: 1.57 ug/ml

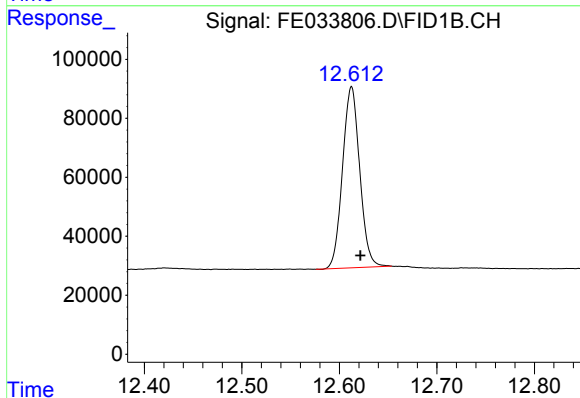


#7 N-EICOSANE

R.T.: 12.613 min
Delta R.T.: -0.009 min
Response: 751043
Conc: 1.64 ug/ml

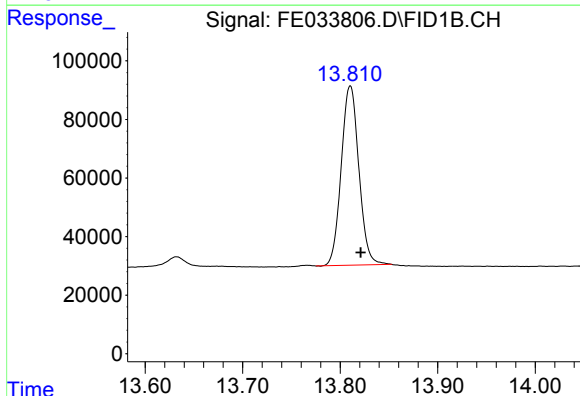


#8 N-DOCOSANE

R.T.: 13.810 min
Delta R.T.: -0.011 min
Response: 768168
Conc: 1.67 ug/ml

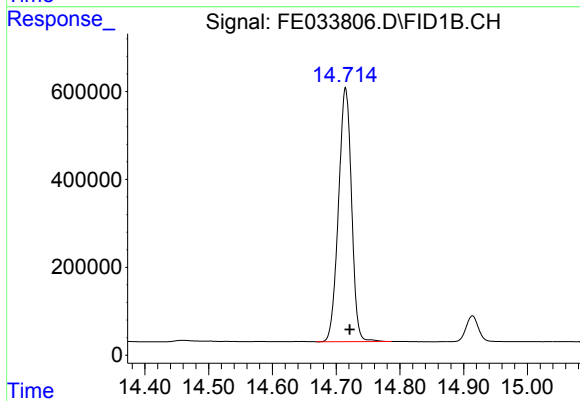


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: -0.007 min
Response: 8209484
Conc: 20.31 ug/ml

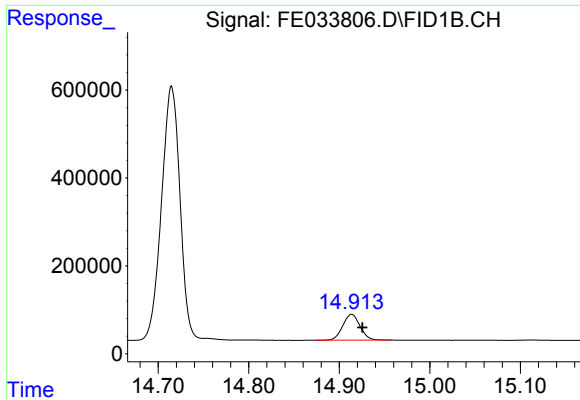


#10 N-TETRACOSANE

R.T.: 14.914 min
Delta R.T.: -0.012 min
Response: 777311
Conc: 1.68 ug/ml

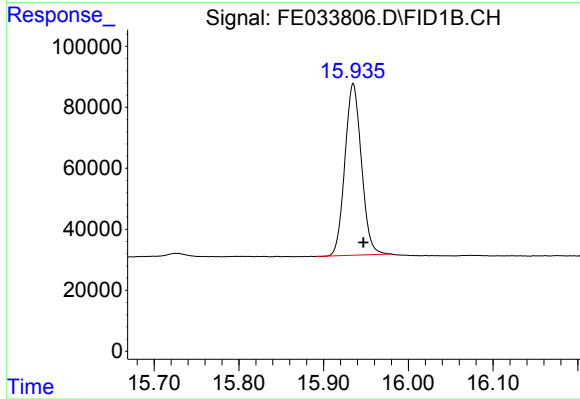

#11 N-HEXACOSANE

R.T.: 15.935 min
Delta R.T.: -0.012 min
Response: 762400
Conc: 1.66 ug/ml

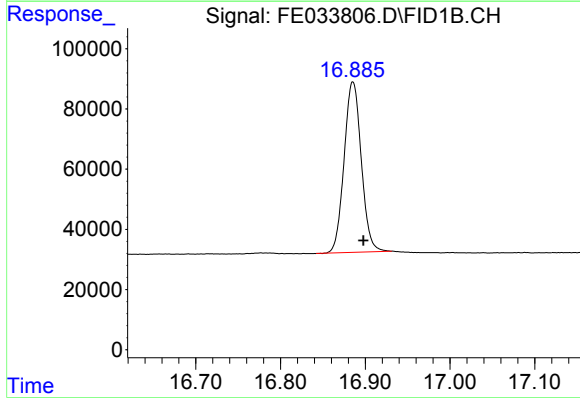

#12 N-OCTACOSANE

R.T.: 16.885 min
Delta R.T.: -0.012 min
Response: 797468
Conc: 1.74 ug/ml