

Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
 Data File : FE027351.D
 Signal(s) : FID1B.CH
 Acq On : 18 May 2018 15:15
 Operator : UA/AJ
 Sample : J2673-03 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 19 04:40:24 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.269	317614	2.157 ug/ml
Target Compounds			
3) N-DODECANE	6.966	125177	0.720 ug/ml
4) N-TETRADECANE	8.775	474348	2.510 ug/ml
5) N-HEXADECANE	10.388	592846	3.015 ug/ml
6) N-OCTADECANE	11.839	548903	2.734 ug/ml
7) N-EICOSANE	13.159	411360	2.160 ug/ml
8) N-DOCOSANE	14.367	380084	2.131 ug/ml
10) N-TETRACOSANE	15.476	717134	4.258 ug/ml
12) N-OCTACOSANE	17.453	159428	0.965 ug/ml
14) N-DOTRIACONTANE	19.183	196993	1.147 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
Data File : FE027351.D
Signal(s) : FID1B.CH
Acq On : 18 May 2018 15:15
Operator : UA/AJ
Sample : J2673-03 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 19 04:40:24 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

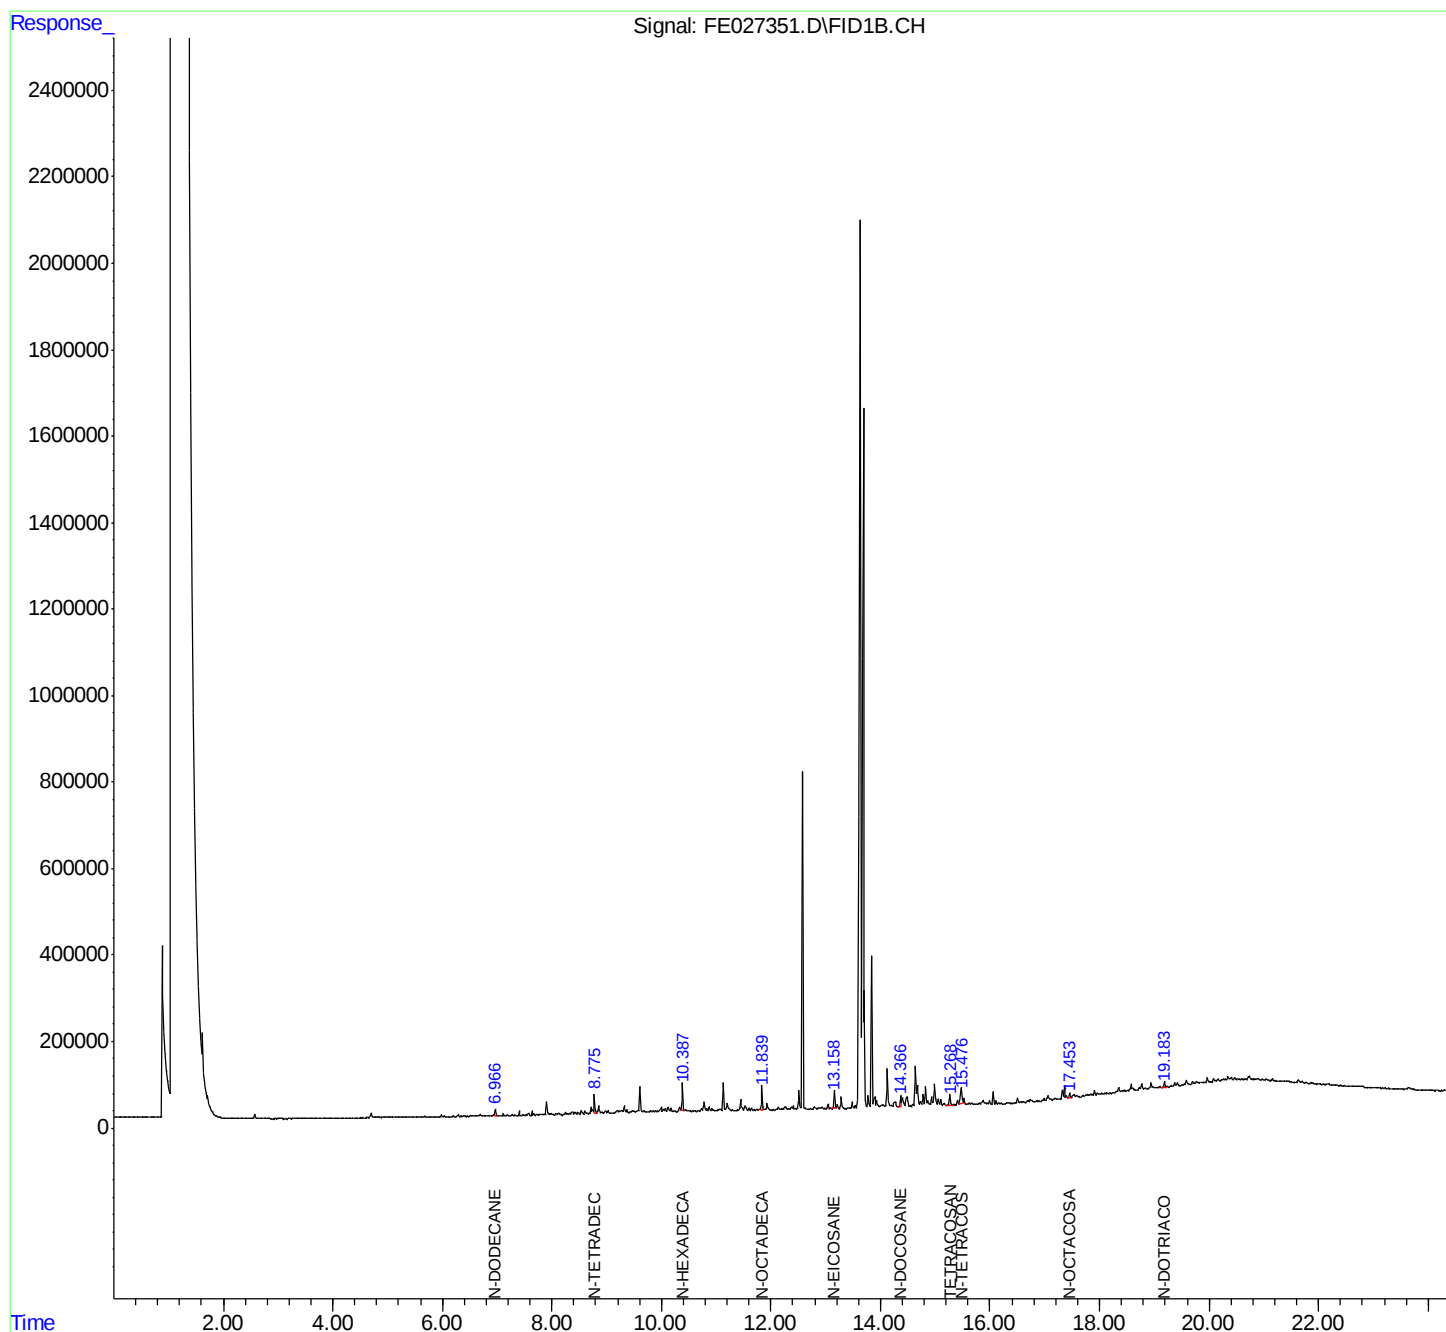


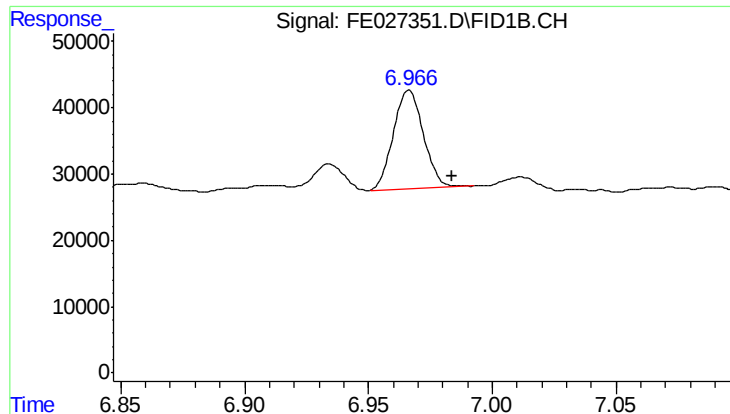

#3 N-DODECANE


R.T.: 6.966 min
Delta R.T.: -0.017 min
Response: 125177
Conc: 0.72 ug/ml

Instrument :
FID_E
ClientSampleId :

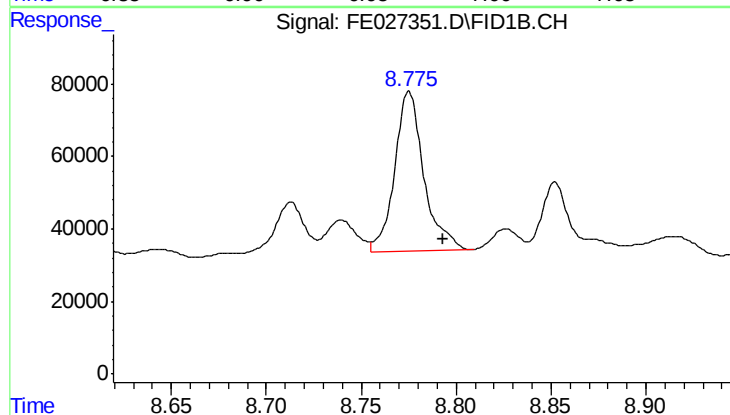


#4 N-TETRADECANE

R.T.: 8.775 min
Delta R.T.: -0.018 min
Response: 474348
Conc: 2.51 ug/ml

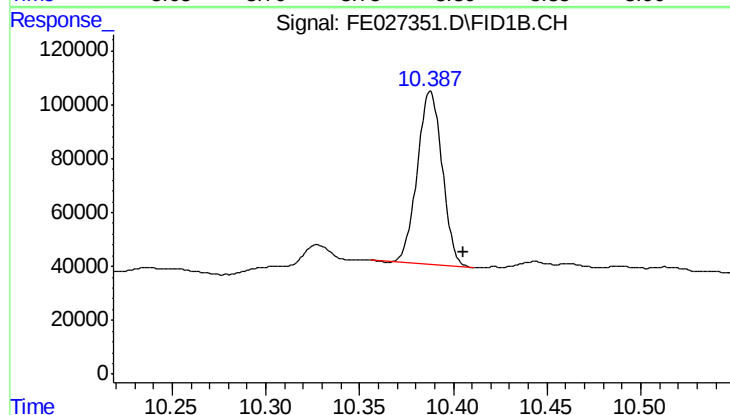


#5 N-HEXADECANE

R.T.: 10.388 min
Delta R.T.: -0.018 min
Response: 592846
Conc: 3.02 ug/ml

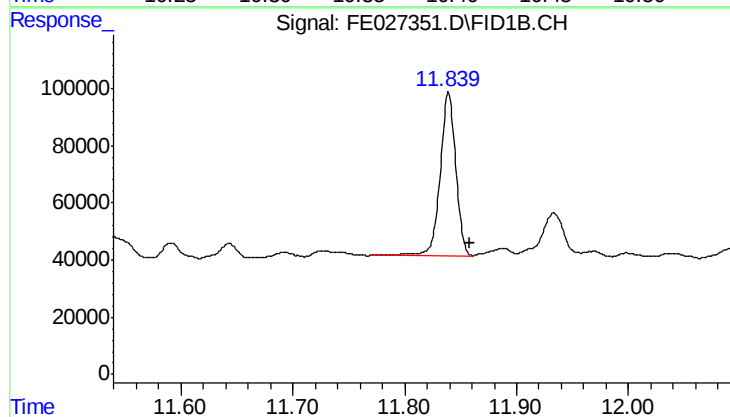

#6 N-OCTADECANE


R.T.: 11.839 min
Delta R.T.: -0.019 min
Response: 548903
Conc: 2.73 ug/ml

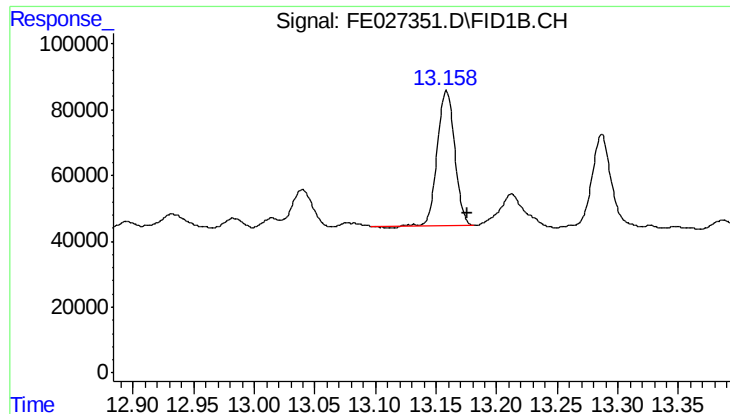

#7 N-EICOSANE


R.T.: 13.159 min
Delta R.T.: -0.018 min
Response: 411360
Conc: 2.16 ug/ml

Instrument :
FID_E
ClientSampleId :

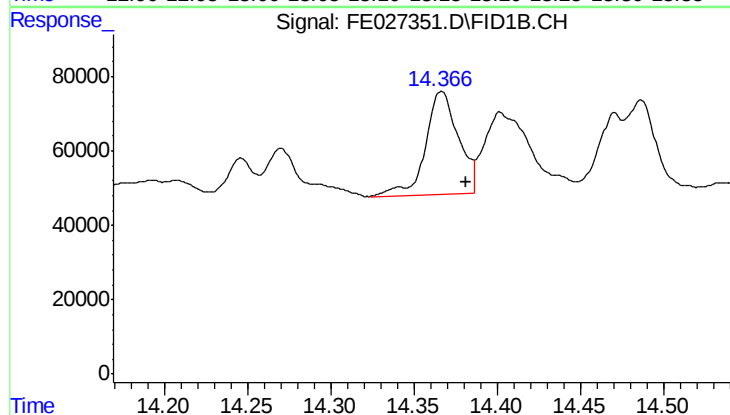


#8 N-DOCOSANE

R.T.: 14.367 min
Delta R.T.: -0.015 min
Response: 380084
Conc: 2.13 ug/ml

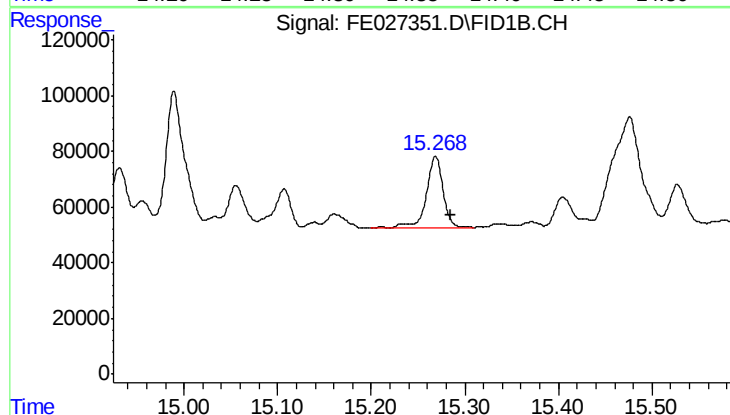


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.269 min
Delta R.T.: -0.016 min
Response: 317614
Conc: 2.16 ug/ml

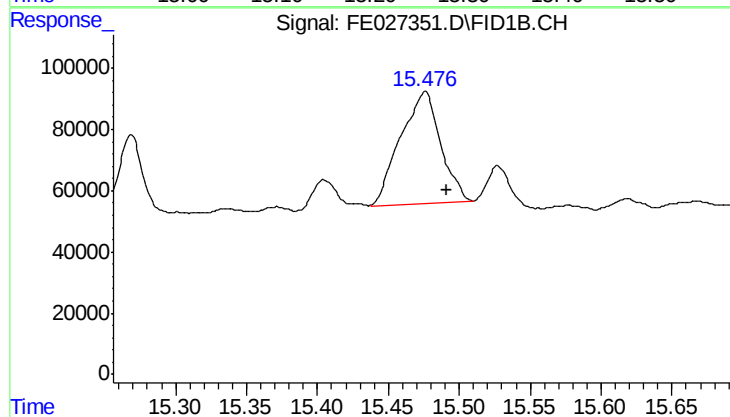

#10 N-TETRACOSANE


R.T.: 15.476 min
Delta R.T.: -0.015 min
Response: 717134
Conc: 4.26 ug/ml

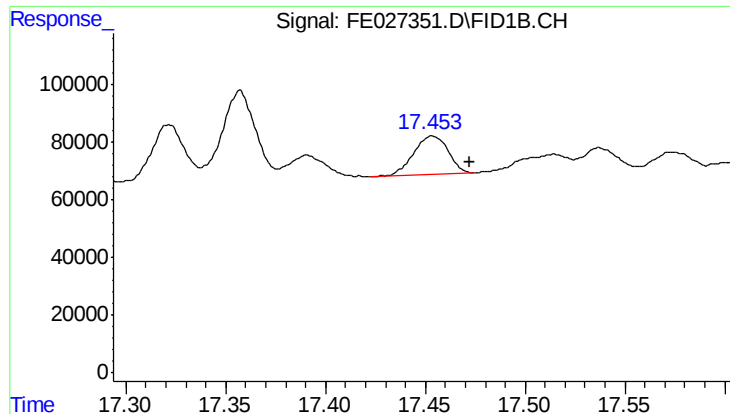

#12 N-OCTACOSANE

R.T.: 17.453 min
Delta R.T.: -0.019 min
Response: 159428
Conc: 0.96 ug/ml

Instrument :
FID_E
ClientSampleId :

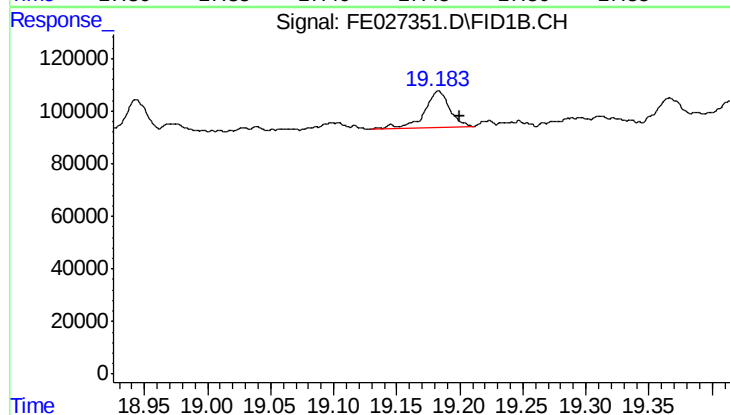

#14 N-DOTRIACONTANE

R.T.: 19.183 min
Delta R.T.: -0.016 min
Response: 196993
Conc: 1.15 ug/ml