

Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
 Data File : FE027356.D
 Signal(s) : FID1B.CH
 Acq On : 18 May 2018 18:05
 Operator : UA/AJ
 Sample : J2673-13 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 19 04:41:20 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.269	450154	3.057 ug/ml
Target Compounds			
4) N-TETRADECANE	8.776	132306	0.700 ug/ml
5) N-HEXADECANE	10.388	287281	1.461 ug/ml
6) N-OCTADECANE	11.840	371647	1.851 ug/ml
7) N-EICOSANE	13.158	299186	1.571 ug/ml
8) N-DOCOSANE	14.366	139692	0.783 ug/ml
10) N-TETRACOSANE	15.474	430079	2.554 ug/ml
13) N-TRIACONTANE	18.350	132652	0.788 ug/ml
14) N-DOTRIACONTANE	19.185	162328	0.945 ug/ml
16) N-HEXATRIACONTANE	20.738	251115	1.427 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
Data File : FE027356.D
Signal(s) : FID1B.CH
Acq On : 18 May 2018 18:05
Operator : UA/AJ
Sample : J2673-13 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 19 04:41:20 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

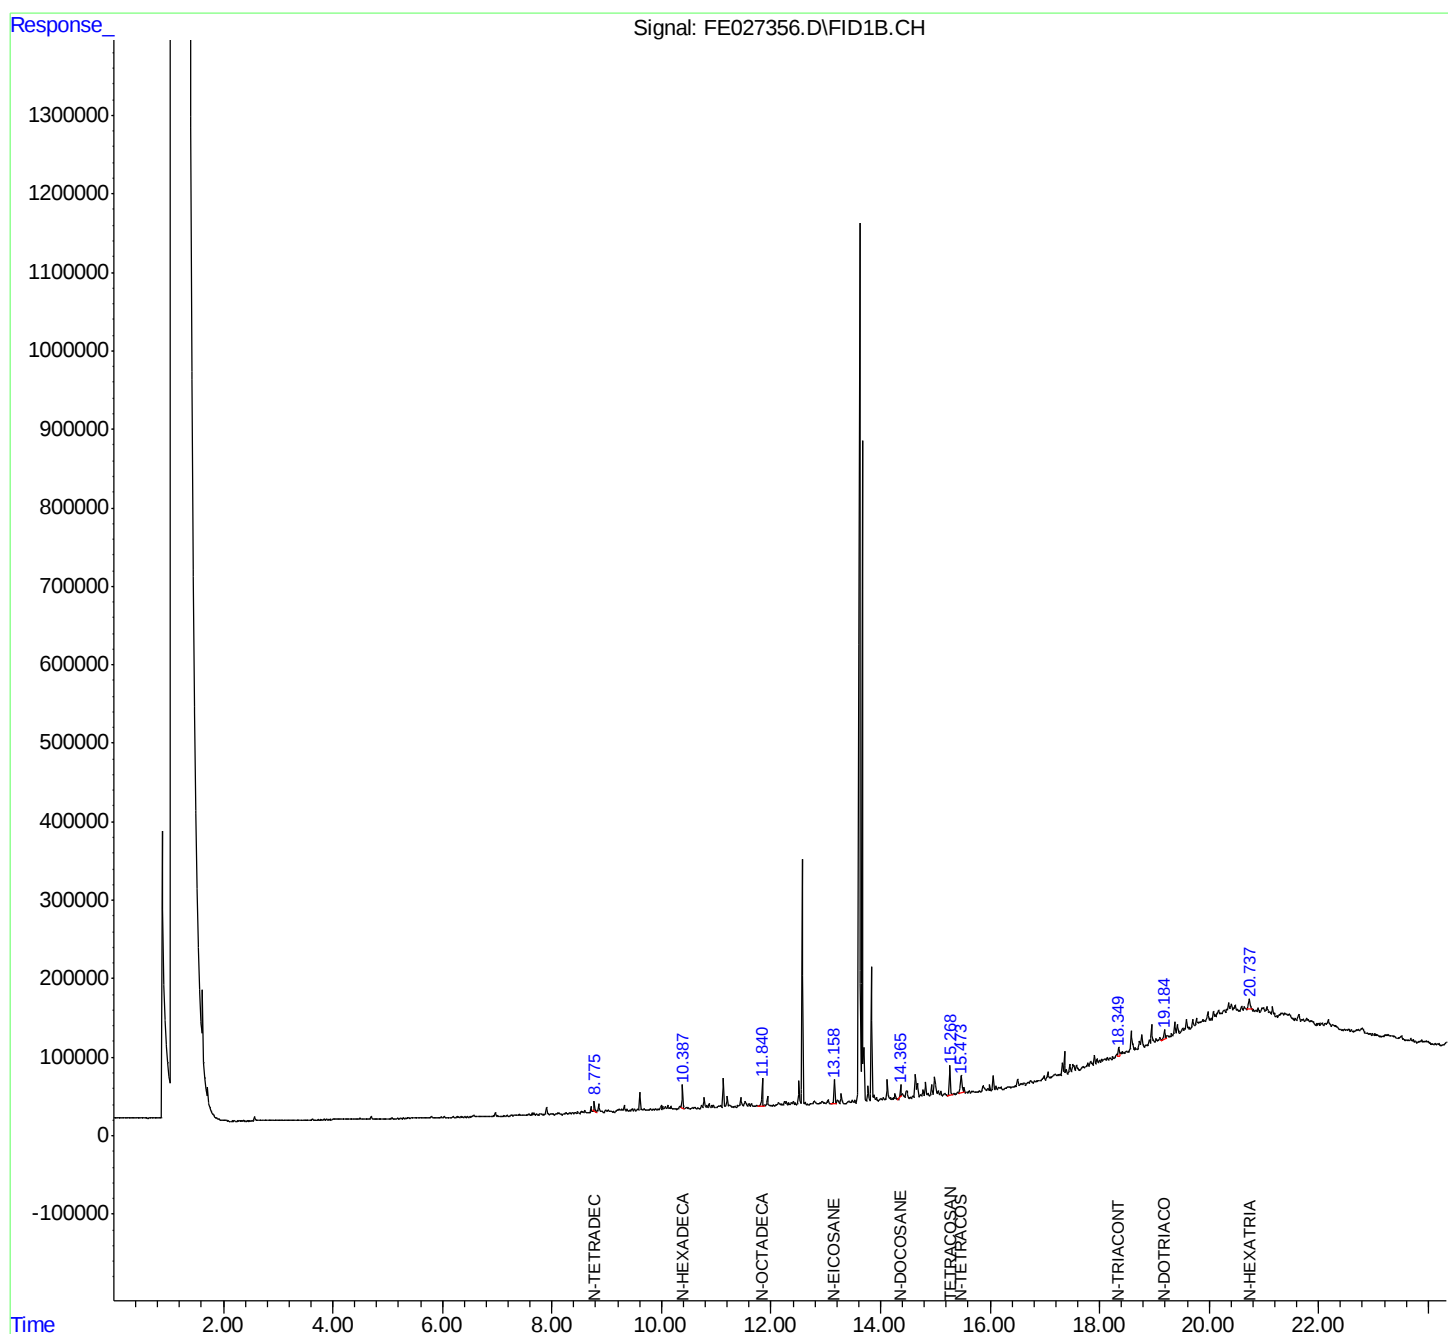


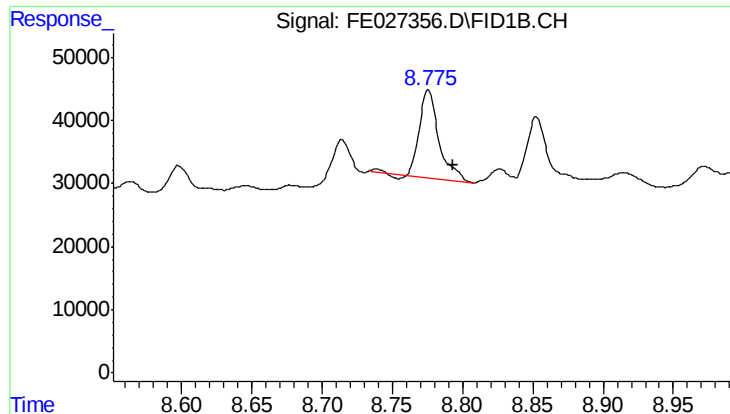

#4 N-TETRADECANE


R.T.: 8.776 min
Delta R.T.: -0.018 min
Response: 132306
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :

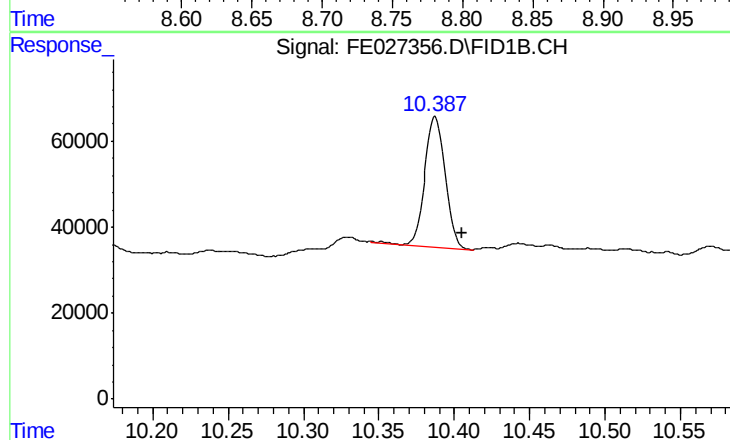


#5 N-HEXADECANE

R.T.: 10.388 min
Delta R.T.: -0.018 min
Response: 287281
Conc: 1.46 ug/ml

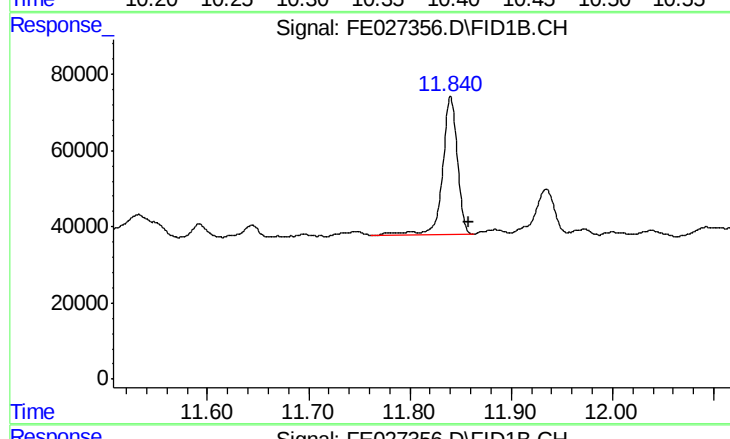


#6 N-OCTADECANE

R.T.: 11.840 min
Delta R.T.: -0.018 min
Response: 371647
Conc: 1.85 ug/ml

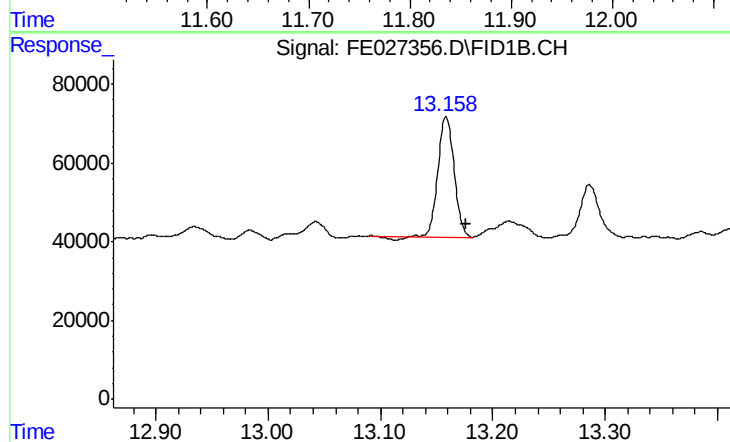

#7 N-EICOSANE


R.T.: 13.158 min
Delta R.T.: -0.018 min
Response: 299186
Conc: 1.57 ug/ml

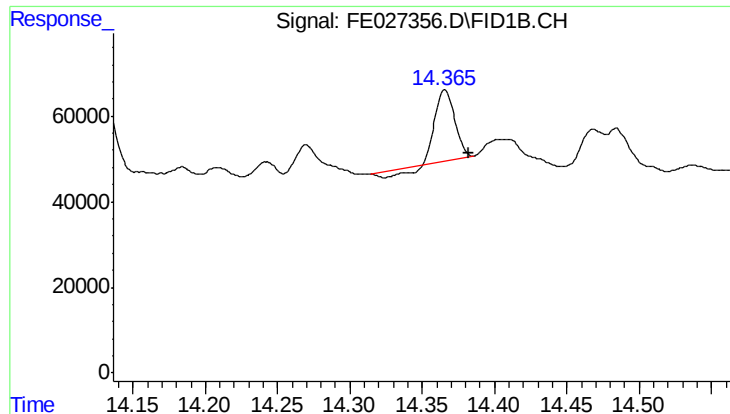

#8 N-DOCOSANE


R.T.: 14.366 min
Delta R.T.: -0.016 min
Response: 139692
Conc: 0.78 ug/ml

Instrument :
FID_E
ClientSampleId :

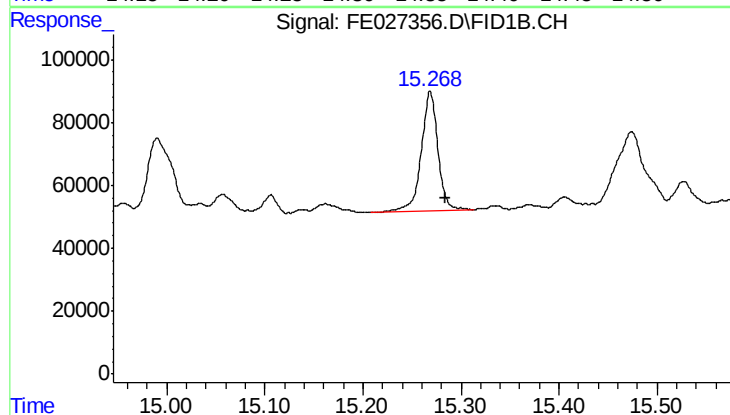


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.269 min
Delta R.T.: -0.016 min
Response: 450154
Conc: 3.06 ug/ml

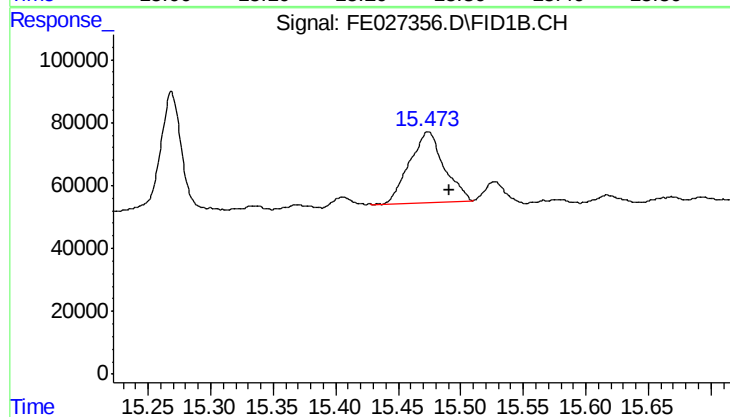


#10 N-TETRACOSANE

R.T.: 15.474 min
Delta R.T.: -0.017 min
Response: 430079
Conc: 2.55 ug/ml

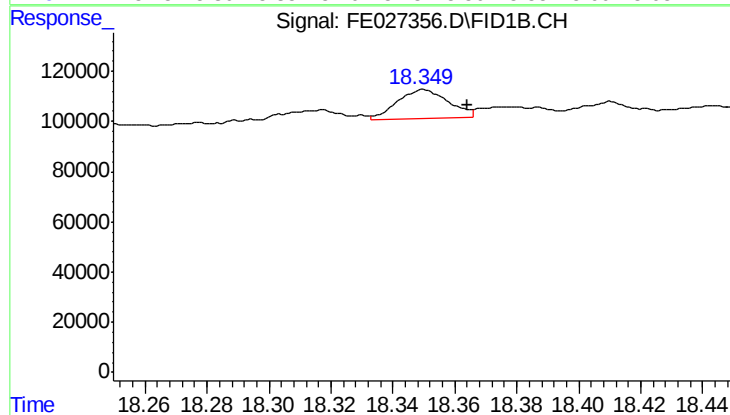

#13 N-TRIACONTANE


R.T.: 18.350 min
Delta R.T.: -0.014 min
Response: 132652
Conc: 0.79 ug/ml

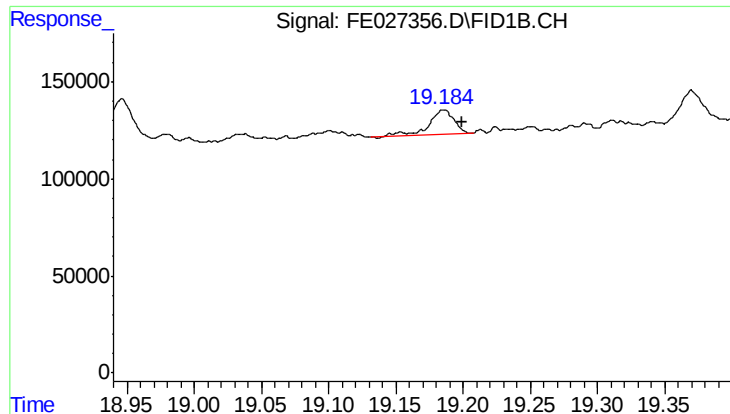

#14 N-DOTRIACONTANE

R.T.: 19.185 min
Delta R.T.: -0.014 min
Response: 162328
Conc: 0.94 ug/ml

Instrument :
FID_E
ClientSampleId :

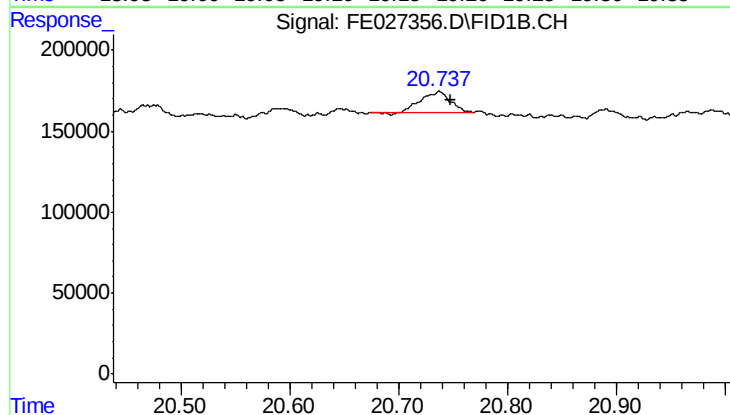

#16 N-HEXATRIACONTANE

R.T.: 20.738 min
Delta R.T.: -0.010 min
Response: 251115
Conc: 1.43 ug/ml