

Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
 Data File : FE027358.D
 Signal(s) : FID1B.CH
 Acq On : 18 May 2018 19:14
 Operator : UA/AJ
 Sample : J2677-05 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 19 04:41:48 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.269	266761	1.812 ug/ml
Target Compounds			
5) N-HEXADECANE	10.389	148236	0.754 ug/ml
6) N-OCTADECANE	11.840	164020	0.817 ug/ml
7) N-EICOSANE	13.159	169508	0.890 ug/ml
8) N-DOCOSANE	14.365	161812	0.907 ug/ml
10) N-TETRACOSANE	15.476	181997	1.081 ug/ml
11) N-HEXACOSANE	16.501	173921	1.053 ug/ml
12) N-OCTACOSANE	17.456	173663	1.051 ug/ml
13) N-TRIACONTANE	18.350	214749	1.276 ug/ml
14) N-DOTRIACONTANE	19.187	250449	1.458 ug/ml
15) N-TETRATRIACONTANE	19.974	231716	1.293 ug/ml
16) N-HEXATRIACONTANE	20.736	358054	2.035 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
Data File : FE027358.D
Signal(s) : FID1B.CH
Acq On : 18 May 2018 19:14
Operator : UA/AJ
Sample : J2677-05 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: May 19 04:41:48 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

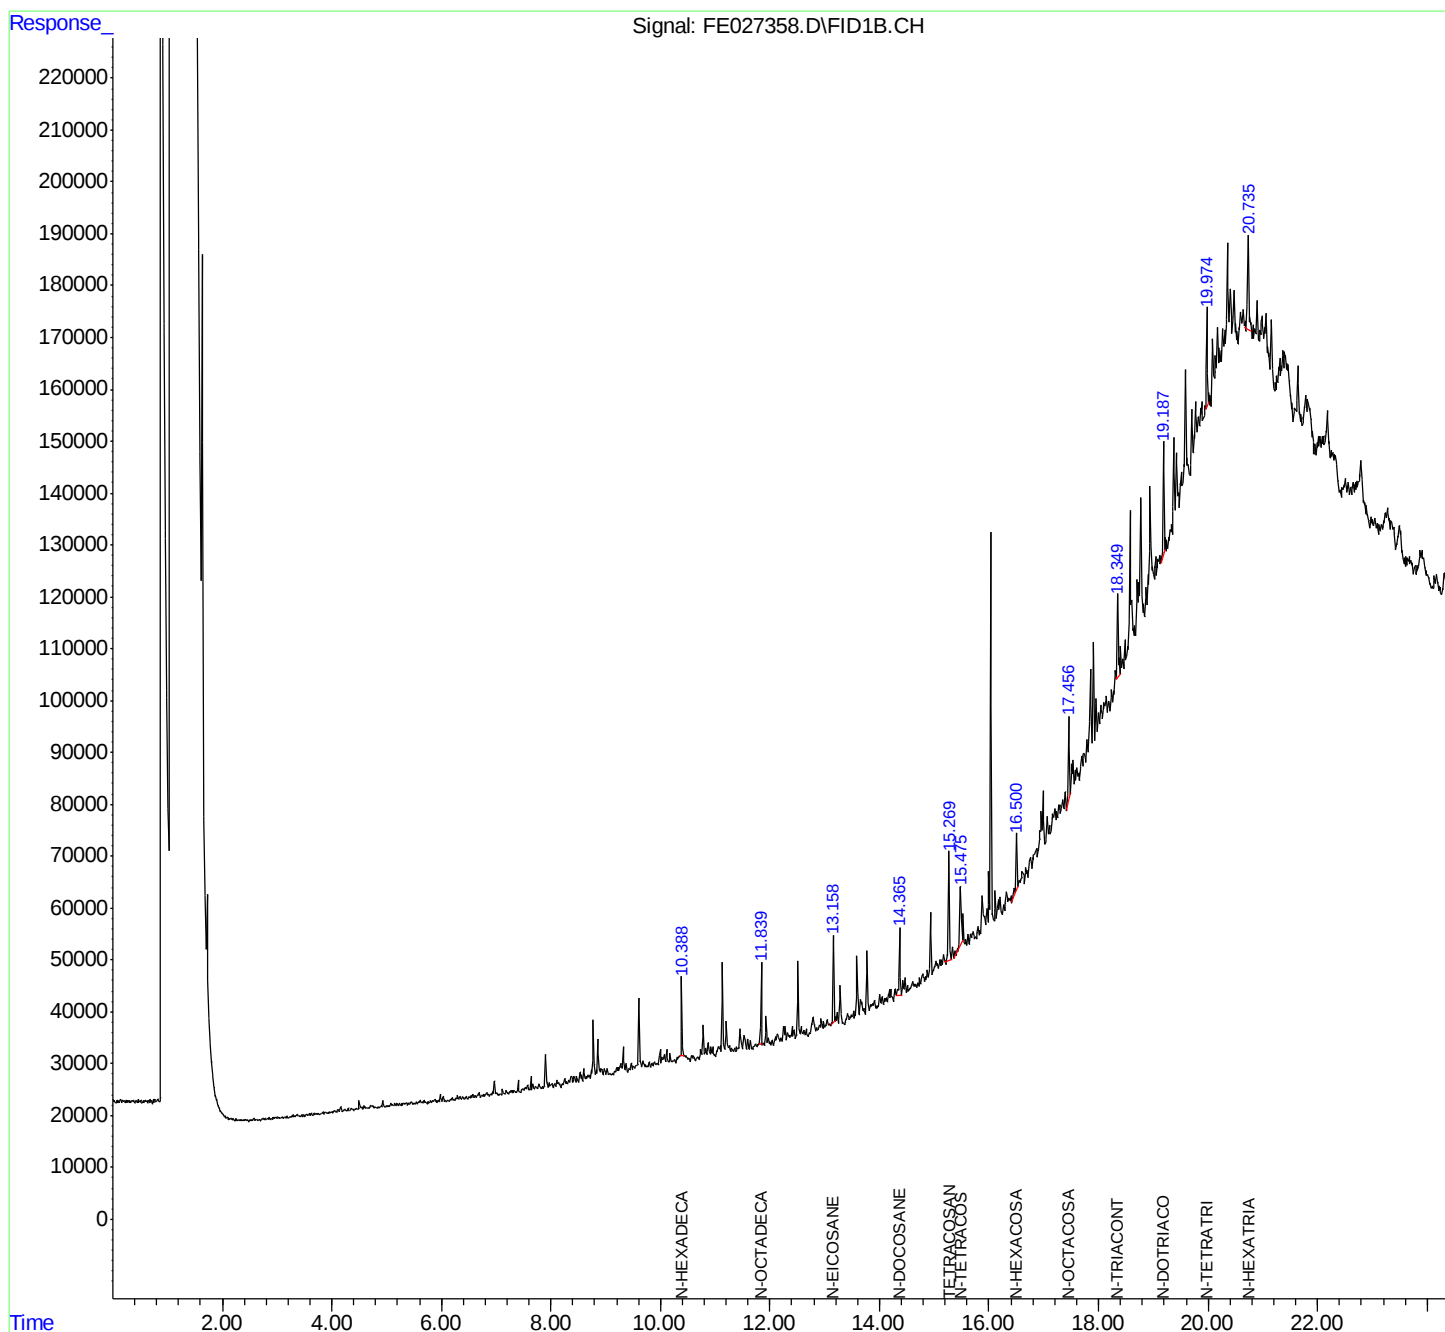


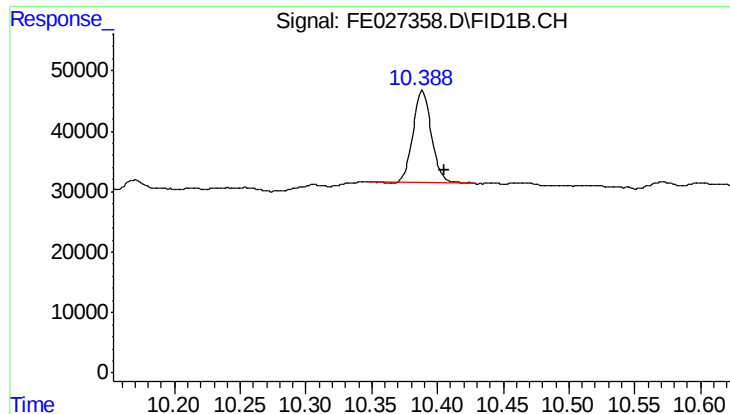

#5 N-HEXADECANE


R.T.: 10.389 min
Delta R.T.: -0.017 min
Response: 148236
Conc: 0.75 ug/ml

Instrument :
FID_E
ClientSampleId :

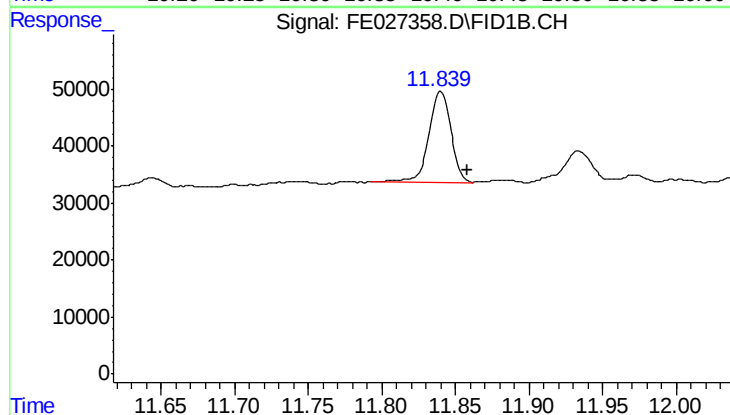


#6 N-OCTADECANE

R.T.: 11.840 min
Delta R.T.: -0.018 min
Response: 164020
Conc: 0.82 ug/ml

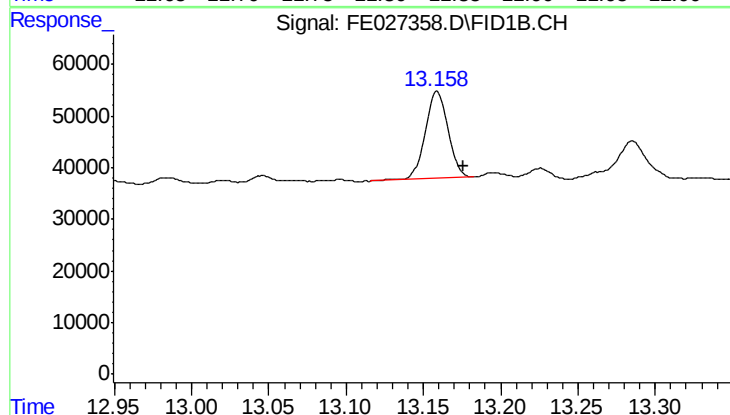


#7 N-EICOSANE

R.T.: 13.159 min
Delta R.T.: -0.018 min
Response: 169508
Conc: 0.89 ug/ml

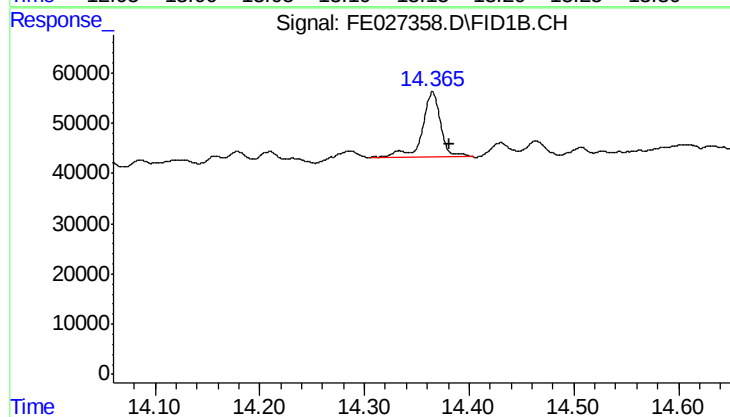

#8 N-DOCOSANE


R.T.: 14.365 min
Delta R.T.: -0.017 min
Response: 161812
Conc: 0.91 ug/ml

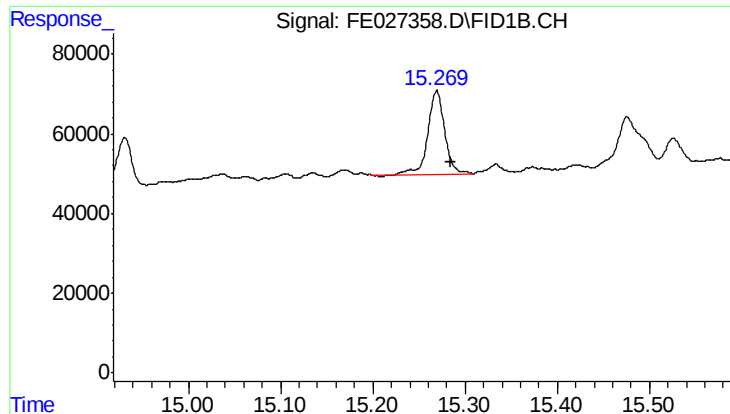

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.269 min
Delta R.T.: -0.015 min
Response: 266761
Conc: 1.81 ug/ml

Instrument :
FID_E
ClientSampleId :

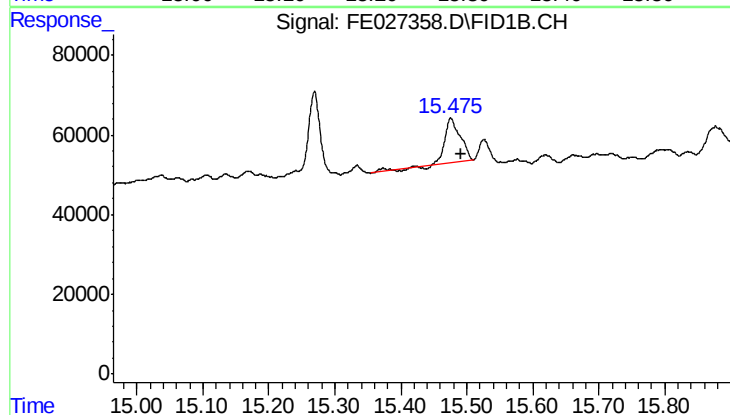


#10 N-TETRACOSANE

R.T.: 15.476 min
Delta R.T.: -0.015 min
Response: 181997
Conc: 1.08 ug/ml

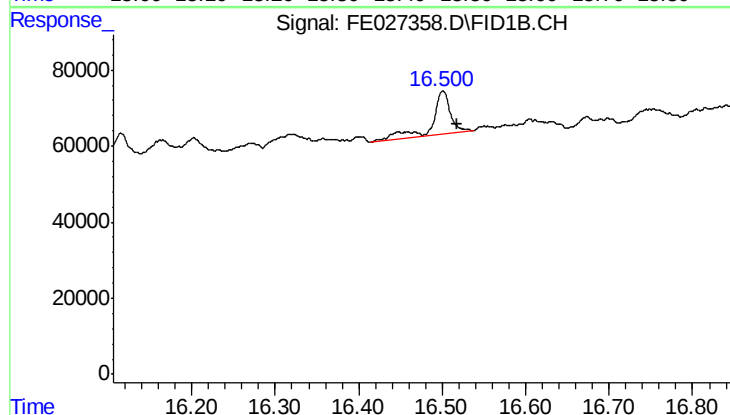


#11 N-HEXACOSANE

R.T.: 16.501 min
Delta R.T.: -0.017 min
Response: 173921
Conc: 1.05 ug/ml

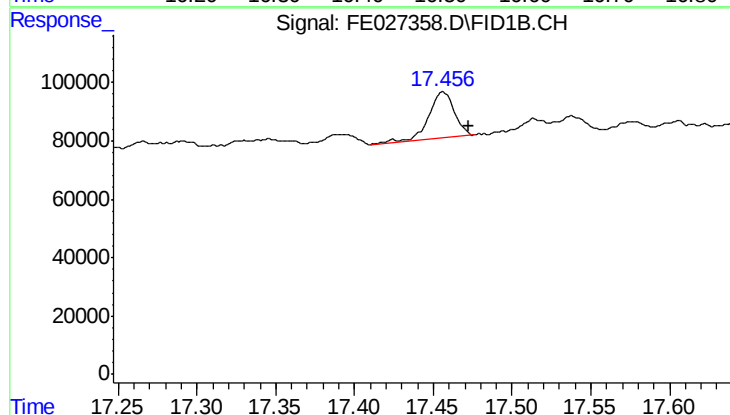

#12 N-OCTACOSANE


R.T.: 17.456 min
Delta R.T.: -0.016 min
Response: 173663
Conc: 1.05 ug/ml

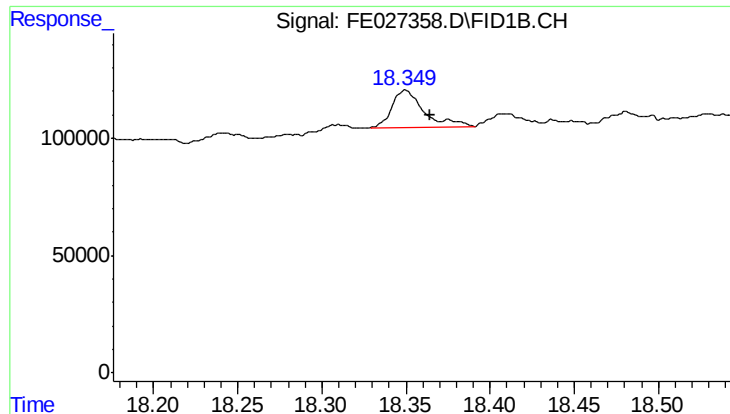

#13 N-TRIACONTANE


R.T.: 18.350 min
Delta R.T.: -0.014 min
Response: 214749
Conc: 1.28 ug/ml

Instrument :
FID_E
ClientSampleId :

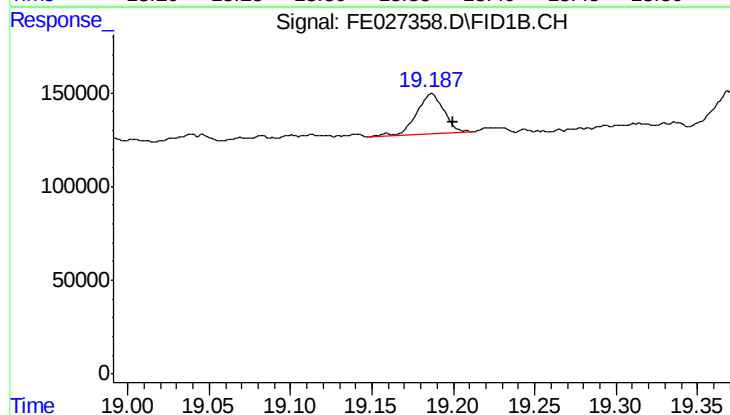


#14 N-DOTRIACONTANE

R.T.: 19.187 min
Delta R.T.: -0.013 min
Response: 250449
Conc: 1.46 ug/ml

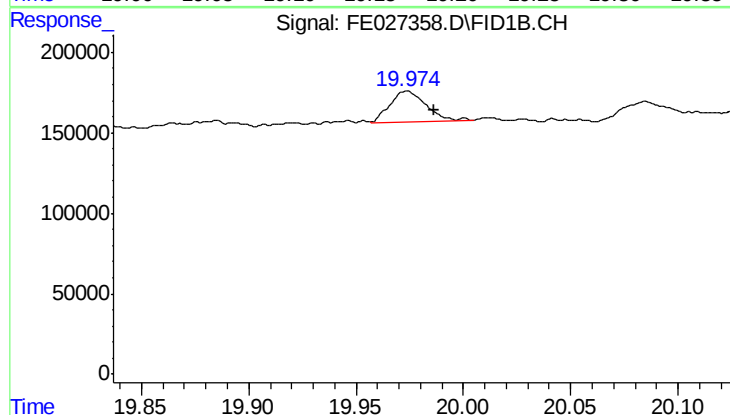

#15 N-TETRATRIACONTANE

R.T.: 19.974 min
Delta R.T.: -0.012 min
Response: 231716
Conc: 1.29 ug/ml

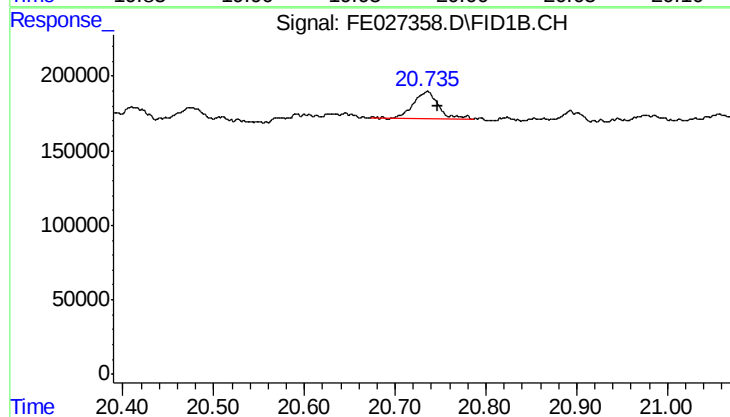

#16 N-HEXATRIACONTANE

R.T.: 20.736 min
Delta R.T.: -0.012 min
Response: 358054
Conc: 2.03 ug/ml