

Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
 Data File : FE027365.D
 Signal(s) : FID1B.CH
 Acq On : 18 May 2018 23:12
 Operator : UA/AJ
 Sample : J2963-09 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 238-COMP1-SL

Integration File: autoint1.e
 Quant Time: May 19 04:43:23 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.269	221187	1.502 ug/ml
Target Compounds			
7) N-EICOSANE	13.159	146815	0.771 ug/ml
10) N-TETRACOSANE	15.484	689523	4.094 ug/ml
12) N-OCTACOSANE	17.455	463398	2.804 ug/ml
13) N-TRIACONTANE	18.355	211060	1.255 ug/ml
14) N-DOTRIACONTANE	19.189	261361	1.521 ug/ml
15) N-TETRATRIACONTANE	19.977	183999	1.027 ug/ml
16) N-HEXATRIACONTANE	20.736	338650	1.925 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
Data File : FE027365.D
Signal(s) : FID1B.CH
Acq On : 18 May 2018 23:12
Operator : UA/AJ
Sample : J2963-09 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
238-COMP1-SL

Integration File: autoint1.e
Quant Time: May 19 04:43:23 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

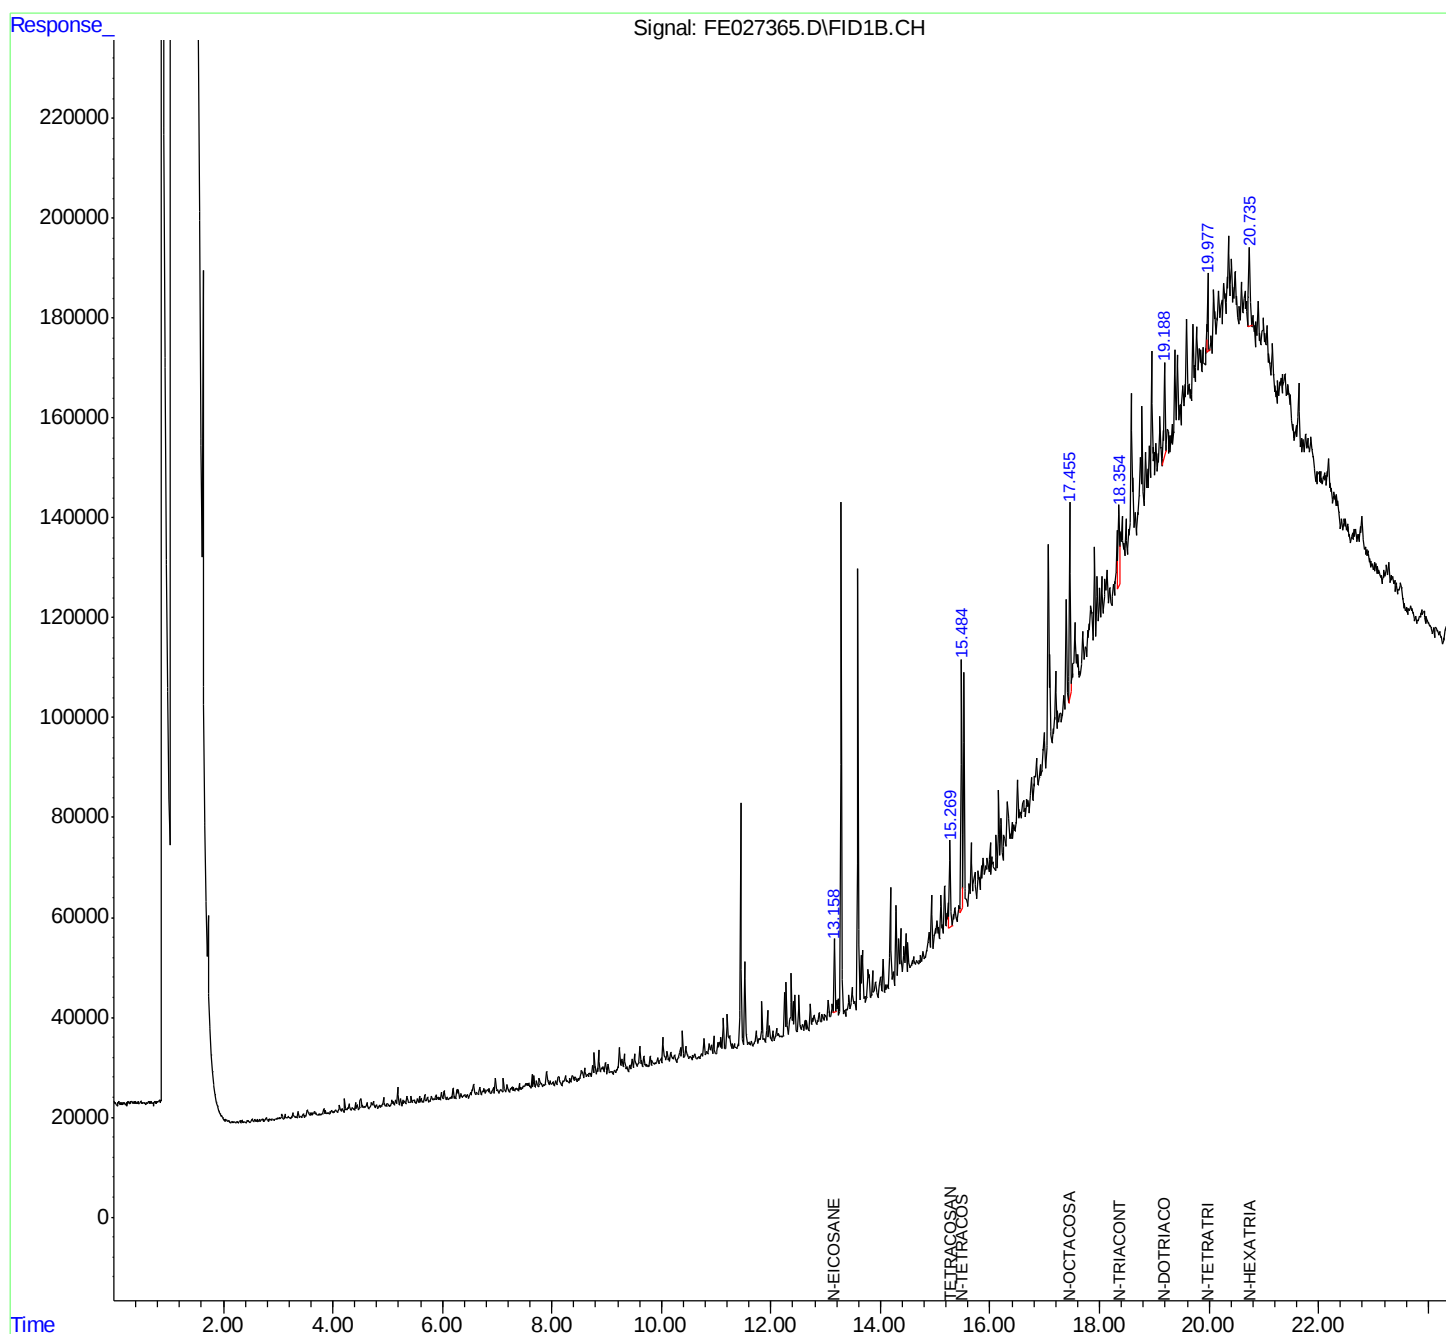


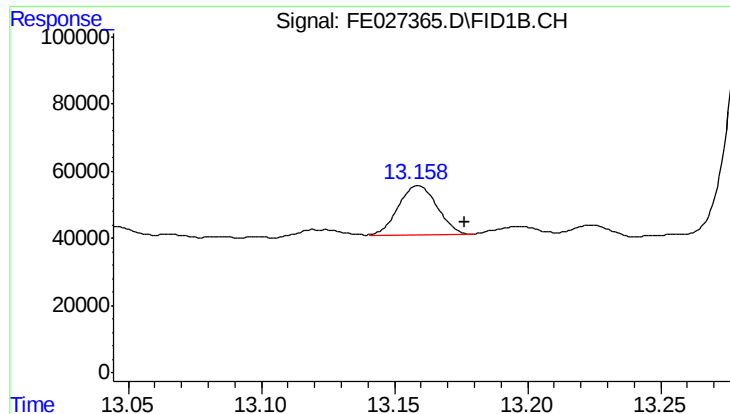

#7 N-EICOSANE


R.T.: 13.159 min
Delta R.T.: -0.017 min
Response: 146815
Conc: 0.77 ug/ml

Instrument :
FID_E
ClientSampleId :
238-COMP1-SL

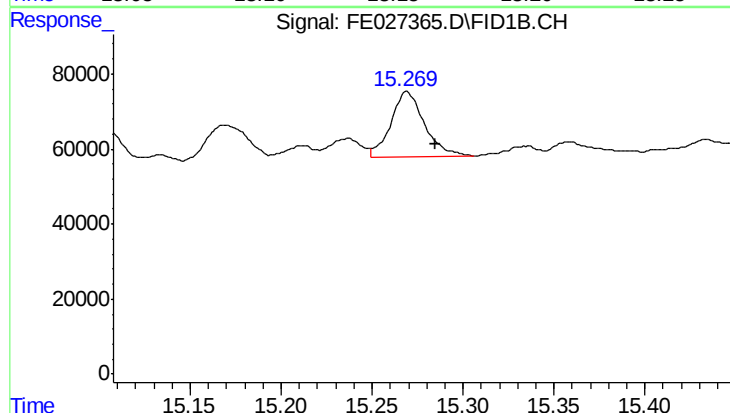


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.269 min
Delta R.T.: -0.015 min
Response: 221187
Conc: 1.50 ug/ml

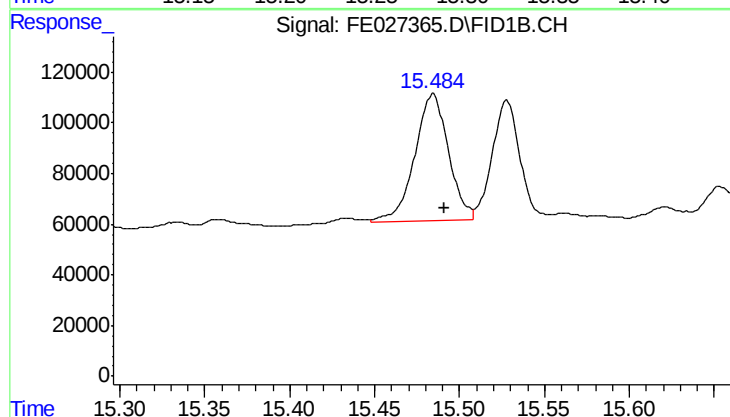


#10 N-TETRACOSANE

R.T.: 15.484 min
Delta R.T.: -0.007 min
Response: 689523
Conc: 4.09 ug/ml

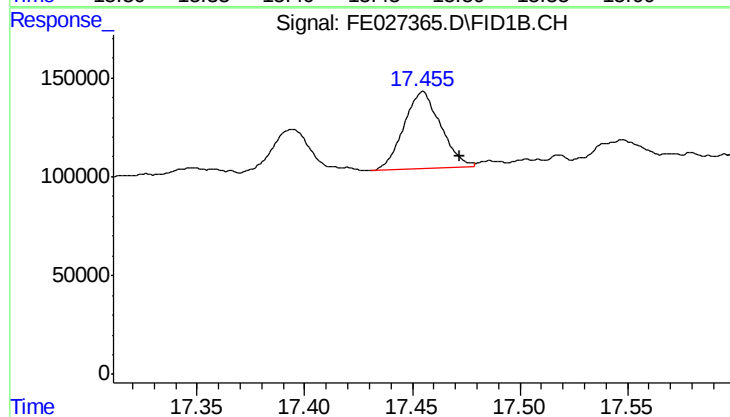

#12 N-OCTACOSANE


R.T.: 17.455 min
Delta R.T.: -0.017 min
Response: 463398
Conc: 2.80 ug/ml

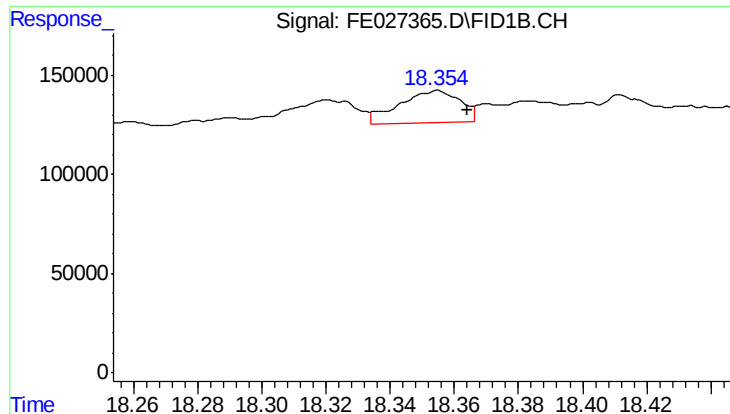

#13 N-TRIACONTANE


R.T.: 18.355 min
Delta R.T.: -0.009 min
Response: 211060
Conc: 1.25 ug/ml

Instrument :
FID_E
ClientSampleId :
238-COMP1-SL

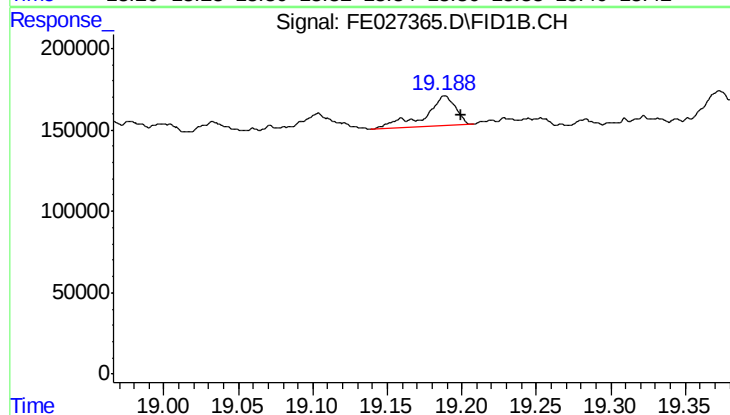


#14 N-DOTRIACONTANE

R.T.: 19.189 min
Delta R.T.: -0.011 min
Response: 261361
Conc: 1.52 ug/ml

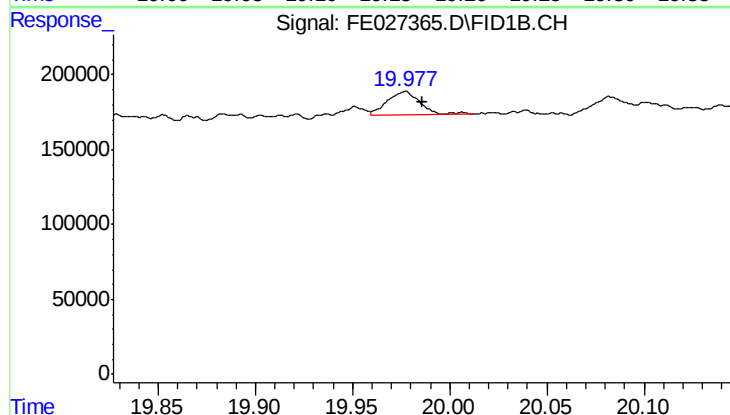

#15 N-TETRATRIACONTANE

R.T.: 19.977 min
Delta R.T.: -0.009 min
Response: 183999
Conc: 1.03 ug/ml

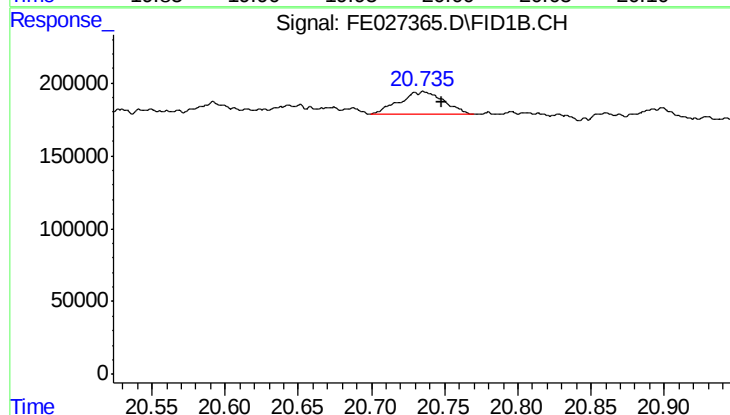

#16 N-HEXATRIACONTANE

R.T.: 20.736 min
Delta R.T.: -0.012 min
Response: 338650
Conc: 1.92 ug/ml