

Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
 Data File : FE027368.D
 Signal(s) : FID1B.CH
 Acq On : 19 May 2018 00:54
 Operator : UA/AJ
 Sample : J2965-01 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 256-COMP1-SL

Integration File: autoint1.e
 Quant Time: May 19 04:43:57 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.269	369272	2.508 ug/ml
Target Compounds			
7) N-EICOSANE	13.159	154460	0.811 ug/ml
10) N-TETRACOSANE	15.482	497862	2.956 ug/ml
12) N-OCTACOSANE	17.455	335358	2.029 ug/ml
13) N-TRIACONTANE	18.353	139627	0.830 ug/ml
14) N-DOTRIACONTANE	19.189	256696	1.494 ug/ml
15) N-TETRATRIACONTANE	19.977	212967	1.188 ug/ml
16) N-HEXATRIACONTANE	20.735	275400	1.565 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
Data File : FE027368.D
Signal(s) : FID1B.CH
Acq On : 19 May 2018 00:54
Operator : UA/AJ
Sample : J2965-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
256-COMP1-SL

Integration File: autoint1.e
Quant Time: May 19 04:43:57 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

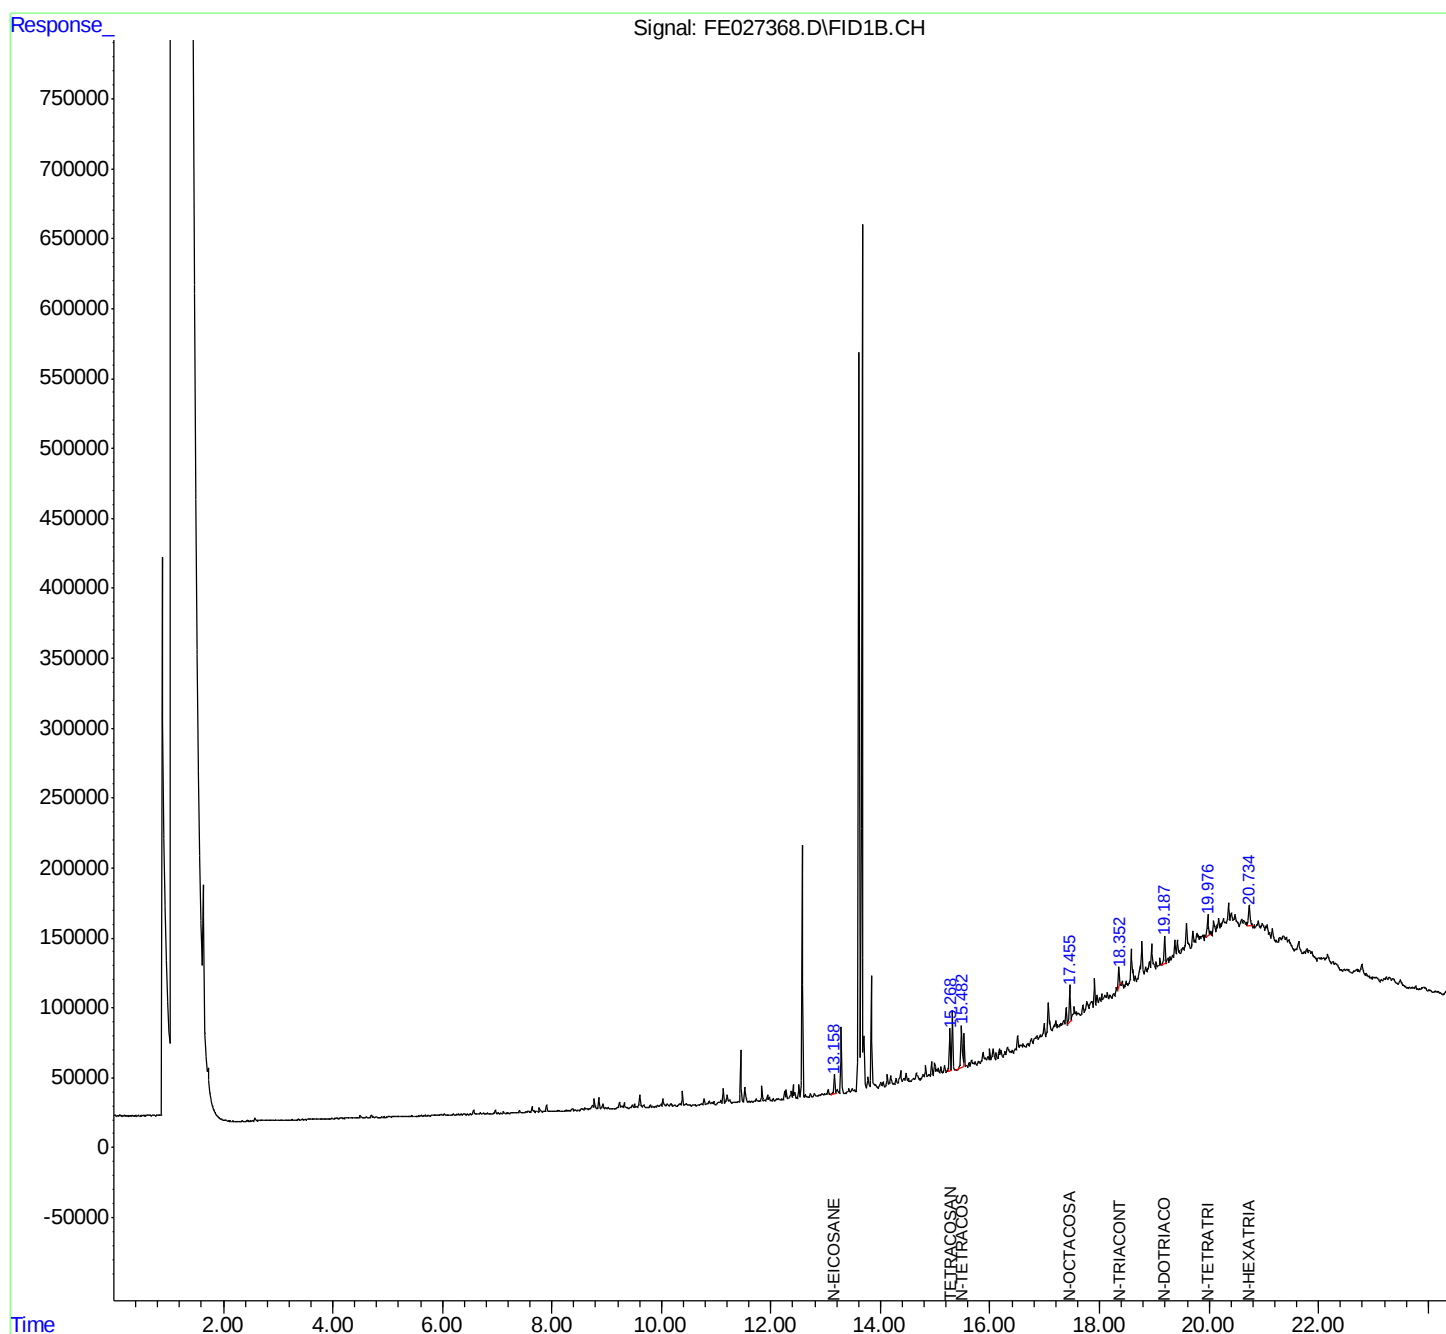


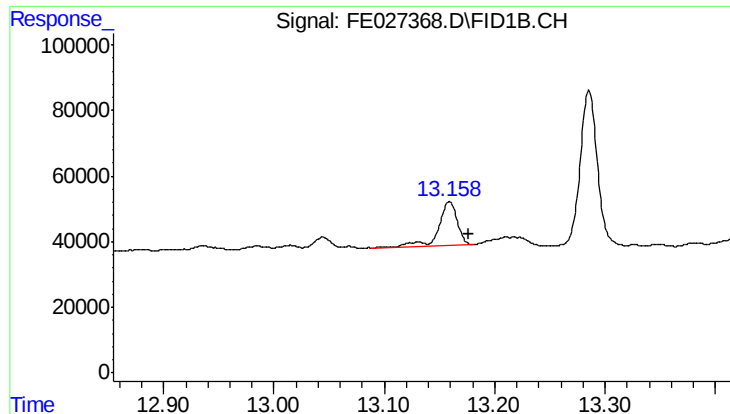

#7 N-EICOSANE


R.T.: 13.159 min
Delta R.T.: -0.017 min
Response: 154460
Conc: 0.81 ug/ml

Instrument :
FID_E
ClientSampleId :
256-COMP1-SL

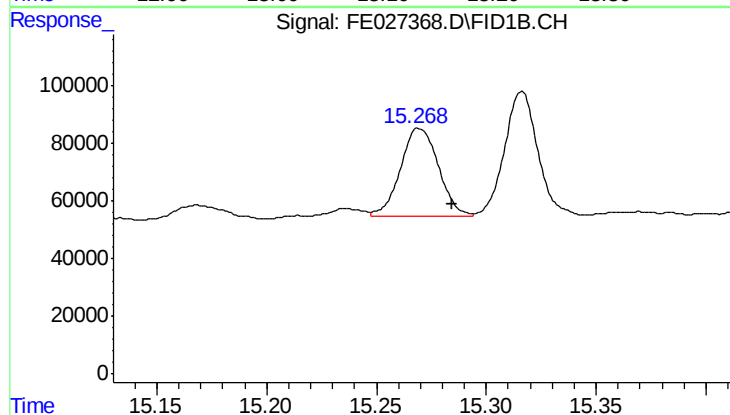


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.269 min
Delta R.T.: -0.015 min
Response: 369272
Conc: 2.51 ug/ml

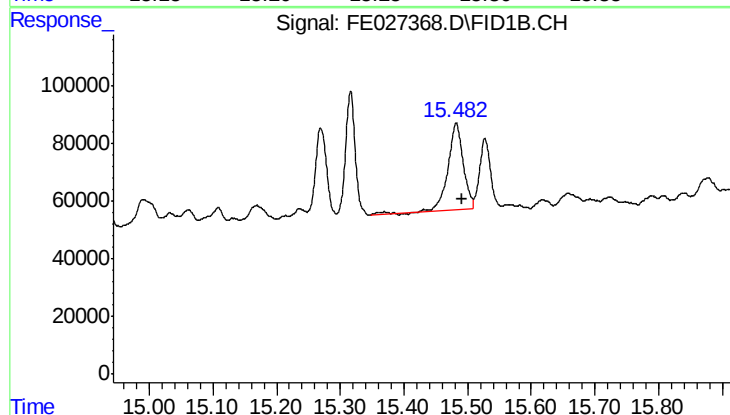


#10 N-TETRACOSANE

R.T.: 15.482 min
Delta R.T.: -0.009 min
Response: 497862
Conc: 2.96 ug/ml

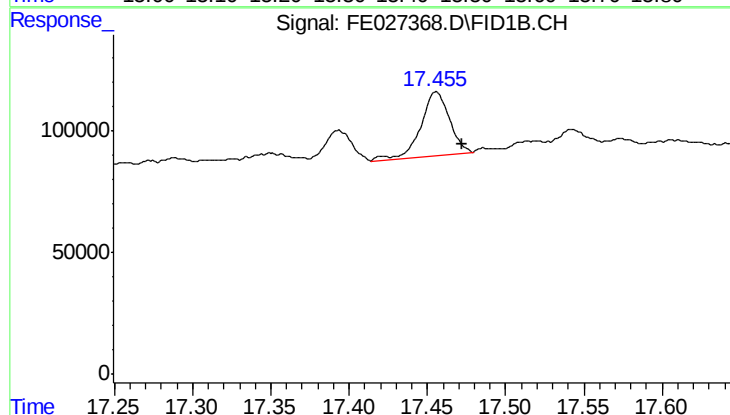

#12 N-OCTACOSANE


R.T.: 17.455 min
Delta R.T.: -0.017 min
Response: 335358
Conc: 2.03 ug/ml

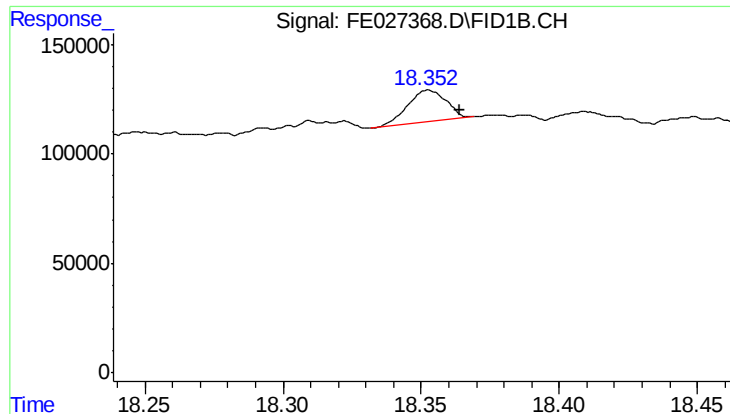

#13 N-TRIACONTANE


R.T.: 18.353 min
Delta R.T.: -0.011 min
Response: 139627
Conc: 0.83 ug/ml

Instrument :
FID_E
ClientSampleId :
256-COMP1-SL

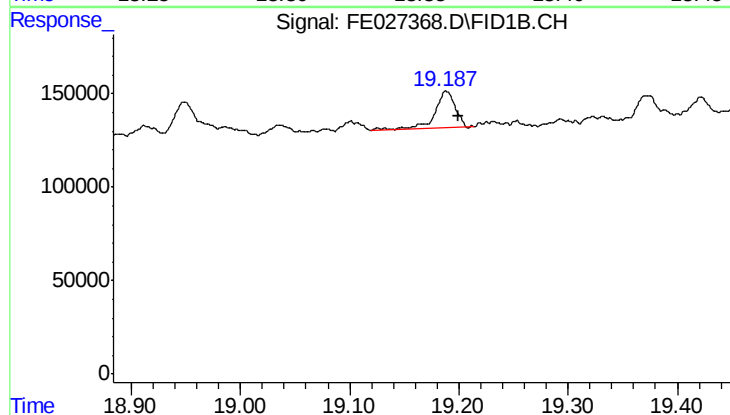


#14 N-DOTRIACONTANE

R.T.: 19.189 min
Delta R.T.: -0.011 min
Response: 256696
Conc: 1.49 ug/ml

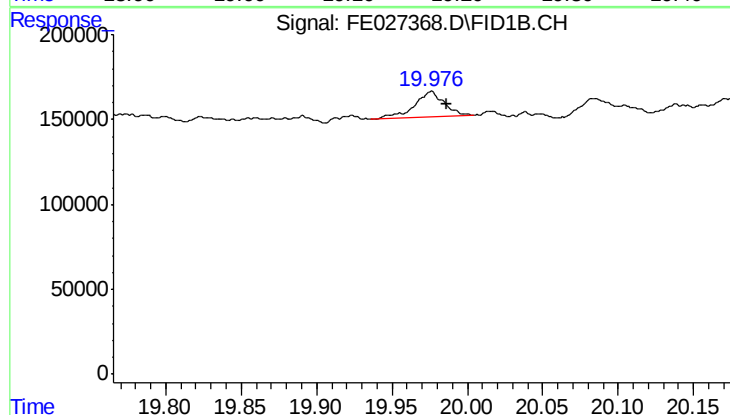

#15 N-TETRATRIACONTANE

R.T.: 19.977 min
Delta R.T.: -0.010 min
Response: 212967
Conc: 1.19 ug/ml

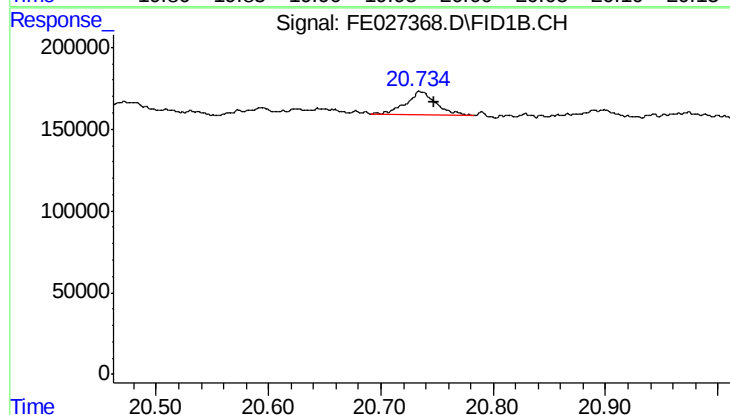

#16 N-HEXATRIACONTANE

R.T.: 20.735 min
Delta R.T.: -0.013 min
Response: 275400
Conc: 1.57 ug/ml