

Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
 Data File : FE027334.D
 Signal(s) : FID1B.CH
 Acq On : 18 May 2018 5:14
 Operator : UA/AJ
 Sample : J2950-01MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 EPE-MX-3(0-5)MS

Integration File: Sample.e
 Quant Time: May 18 08:20:33 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.274	2585617	17.560 ug/ml
Target Compounds			
2) N-DECANE	4.929	2310177	14.182 ug/ml
3) N-DODECANE	6.970	2725070	15.676 ug/ml
4) N-TETRADECANE	8.781	3050958	16.143 ug/ml
5) N-HEXADECANE	10.393	3190416	16.227 ug/ml
6) N-OCTADECANE	11.845	3169067	15.782 ug/ml
7) N-EICOSANE	13.164	3167123	16.631 ug/ml
8) N-DOCOSANE	14.370	3063841	17.176 ug/ml
10) N-TETRACOSANE	15.481	2965420	17.607 ug/ml
11) N-HEXACOSANE	16.507	2864730	17.342 ug/ml
12) N-OCTACOSANE	17.462	2941811	17.802 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE051818\
Data File : FE027334.D
Signal(s) : FID1B.CH
Acq On : 18 May 2018 5:14
Operator : UA/AJ
Sample : J2950-01MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
EPE-MX-3(0-5)MS

Integration File: Sample.e
Quant Time: May 18 08:20:33 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

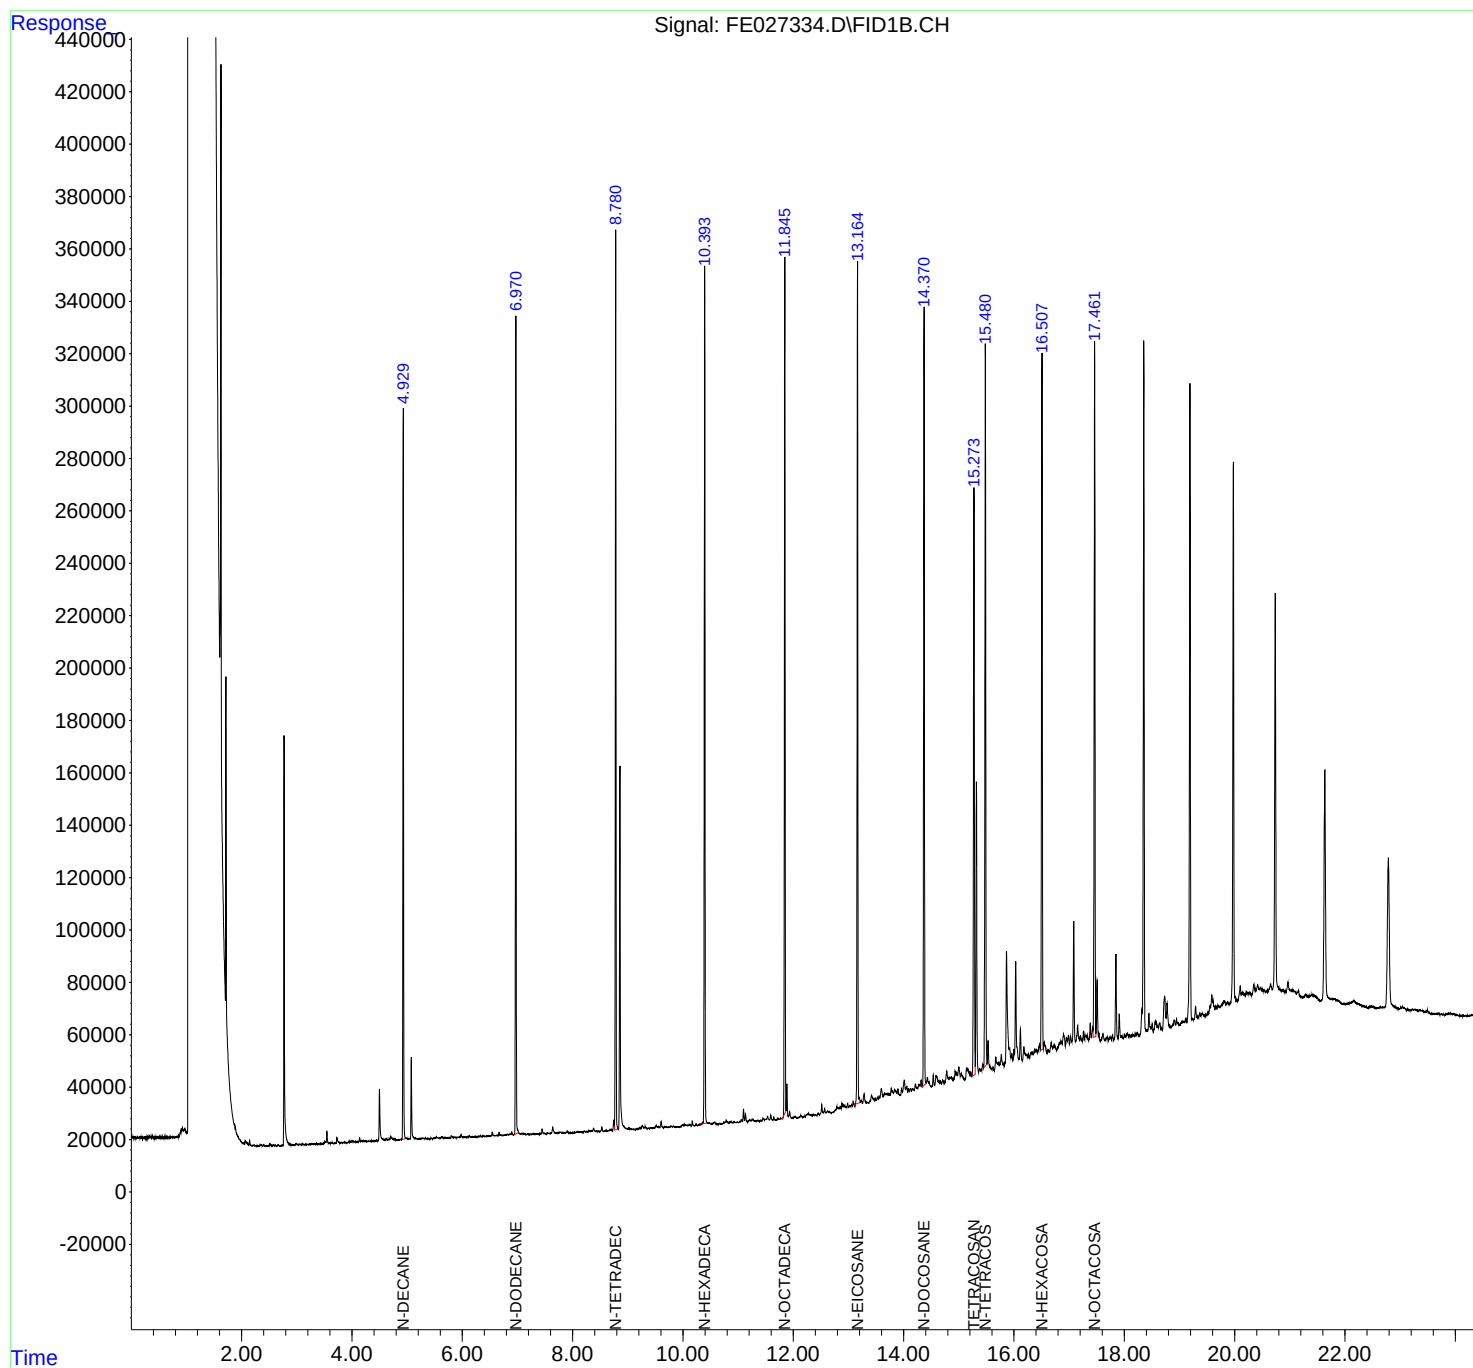


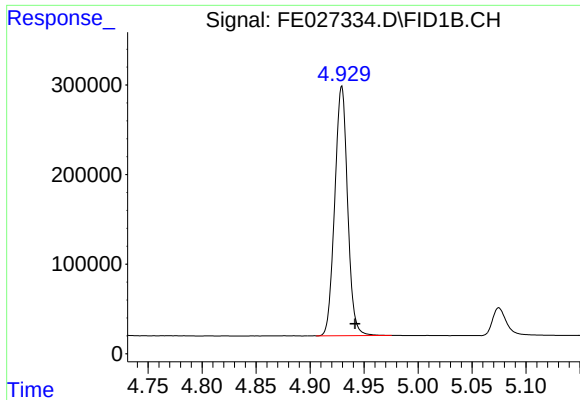

#2 N-DECANE


R.T.: 4.929 min
Delta R.T.: -0.012 min
Response: 2310177
Conc: 14.18 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-MX-3(0-5)MS

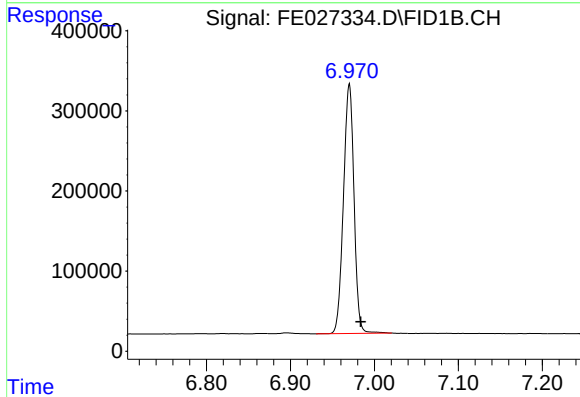


#3 N-DODECANE

R.T.: 6.970 min
Delta R.T.: -0.013 min
Response: 2725070
Conc: 15.68 ug/ml

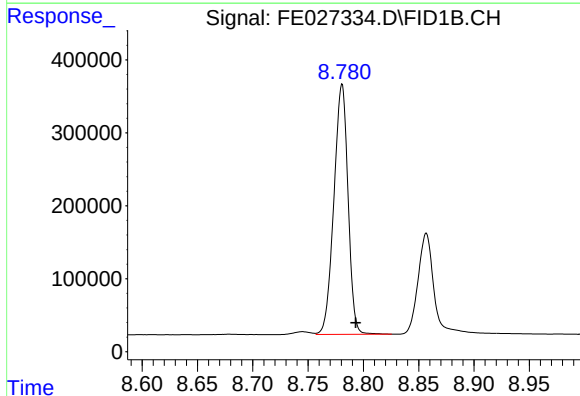


#4 N-TETRADECANE

R.T.: 8.781 min
Delta R.T.: -0.013 min
Response: 3050958
Conc: 16.14 ug/ml

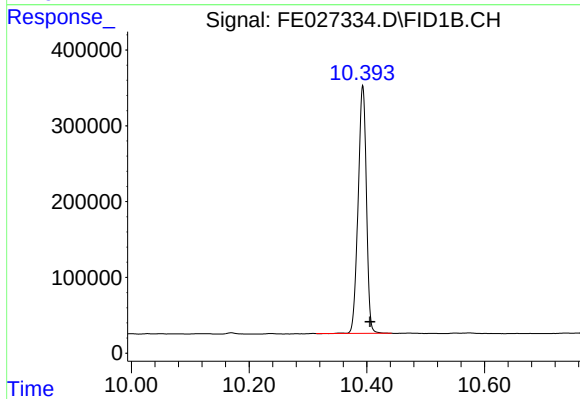

#5 N-HEXADECANE


R.T.: 10.393 min
Delta R.T.: -0.012 min
Response: 3190416
Conc: 16.23 ug/ml

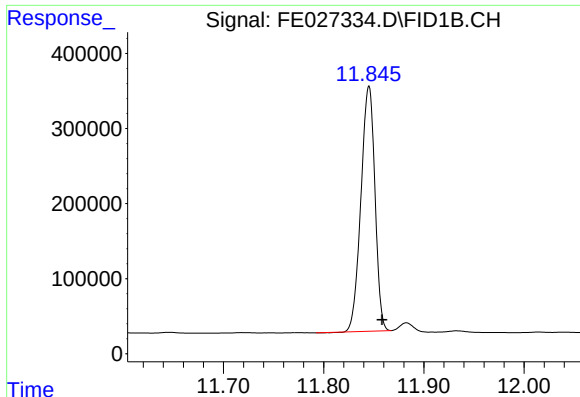

#6 N-OCTADECANE


R.T.: 11.845 min
Delta R.T.: -0.013 min
Response: 3169067
Conc: 15.78 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-MX-3(0-5)MS

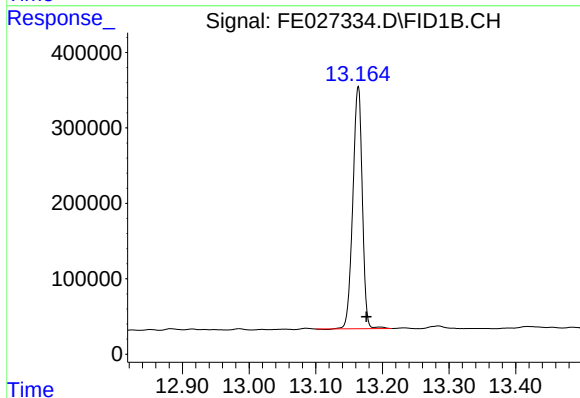


#7 N-EICOSANE

R.T.: 13.164 min
Delta R.T.: -0.012 min
Response: 3167123
Conc: 16.63 ug/ml

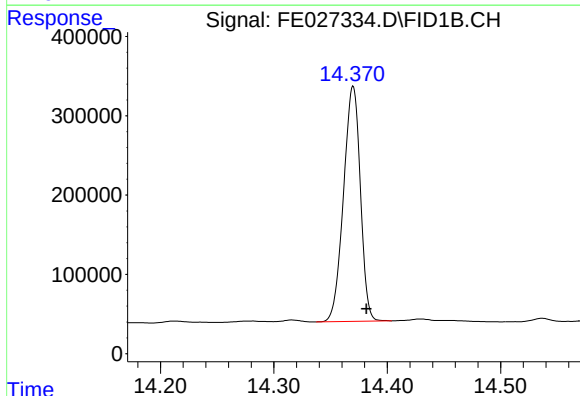


#8 N-DOCOSANE

R.T.: 14.370 min
Delta R.T.: -0.012 min
Response: 3063841
Conc: 17.18 ug/ml

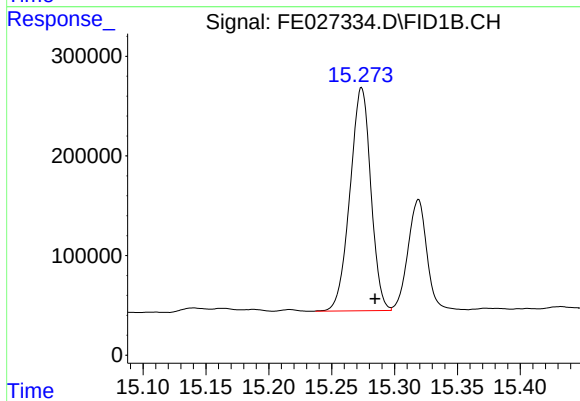

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.274 min
Delta R.T.: -0.011 min
Response: 2585617
Conc: 17.56 ug/ml

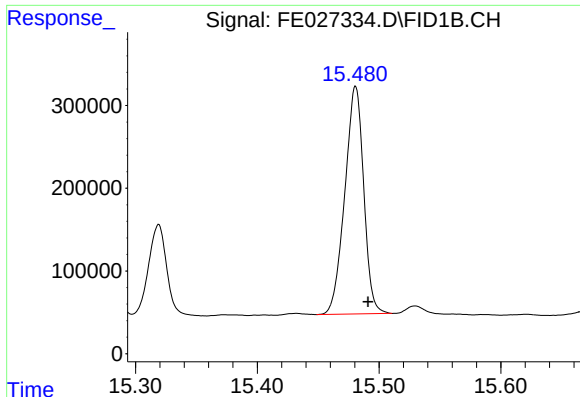

#10 N-TETRACOSANE


R.T.: 15.481 min
Delta R.T.: -0.010 min
Response: 2965420
Conc: 17.61 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-MX-3(0-5)MS

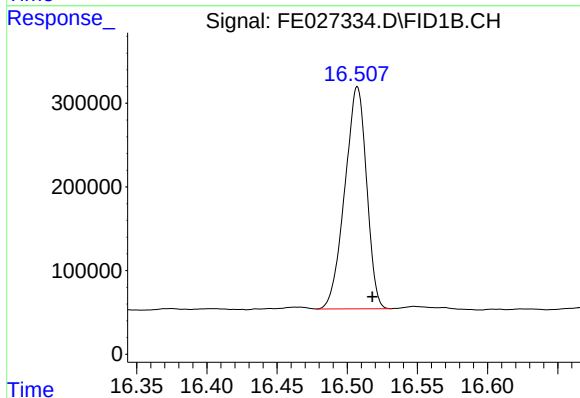

#11 N-HEXACOSANE

R.T.: 16.507 min
Delta R.T.: -0.011 min
Response: 2864730
Conc: 17.34 ug/ml

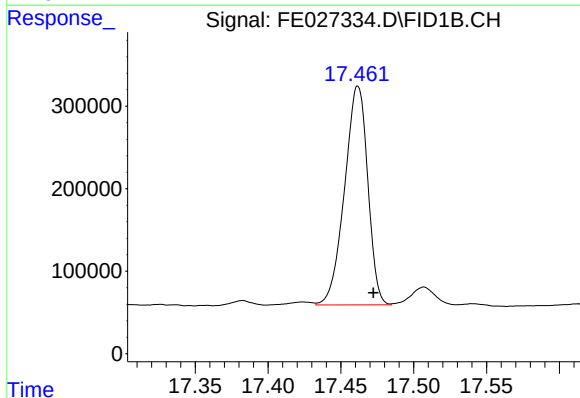

#12 N-OCTACOSANE

R.T.: 17.462 min
Delta R.T.: -0.010 min
Response: 2941811
Conc: 17.80 ug/ml