

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051923AL\  
 Data File : FE041983.D  
 Signal(s) : FID1B.ch  
 Acq On : 18 May 2023 09:26  
 Operator : YP\AJ  
 Sample : 02810-01DL 5X  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 OR-02-051623DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 05/19/2023  
 Supervised By :Ankita Jodhani 05/19/2023

Integration File: autoint1.e  
 Quant Time: May 19 01:40:18 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 051823.M  
 Quant Title : GC Extractables  
 QLast Update : Thu May 18 06:27:12 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.964 | 932305     | 5.280 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 10.56%       |
| 12) S 1-chlorooctadecane (S... | 13.401 | 855966     | 6.442 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 12.88%       |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE051923AL\  
Data File : FE041983.D  
Signal(s) : FID1B.ch  
Acq On : 18 May 2023 09:26  
Operator : YP\AJ  
Sample : 02810-01DL 5X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

## Instrument :

FID\_E

## Client Sample Id :

OR-02-051623DL

## Manual Integrations

## APPROVED

Reviewed By :Yogesh Patel 05/19/2023

Supervised By :Ankita Jodhani 05/19/2023

Integration File: autoint1.e

Quant Time: May 19 01:40:18 2023

Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 051823.

Quant Title : GC Extractables

QLast Update : Thu May 18 06:27:12 2023


Response via : Initial Calibration


Integrator: ChemStation

Volume Inj. : 1 ul

Signal Phase : Rxi-1ms

Signal Info : 20M x 0.18mm x 0.18um

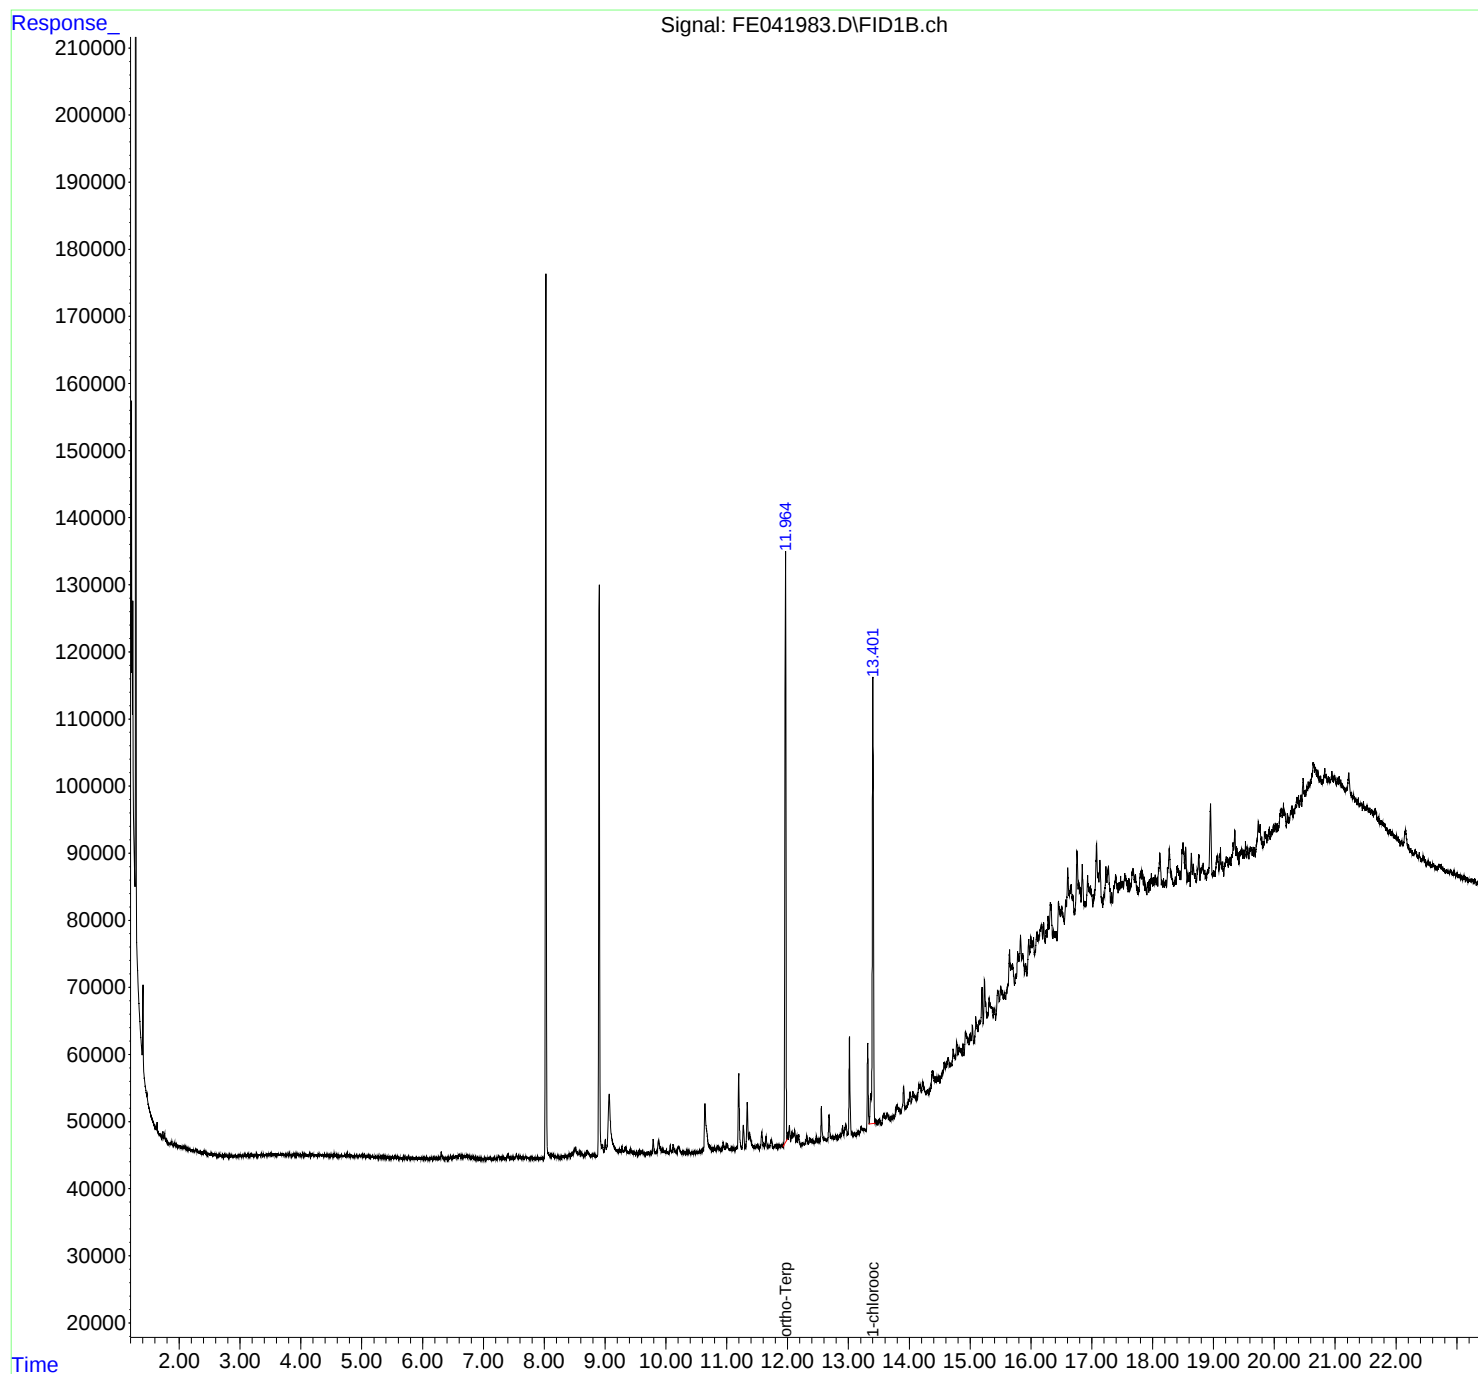

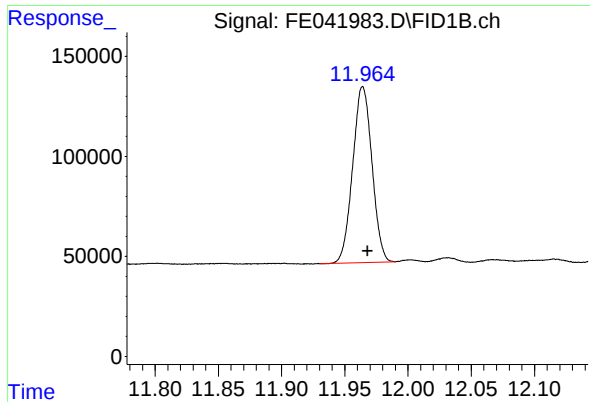


#9 ortho-Terphenyl (SURR)

R.T.: 11.964 min  
Delta R.T.: -0.004 min  
Response: 932305  
Conc: 5.28 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
OR-02-051623DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 05/19/2023  
Supervised By :Ankita Jodhani 05/19/2023

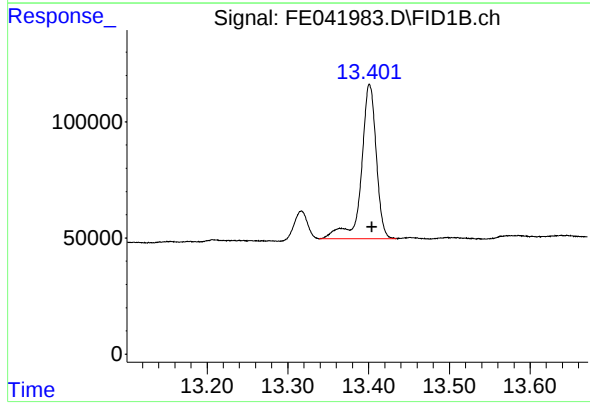

#12 1-chlorooctadecane (SURR)

R.T.: 13.401 min  
Delta R.T.: -0.003 min  
Response: 855966  
Conc: 6.44 ug/ml m