

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052124AL\
Data File : FE048315.D
Signal(s) : FID1B.ch
Acq On : 21 May 2024 20:08
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 22 02:27:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042724.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 03:29:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.710	195086	1.432 ug/ml
21) T	n-Octatriacontane (C38)	21.146f	27740	0.201 ug/ml
22) T	n-Tetracontane (C40)	22.082	133932	0.961 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052124AL\
Data File : FE048315.D
Signal(s) : FID1B.ch
Acq On : 21 May 2024 20:08
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 22 02:27:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042724.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 03:29:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

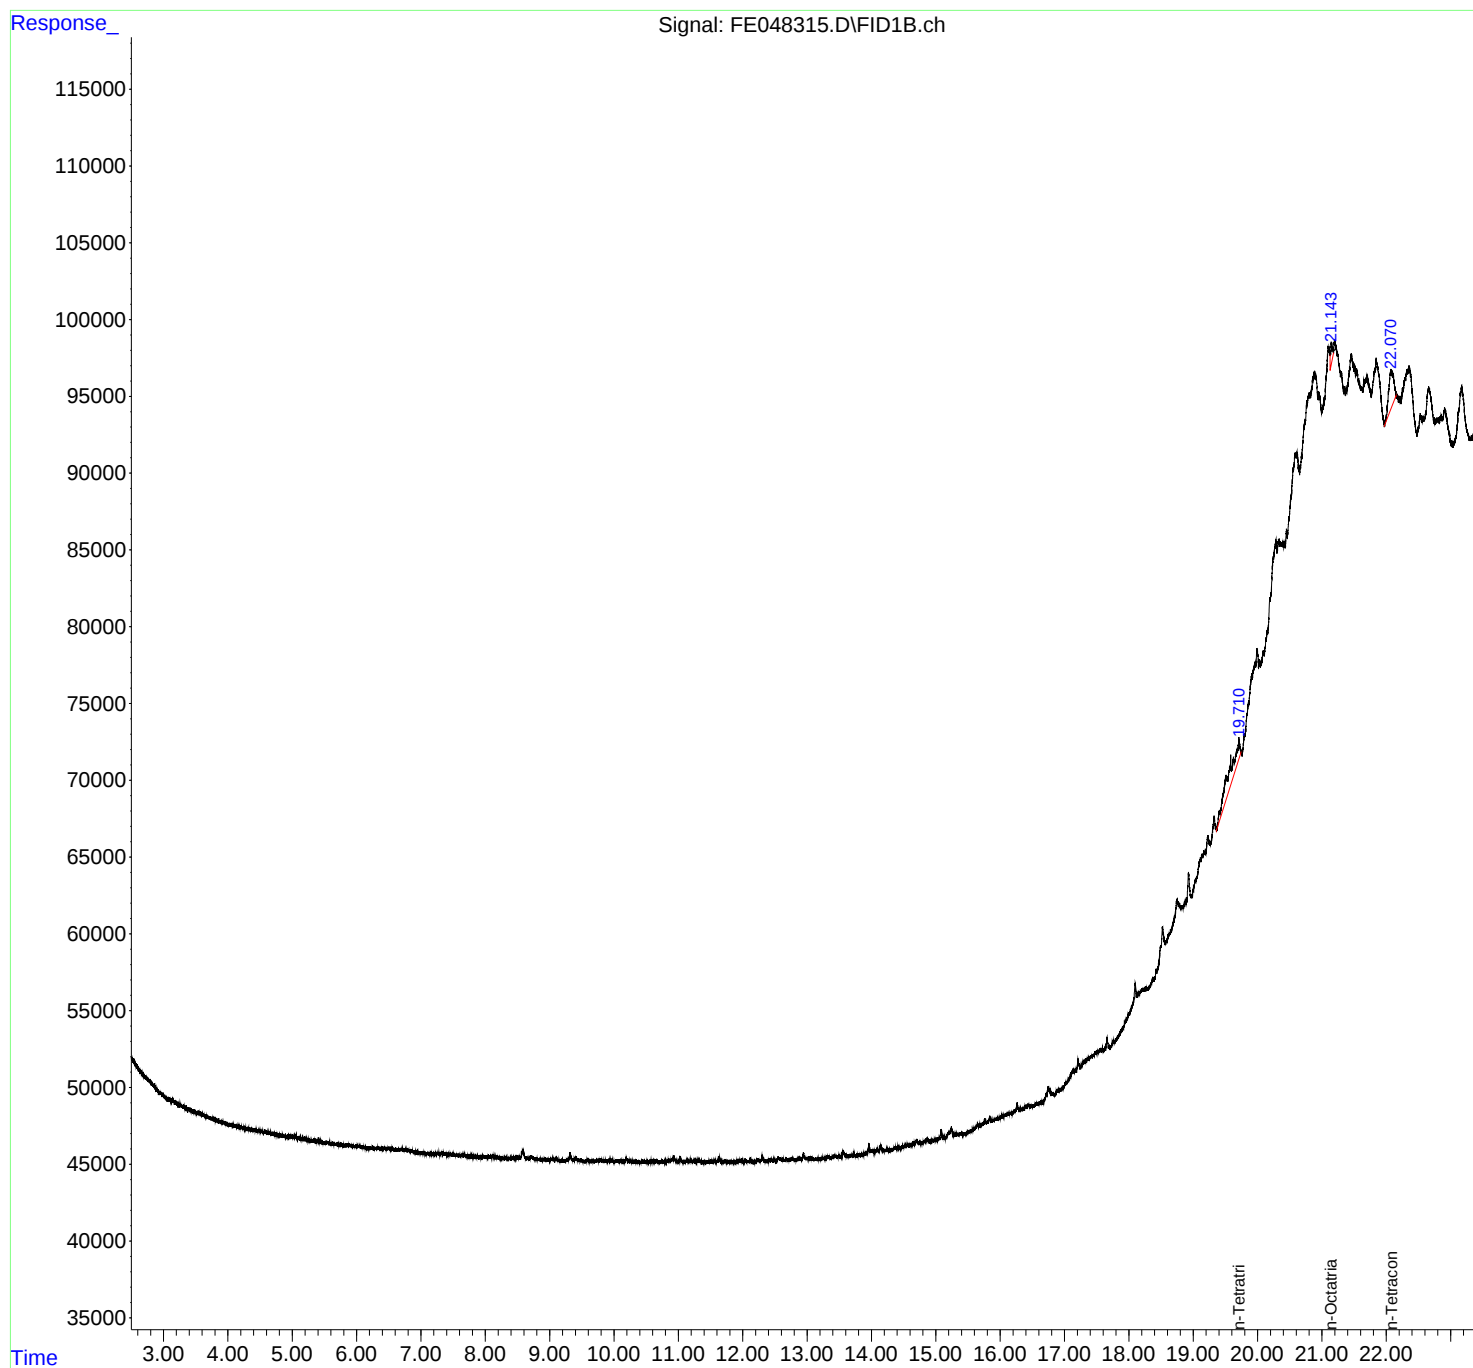


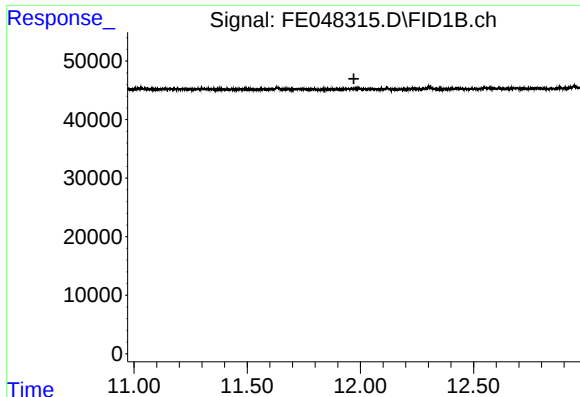

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.971 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

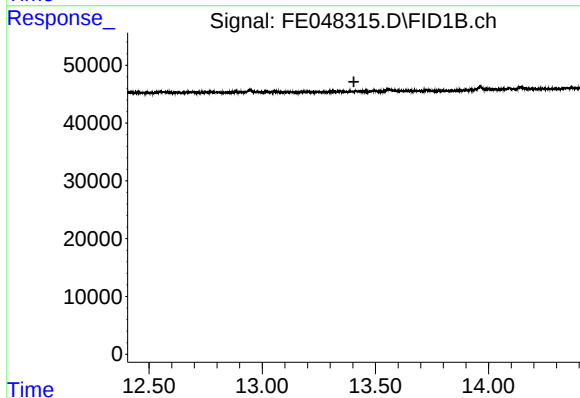


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.405 min
Response: 0
Conc: N.D.

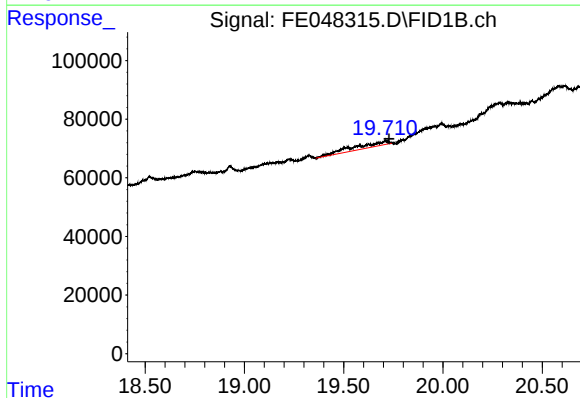


#19 n-Tetratriacontane (C34)

R.T.: 19.710 min
Delta R.T.: -0.017 min
Response: 195086
Conc: 1.43 ug/ml

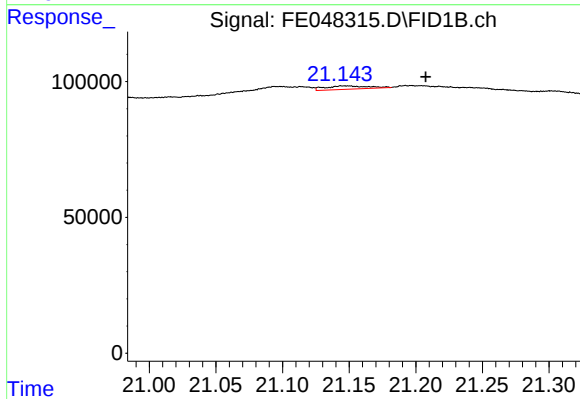

#21 n-Octatriacontane (C38)

R.T.: 21.146 min
Delta R.T.: -0.062 min
Response: 27740
Conc: 0.20 ug/ml

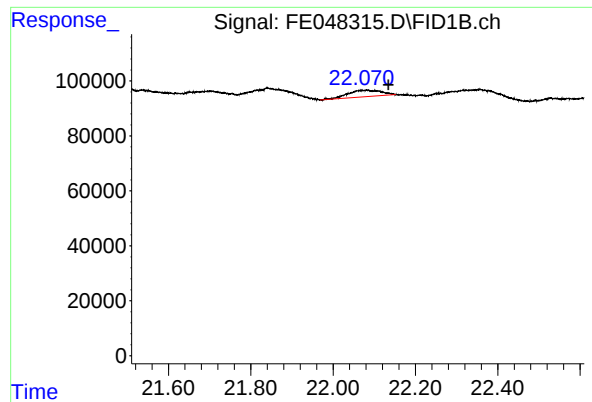

#22 n-Tetracontane (C40)

R.T.: 22.082 min
Delta R.T.: -0.053 min
Response: 133932
Conc: 0.96 ug/ml

Instrument :

FID_E

ClientSampleId :