

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052224AL\
Data File : FE048337.D
Signal(s) : FID1B.ch
Acq On : 22 May 2024 21:26
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 23 01:38:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042724.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 03:29:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.625f	13797	0.104 ug/ml
18) T	n-Dotriacontane (C32)	18.934	44938	0.325 ug/ml
20) T	n-Hexatriacontane (C36)	20.496	79765	0.589 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052224AL\
Data File : FE048337.D
Signal(s) : FID1B.ch
Acq On : 22 May 2024 21:26
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 23 01:38:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042724.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 03:29:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

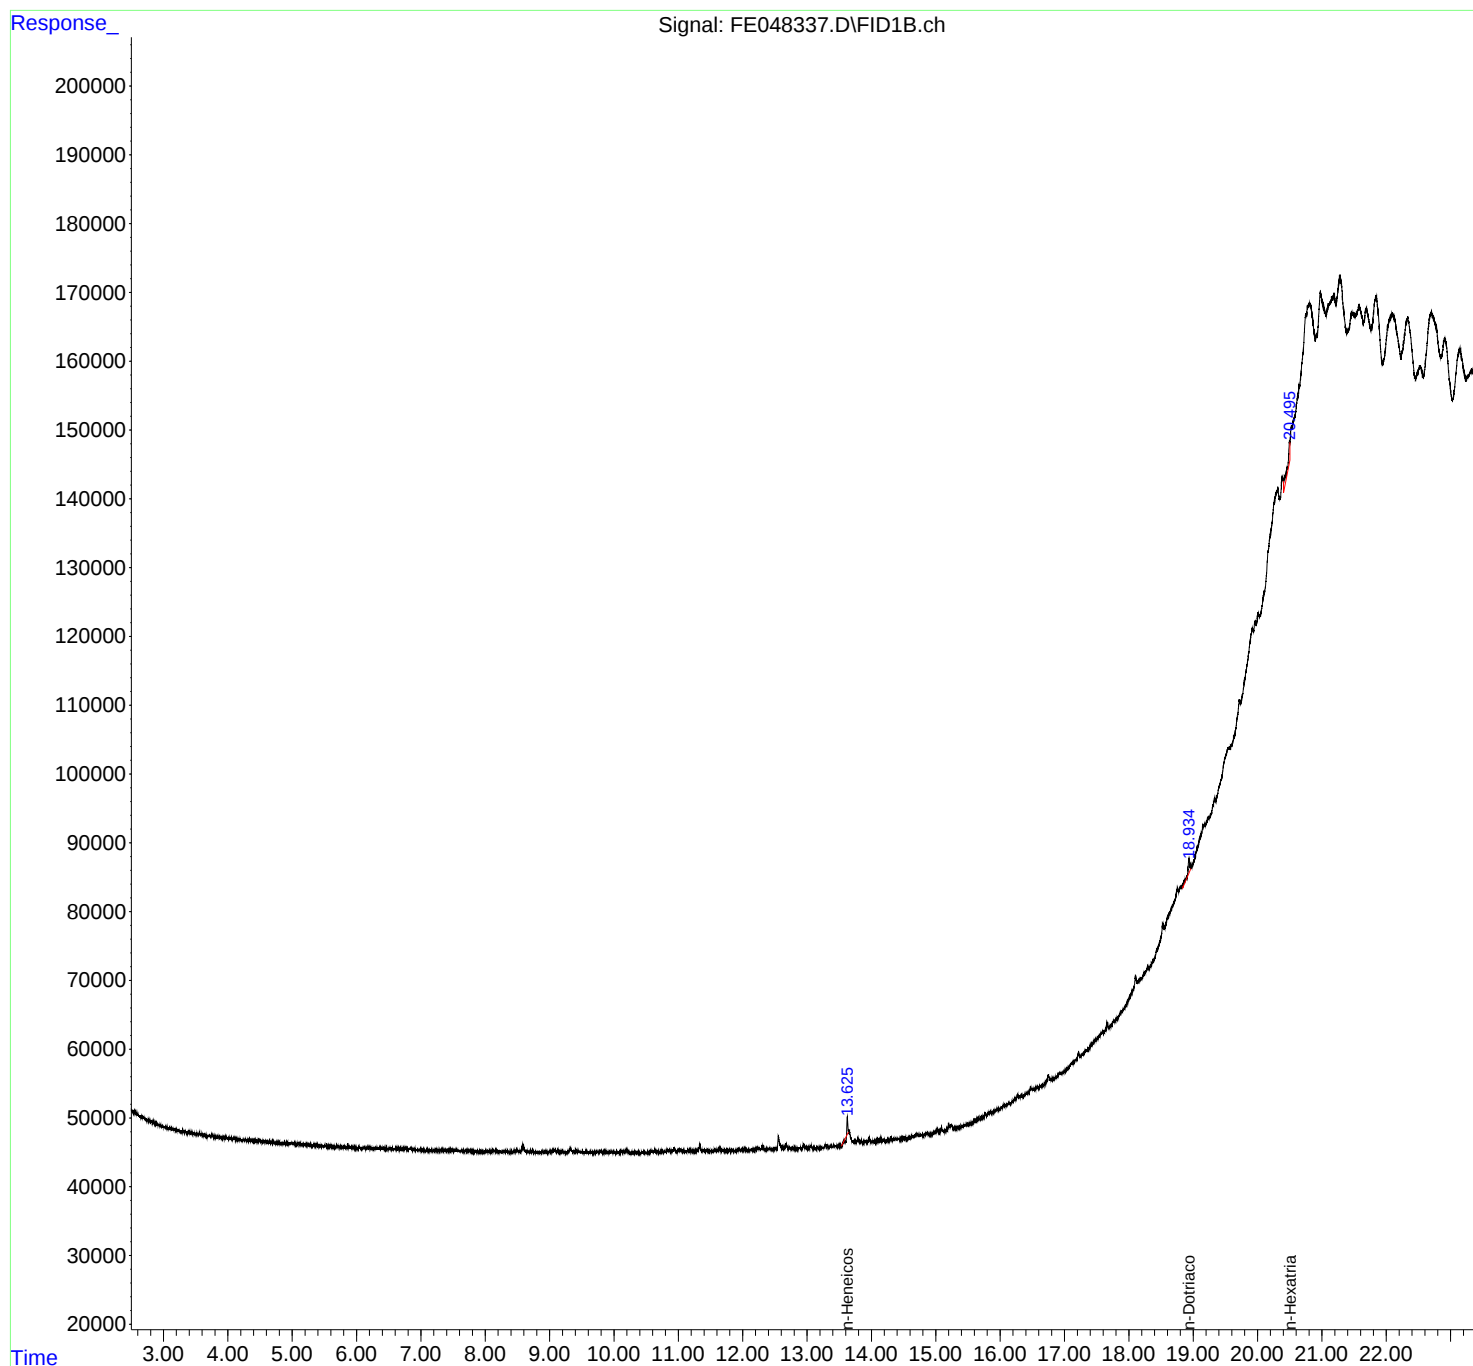


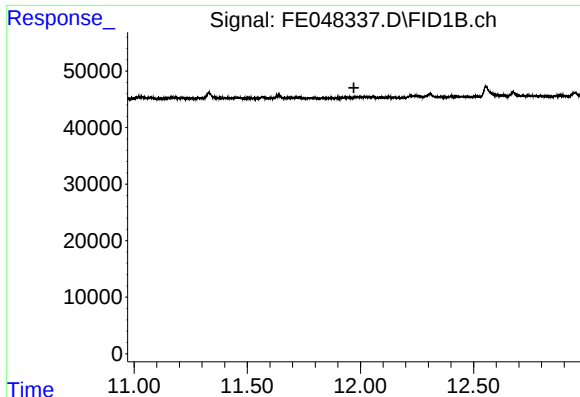

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T. : 11.971 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

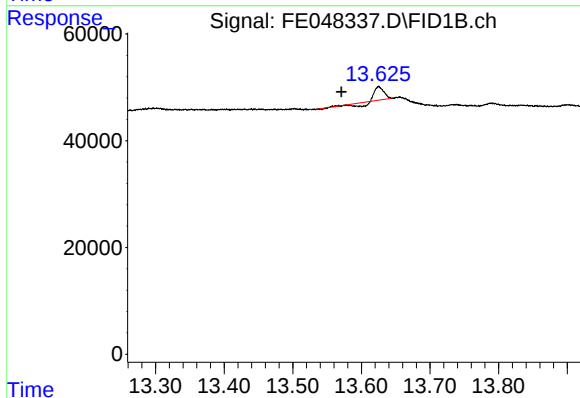


#11 n-Heneicosane (C21)

R.T.: 13.625 min
Delta R.T.: 0.054 min
Response: 13797
Conc: 0.10 ug/ml

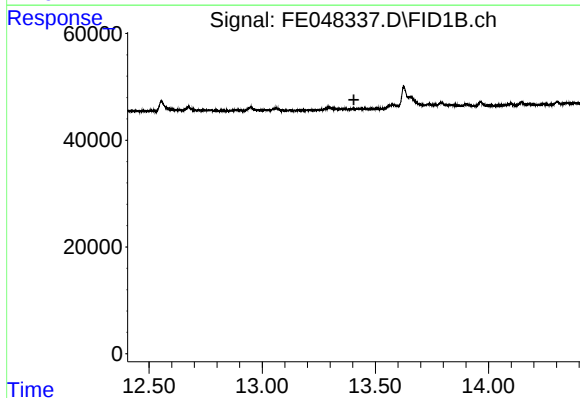


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T. : 13.405 min
Response: 0
Conc: N.D.

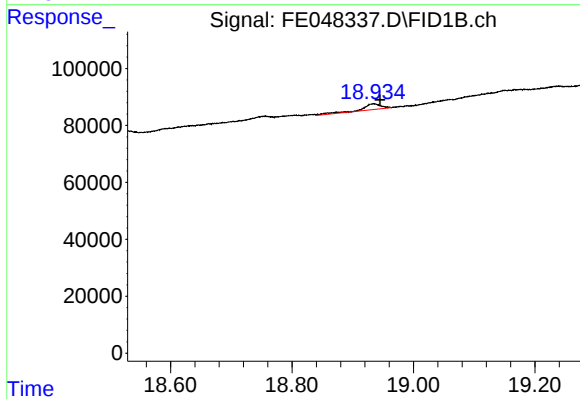

#18 n-Dotriacontane (C32)

R.T.: 18.934 min
Delta R.T.: -0.011 min
Response: 44938
Conc: 0.33 ug/ml

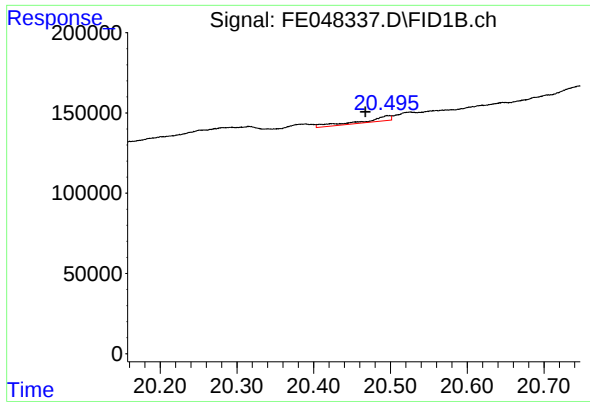

#20 n-Hexatriacontane (C36)

R.T.: 20.496 min
Delta R.T.: 0.029 min
Response: 79765
Conc: 0.59 ug/ml

Instrument :
FID_E
ClientSampleId :