

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052523AL\
Data File : FE042237.D
Signal(s) : FID1B.ch
Acq On : 26 May 2023 05:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 26 06:42:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
Quant Title : GC Extractables
QLast Update : Thu May 18 06:27:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
20) T	n-Hexatriacontane (C36)	20.428	1151355	8.858 ug/ml
21) T	n-Octatriacontane (C38)	21.219	188791	1.392 ug/ml
22) T	n-Tetracontane (C40)	22.189	365770	2.629 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052523AL\
Data File : FE042237.D
Signal(s) : FID1B.ch
Acq On : 26 May 2023 05:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 26 06:42:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
Quant Title : GC Extractables
QLast Update : Thu May 18 06:27:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

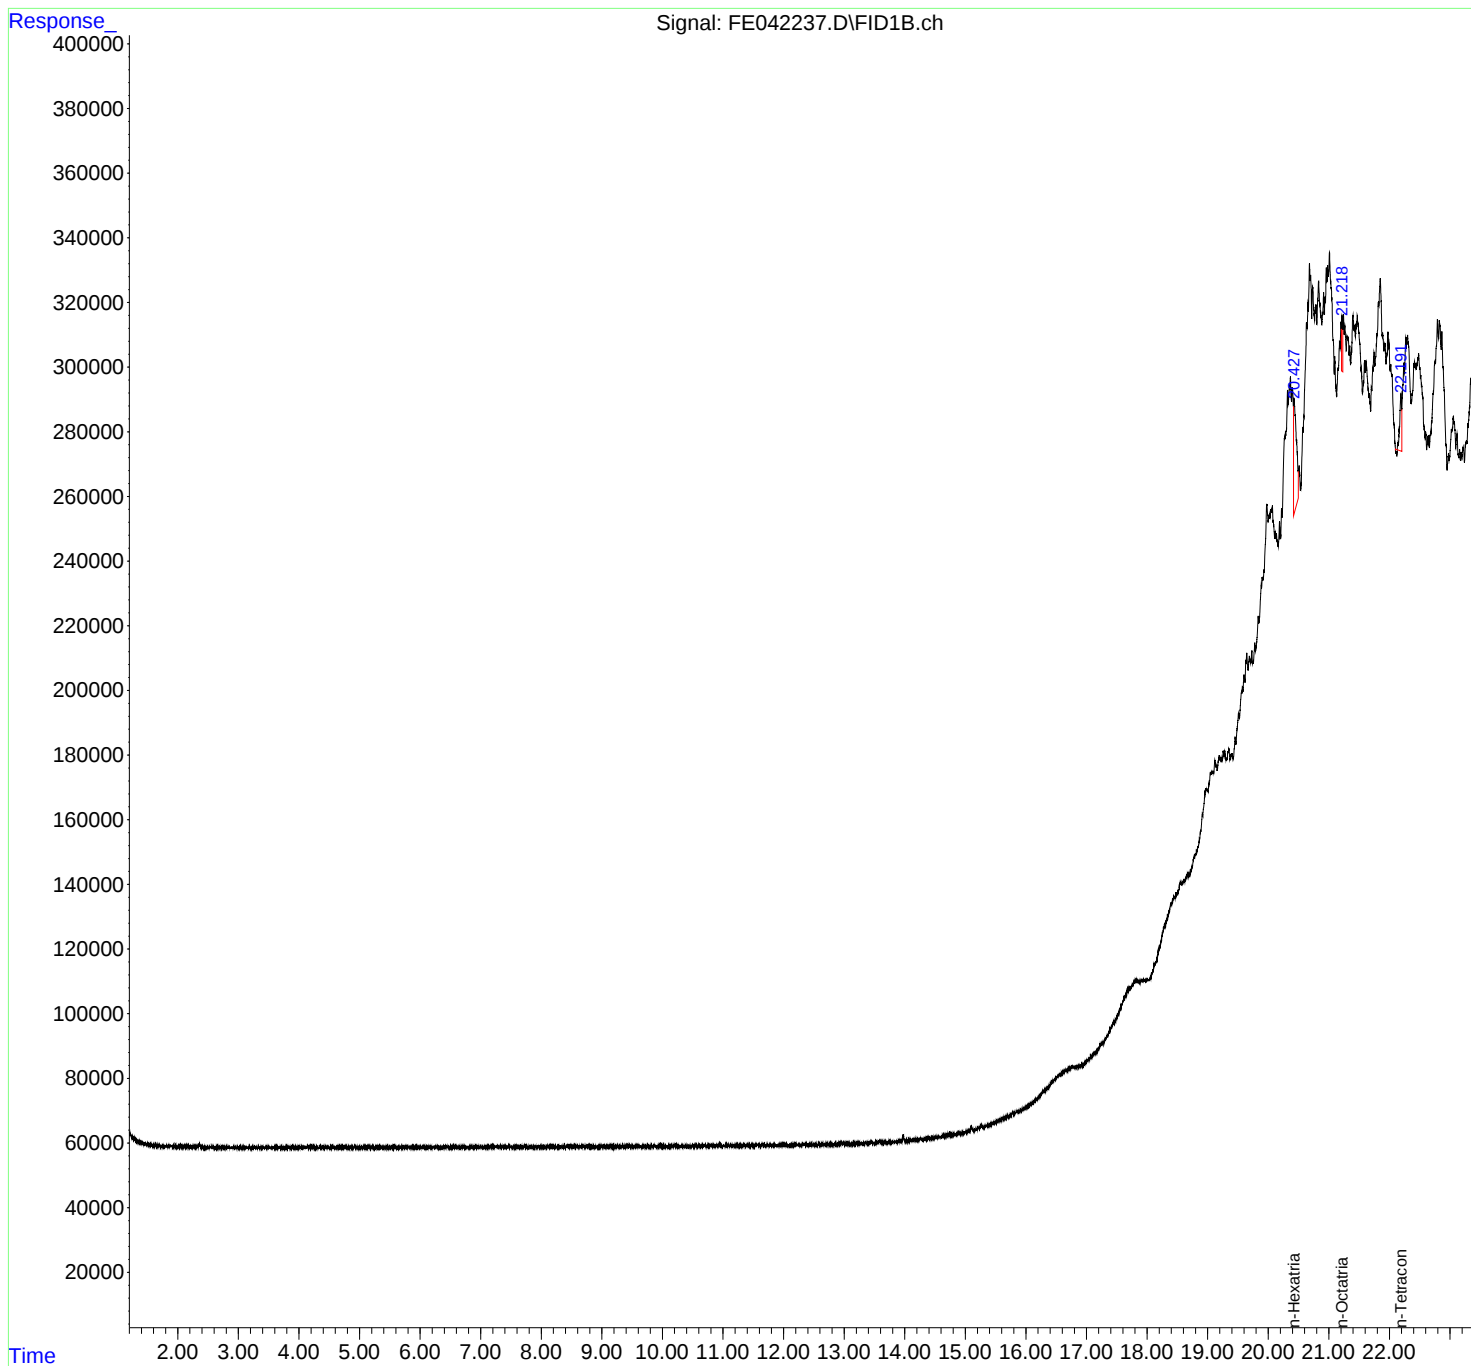


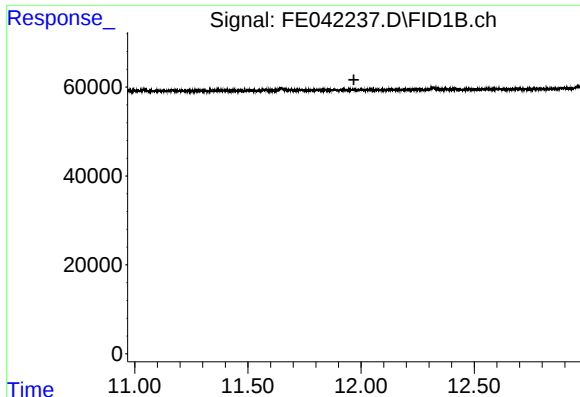

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.968 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

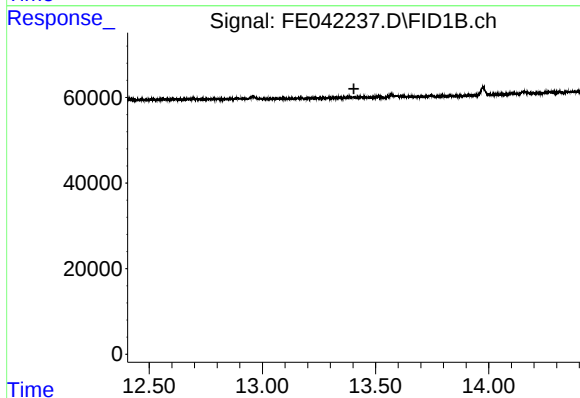


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.404 min
Response: 0
Conc: N.D.

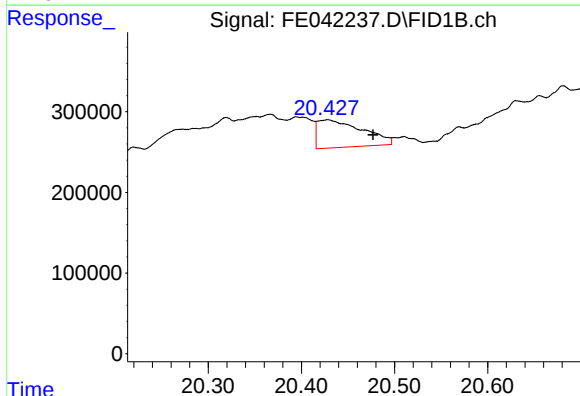


#20 n-Hexatriacontane (C36)

R.T.: 20.428 min
Delta R.T.: -0.048 min
Response: 1151355
Conc: 8.86 ug/ml

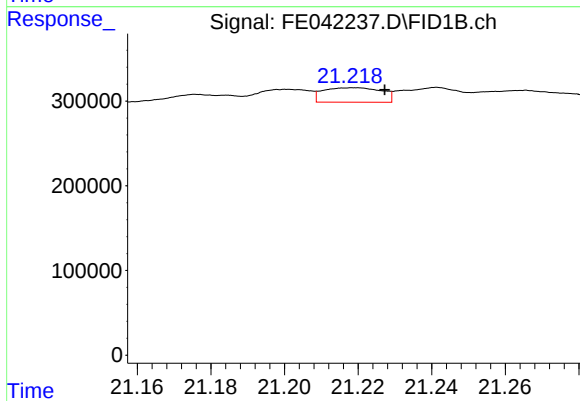

#21 n-Octatriacontane (C38)

R.T.: 21.219 min
Delta R.T.: -0.008 min
Response: 188791
Conc: 1.39 ug/ml

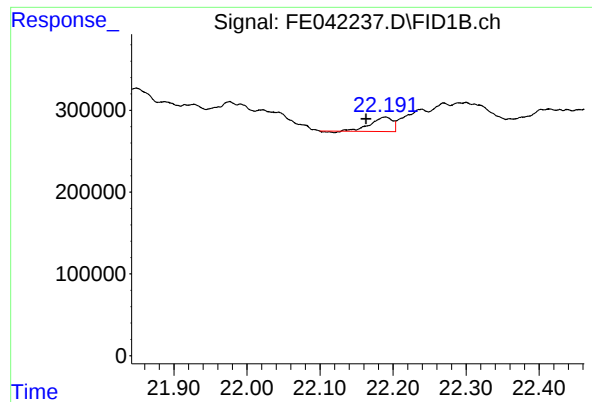

#22 n-Tetracontane (C40)

R.T.: 22.189 min
Delta R.T.: 0.026 min
Response: 365770
Conc: 2.63 ug/ml

Instrument :
FID_E
ClientSampleId :