

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052623AL\
 Data File : FE042248.D
 Signal(s) : FID1B.ch
 Acq On : 26 May 2023 12:03
 Operator : YP\AJ
 Sample : 02941-03DL2 50X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 27 00:27:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
 Quant Title : GC Extractables
 QLast Update : Thu May 18 06:27:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10) T	n-Eicosane (C20)	13.017f	297830	1.965 ug/ml
20) T	n-Hexatriacontane (C36)	20.505	746620	5.744 ug/ml
22) T	n-Tetracontane (C40)	22.193	785547	5.647 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052623AL\
Data File : FE042248.D
Signal(s) : FID1B.ch
Acq On : 26 May 2023 12:03
Operator : YP\AJ
Sample : 02941-03DL2 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 27 00:27:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
Quant Title : GC Extractables
QLast Update : Thu May 18 06:27:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

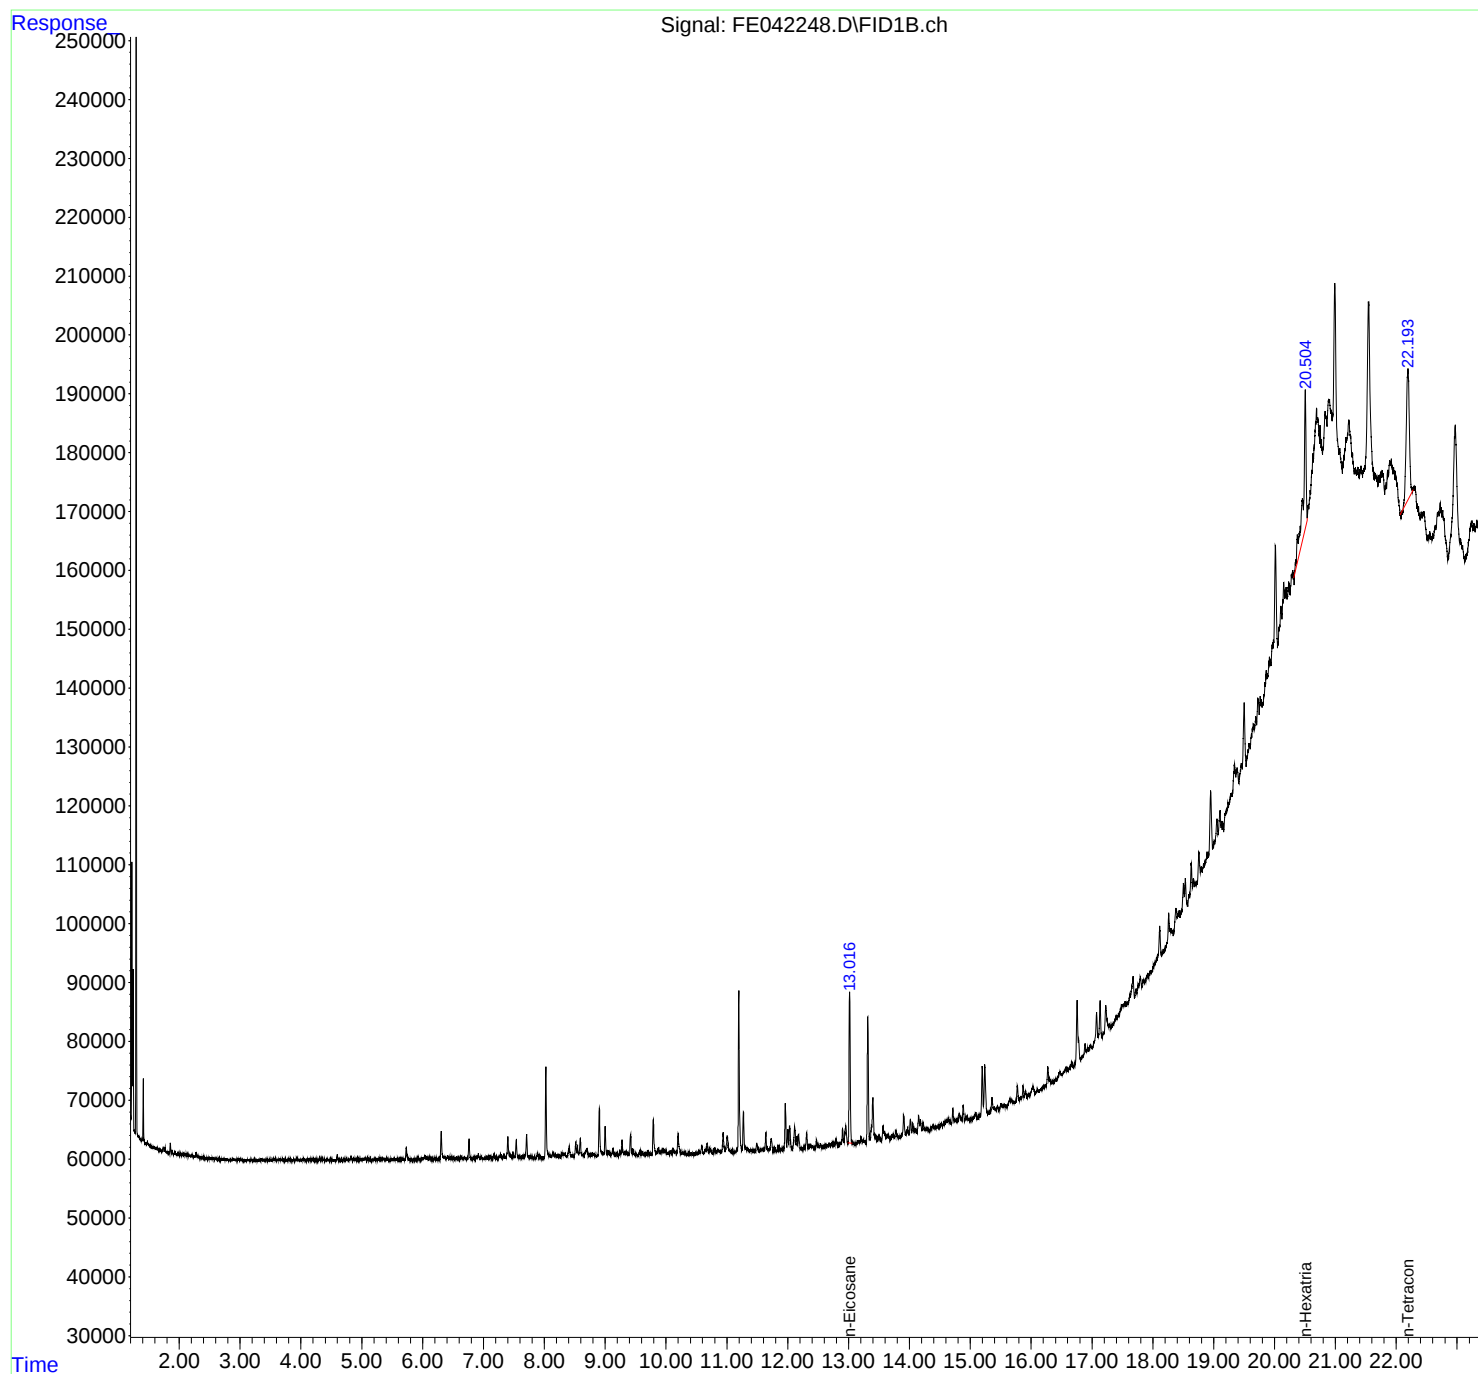


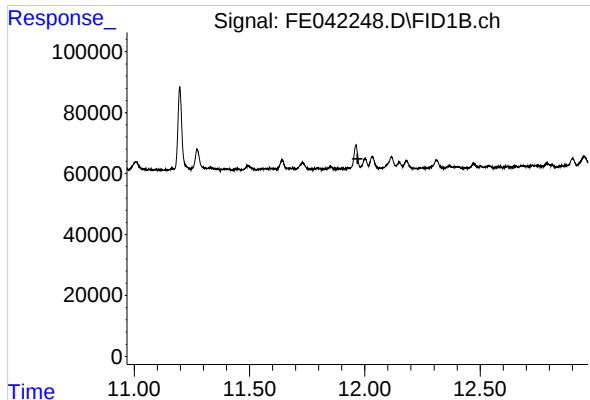

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.968 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

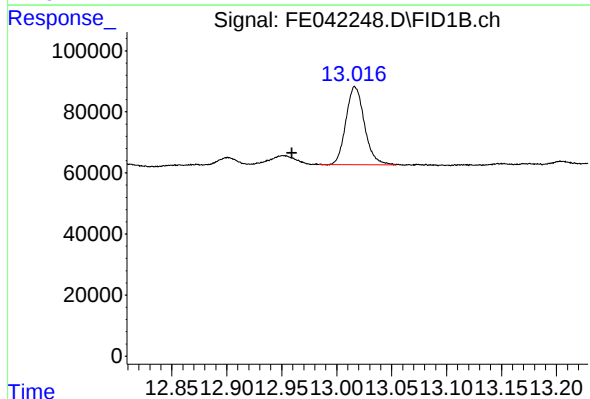


#10 n-Eicosane (C20)

R.T.: 13.017 min
Delta R.T.: 0.058 min
Response: 297830
Conc: 1.96 ug/ml

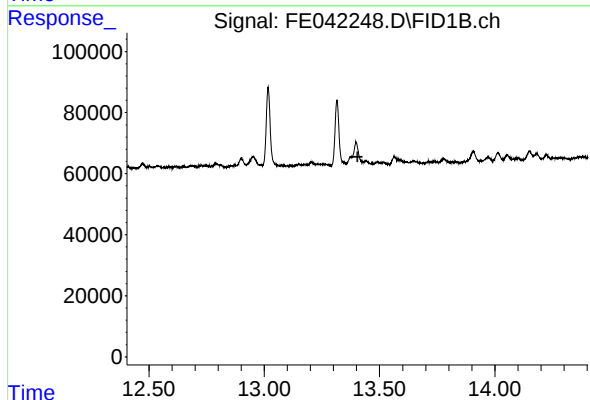


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.404 min
Response: 0
Conc: N.D.

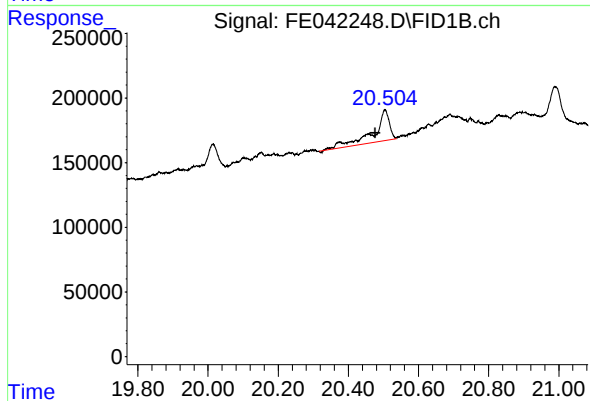

#20 n-Hexatriacontane (C36)

R.T.: 20.505 min
Delta R.T.: 0.028 min
Response: 746620
Conc: 5.74 ug/ml

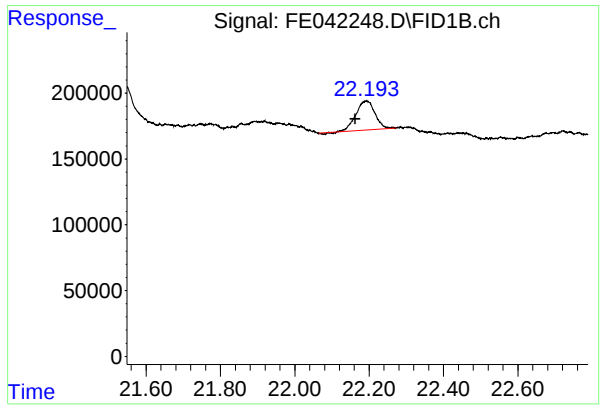

#22 n-Tetracontane (C40)

R.T.: 22.193 min
Delta R.T.: 0.030 min
Response: 785547
Conc: 5.65 ug/ml

Instrument :
FID_E
ClientSampleId :