

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE052822\  
Data File : FE035808.D  
Signal(s) : FID1B.CH  
Acq On : 28 May 2022 16:36  
Operator : YP\AJ  
Sample : N3074-01MS  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: May 30 00:30:48 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE051322.M  
Quant Title :  
QLast Update : Fri May 13 15:02:22 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.034  | 168438   | 1.500 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 12.003f | 240917   | 1.877 ug/ml |
| 10) N-TETRACOSANE             | 14.214  | 148897   | 1.175 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE052822\  
Data File : FE035808.D  
Signal(s) : FID1B.CH  
Acq On : 28 May 2022 16:36  
Operator : YP\AJ  
Sample : N3074-01MS  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: May 30 00:30:48 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE051322.M  
Quant Title :  
QLast Update : Fri May 13 15:02:22 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

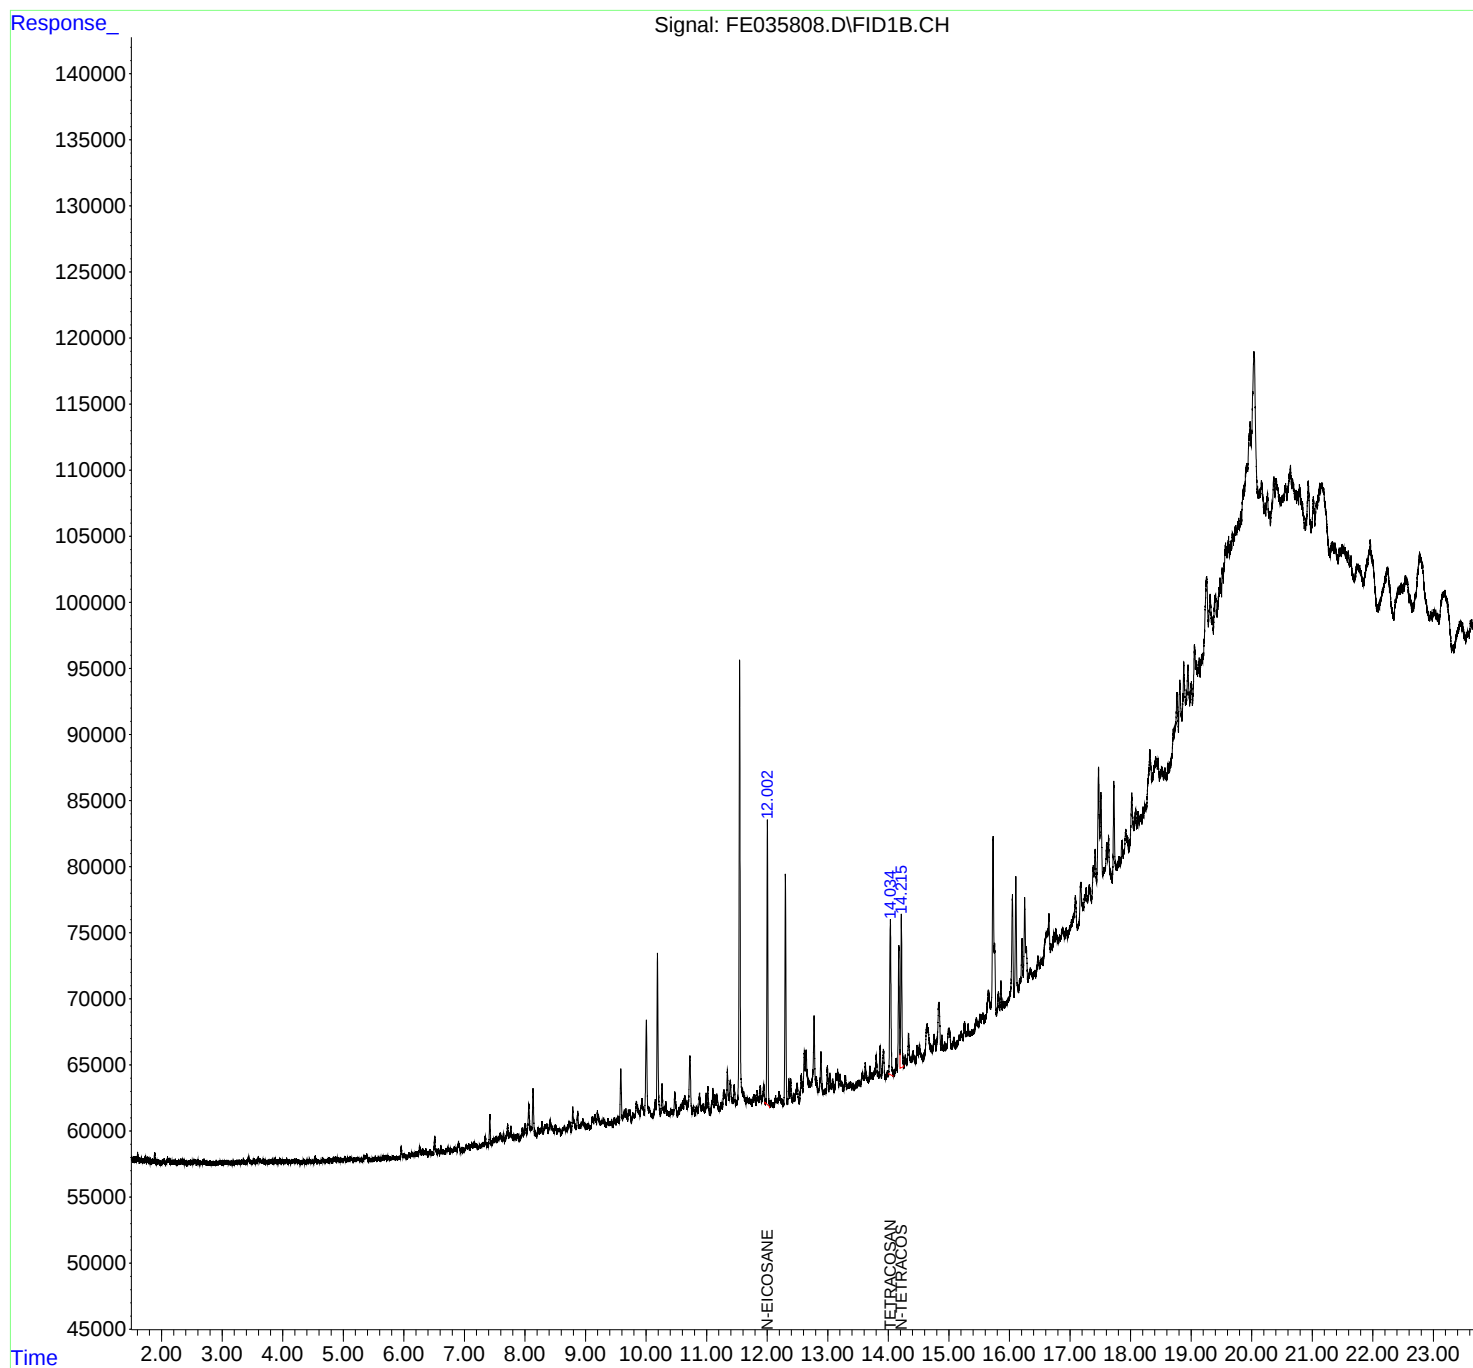


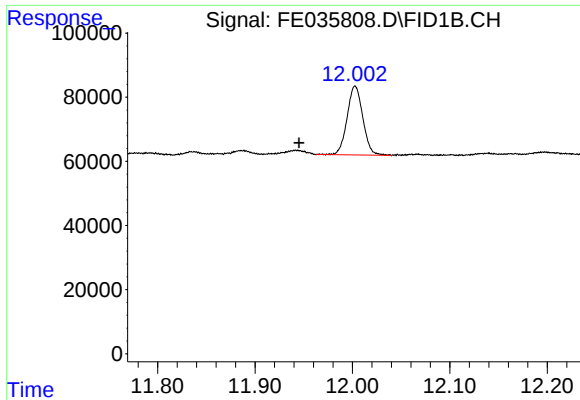

#7 N-EICOSANE


R.T.: 12.003 min  
Delta R.T.: 0.058 min  
Response: 240917  
Conc: 1.88 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

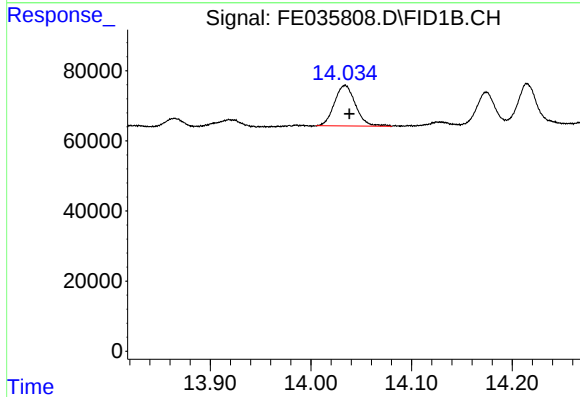

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.034 min  
Delta R.T.: -0.004 min  
Response: 168438  
Conc: 1.50 ug/ml

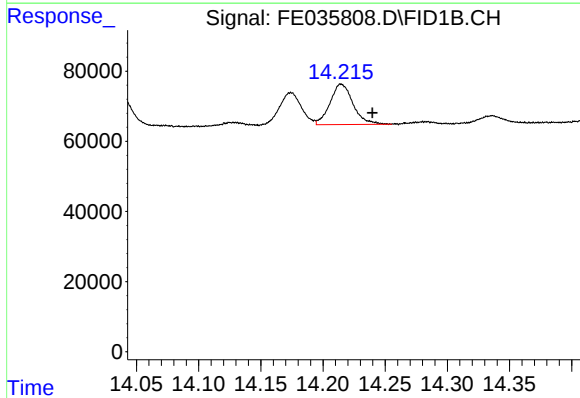

#10 N-TETRACOSANE

R.T.: 14.214 min  
Delta R.T.: -0.026 min  
Response: 148897  
Conc: 1.17 ug/ml