

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052822\
Data File : FE035808.D
Signal(s) : FID1B.CH
Acq On : 28 May 2022 16:36
Operator : YP\AJ
Sample : N3074-01MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
WASTEMS

Integration File: Sample.e
Quant Time: May 30 00:30:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
Quant Title :
QLast Update : Fri May 13 15:02:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.034	168438	1.500 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE052822\
Data File : FE035808.D
Signal(s) : FID1B.CH
Acq On : 28 May 2022 16:36
Operator : YP\AJ
Sample : N3074-01MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
WASTEMS

Integration File: Sample.e
Quant Time: May 30 00:30:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
Quant Title :
QLast Update : Fri May 13 15:02:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

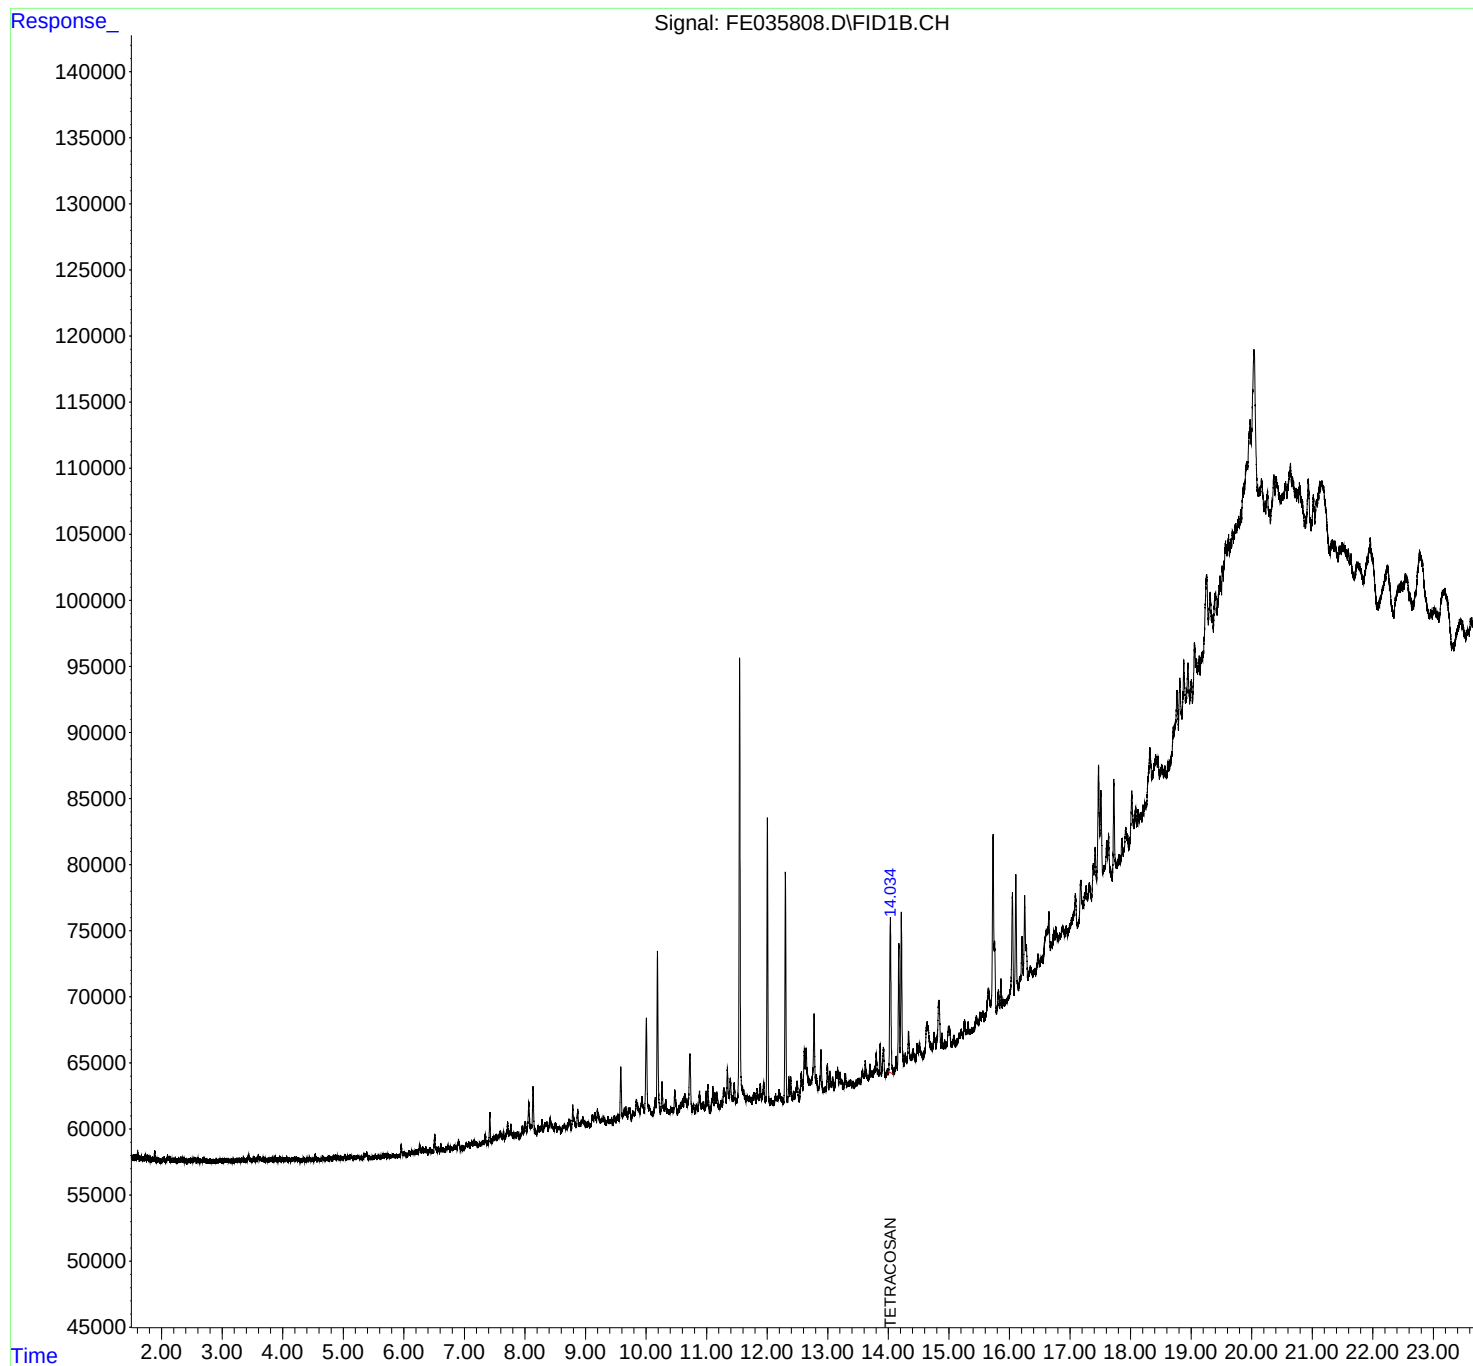

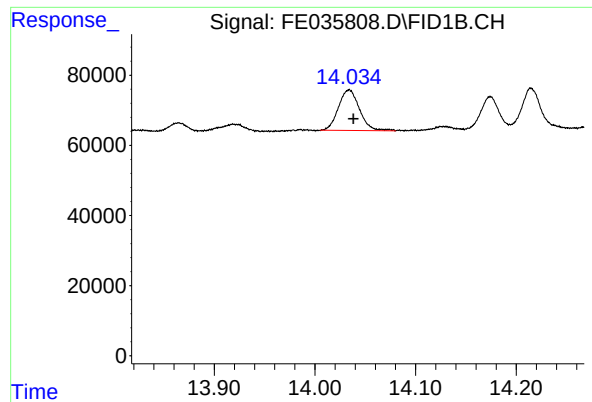

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.034 min
Delta R.T.: -0.004 min
Response: 168438
Conc: 1.50 ug/ml

Instrument :
FID_E
ClientSampleId :
WASTEMS