

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051322\
 Data File : FE035812.D
 Signal(s) : FID1B.CH
 Acq On : 31 May 2022 9:49
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 01 01:37:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
 Quant Title :
 QLast Update : Fri May 13 15:02:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
8) N-DOCOSANE	13.119	419618	3.279 ug/ml
10) N-TETRACOSANE	14.227	467137	3.686 ug/ml
11) N-HEXACOSANE	15.252	625635	4.976 ug/ml
12) N-OCTACOSANE	16.202	477667	3.867 ug/ml
13) N-TRIACONTANE	17.088	441521	3.645 ug/ml
14) N-DOTRIACONTANE	17.920	384348	3.410 ug/ml
15) N-TETRATRIACONTANE	18.697	118469	1.197 ug/ml
16) N-HEXATRIACONTANE	19.433	8375	0.105 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE053122\
Data File : FE035812.D
Signal(s) : FID1B.CH
Acq On : 31 May 2022 9:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 01 01:37:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
Quant Title :
QLast Update : Fri May 13 15:02:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

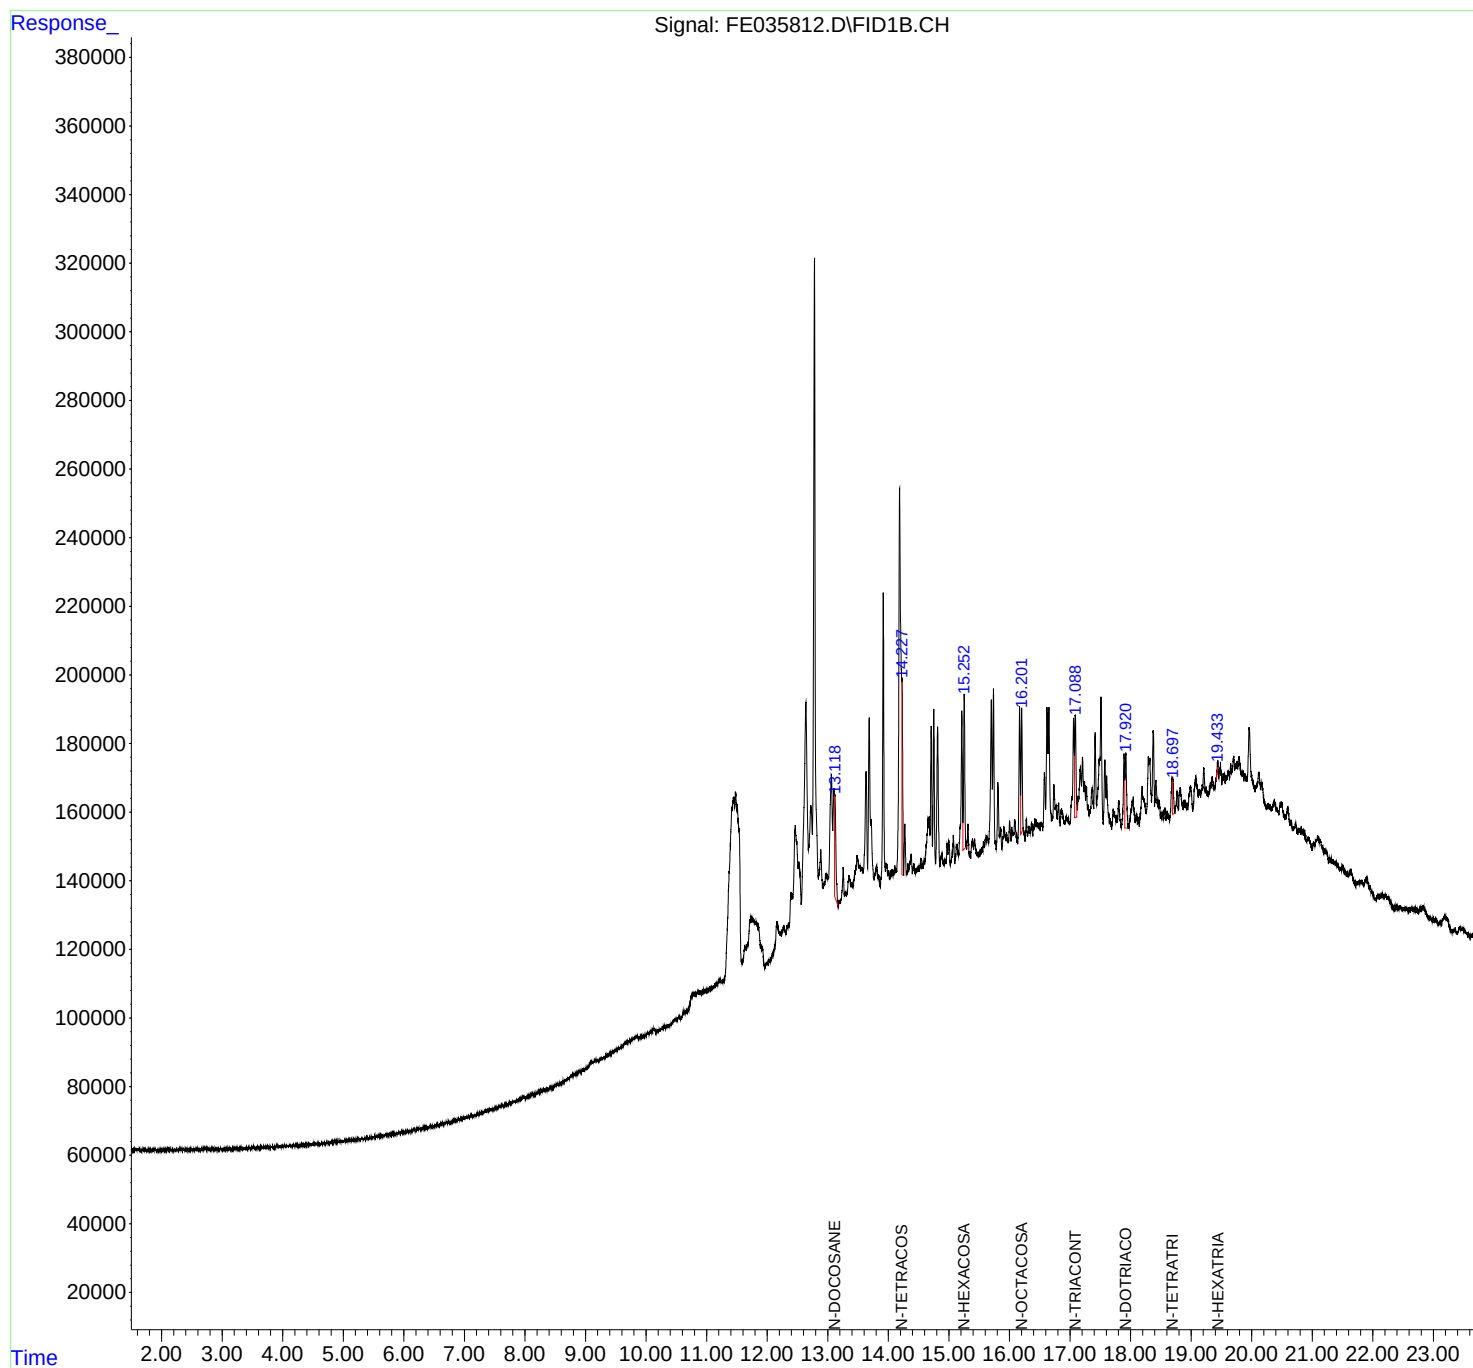


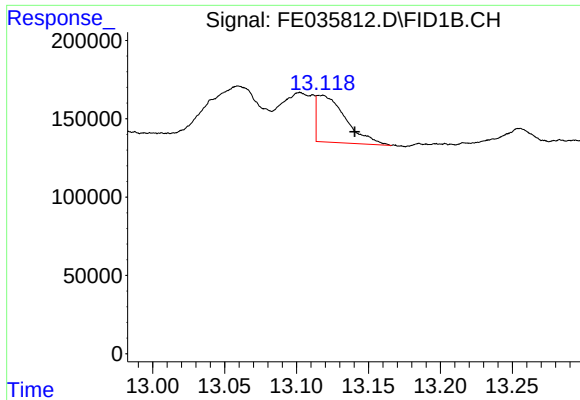

#8 N-DOCOSANE


R.T.: 13.119 min
Delta R.T.: -0.022 min
Response: 419618
Conc: 3.28 ug/ml

Instrument :
FID_E
ClientSampleId :

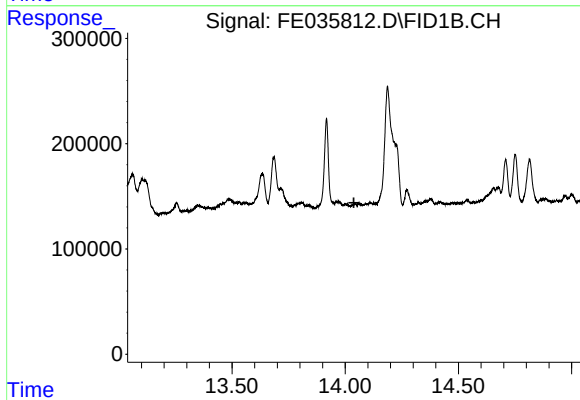


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.038 min
Response: 0
Conc: N.D.

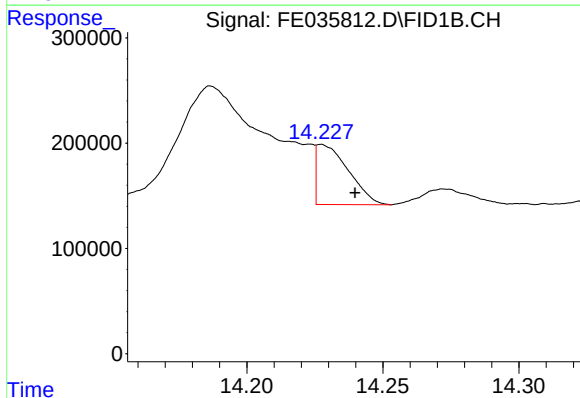


#10 N-TETRACOSANE

R.T.: 14.227 min
Delta R.T.: -0.012 min
Response: 467137
Conc: 3.69 ug/ml

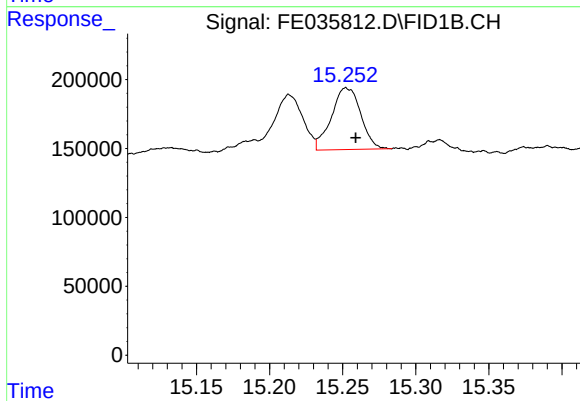

#11 N-HEXACOSANE


R.T.: 15.252 min
Delta R.T.: -0.007 min
Response: 625635
Conc: 4.98 ug/ml

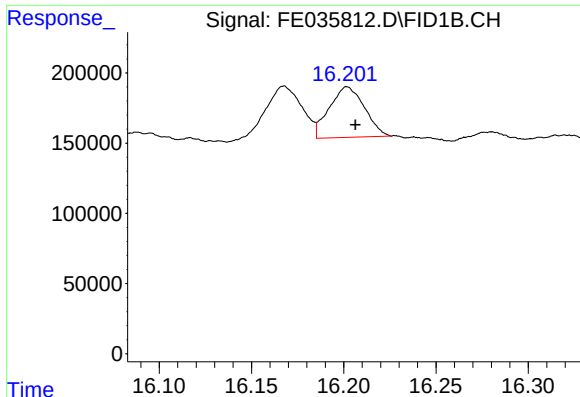

#12 N-OCTACOSANE


R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 477667
Conc: 3.87 ug/ml

Instrument :
FID_E
ClientSampleId :

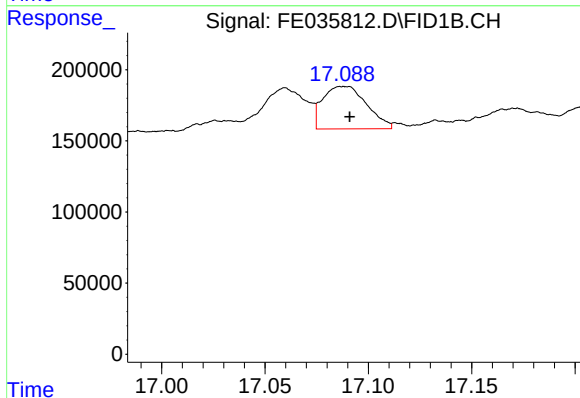


#13 N-TRIACONTANE

R.T.: 17.088 min
Delta R.T.: -0.003 min
Response: 441521
Conc: 3.65 ug/ml

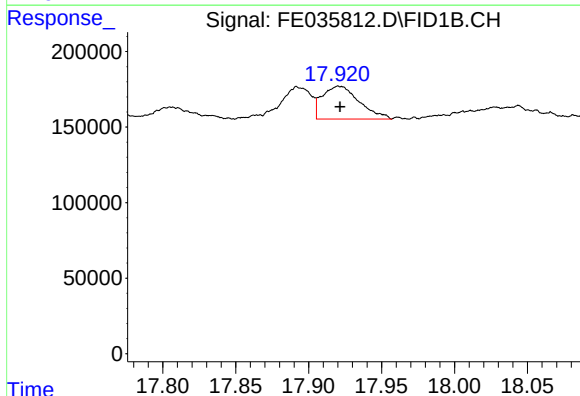


#14 N-DOTRIACONTANE

R.T.: 17.920 min
Delta R.T.: -0.001 min
Response: 384348
Conc: 3.41 ug/ml

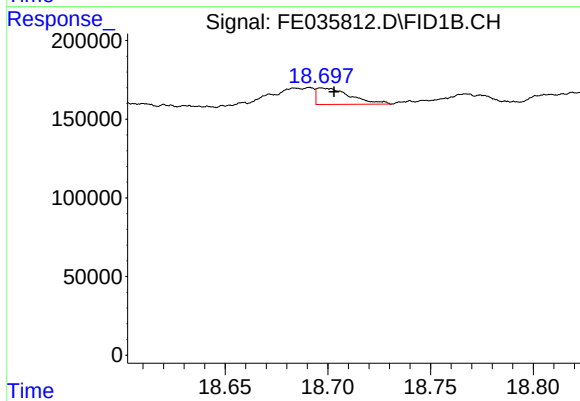

#15 N-TETRATRIACONTANE

R.T.: 18.697 min
Delta R.T.: -0.006 min
Response: 118469
Conc: 1.20 ug/ml

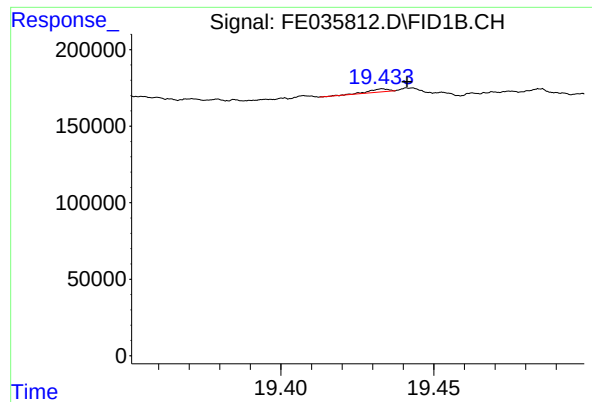

#16 N-HEXATRIACONTANE

R.T.: 19.433 min
Delta R.T.: -0.008 min
Response: 8375
Conc: 0.11 ug/ml

Instrument :

FID_E

ClientSampleId :