

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE051322\
 Data File : FE035815.D
 Signal(s) : FID1B.CH
 Acq On : 31 May 2022 11:23
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 01 01:37:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
 Quant Title :
 QLast Update : Fri May 13 15:02:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	5.812	3673920	28.730 ug/ml
12)	N-OCTACOSANE	16.205	3282176	26.570 ug/ml
13)	N-TRIACONTANE	17.089	93586	0.773 ug/ml
14)	N-DOTRIACONTANE	17.920	117131	1.039 ug/ml
15)	N-TETRATRIACONTANE	18.702	99896	1.010 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE053122\
Data File : FE035815.D
Signal(s) : FID1B.CH
Acq On : 31 May 2022 11:23
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 01 01:37:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE051322.M
Quant Title :
QLast Update : Fri May 13 15:02:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

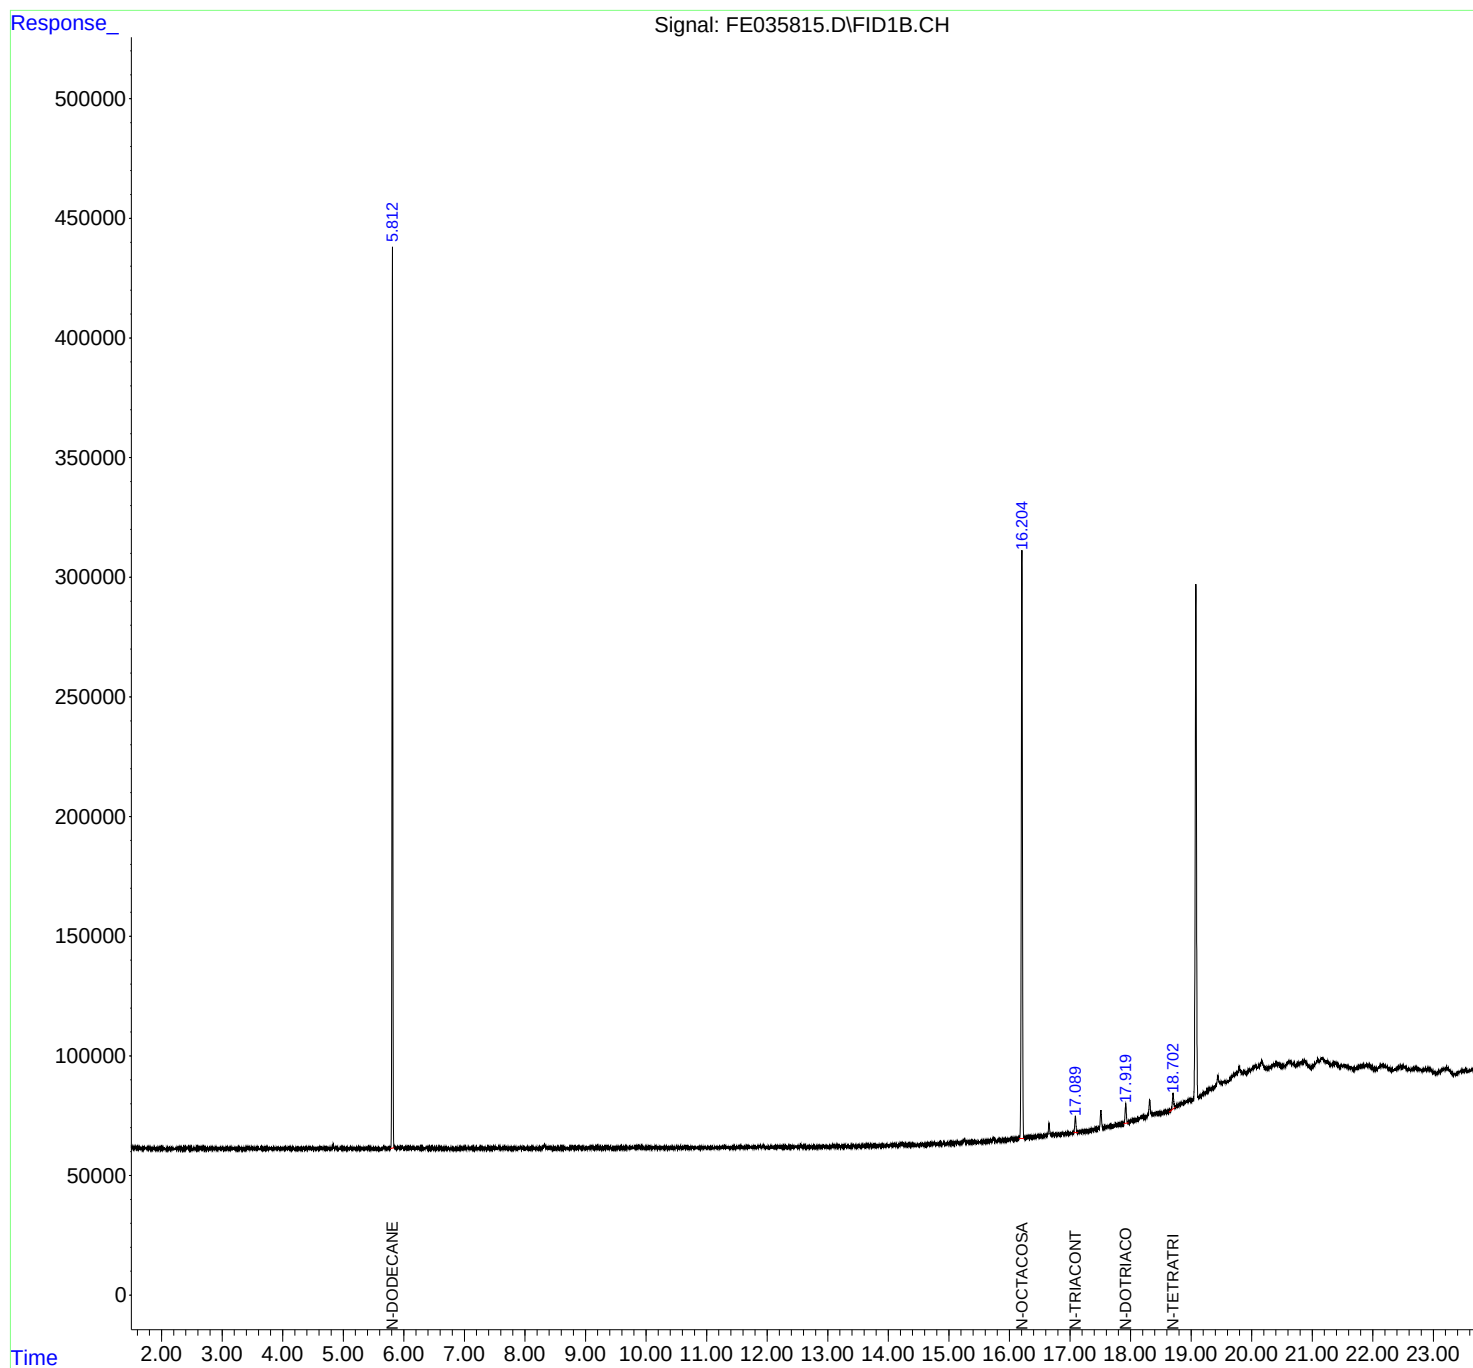

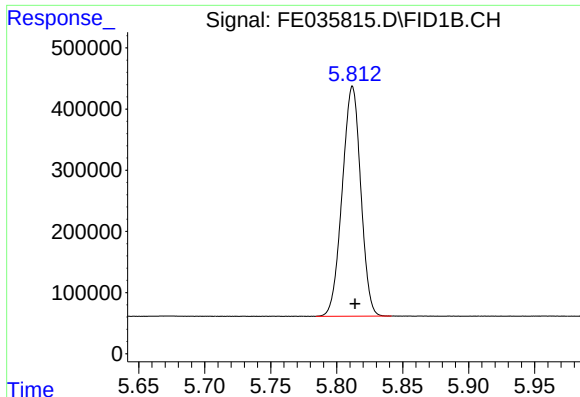


#3 N-DODECANE

R.T.: 5.812 min
Delta R.T.: -0.002 min
Response: 3673920
Conc: 28.73 ug/ml

Instrument :


FID_E

ClientSampleId :

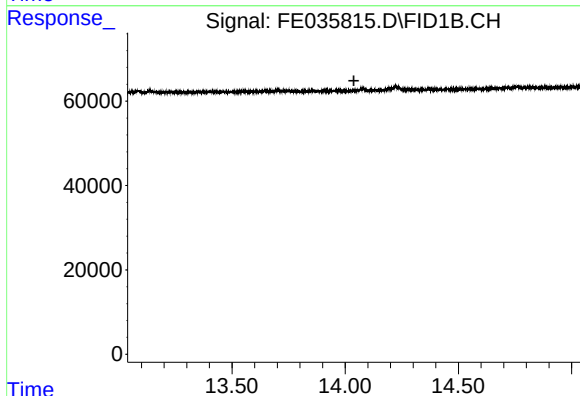


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.038 min
Response: 0
Conc: N.D.

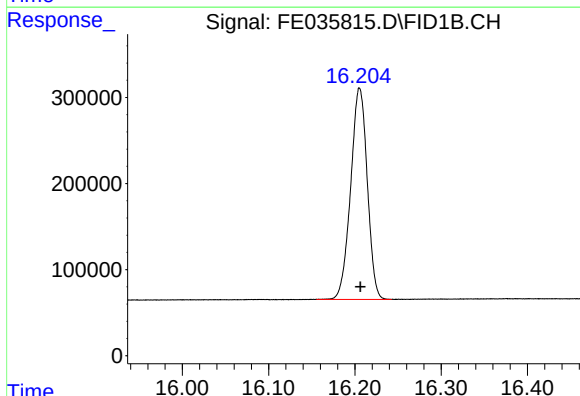


#12 N-OCTACOSANE

R.T.: 16.205 min
Delta R.T.: -0.001 min
Response: 3282176
Conc: 26.57 ug/ml

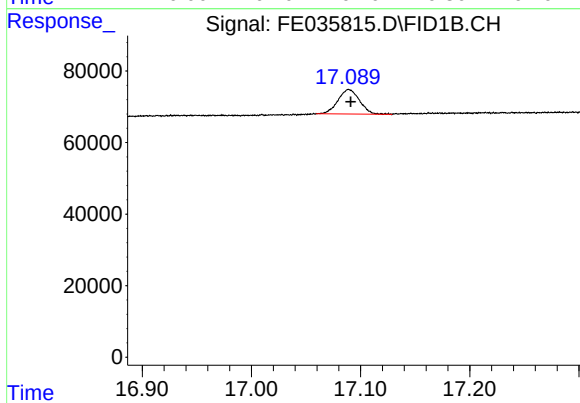

#13 N-TRIACONTANE


R.T.: 17.089 min
Delta R.T.: -0.002 min
Response: 93586
Conc: 0.77 ug/ml

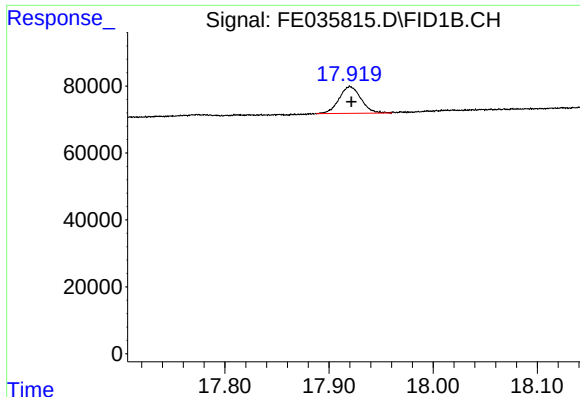

#14 N-DOTRIACONTANE

R.T.: 17.920 min
Delta R.T.: -0.001 min
Response: 117131
Conc: 1.04 ug/ml

Instrument :
FID_E
ClientSampleId :

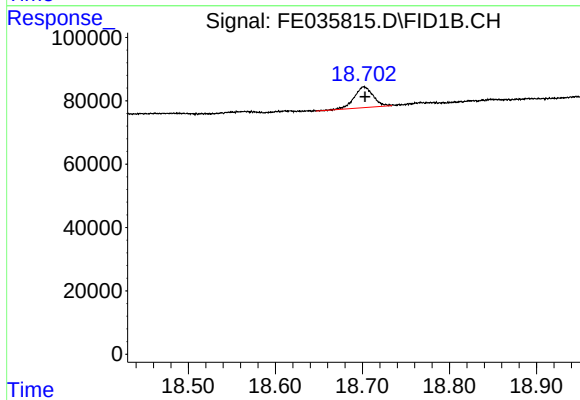

#15 N-TETRATRIACONTANE

R.T.: 18.702 min
Delta R.T.: -0.001 min
Response: 99896
Conc: 1.01 ug/ml