

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060121\
 Data File : FE033847.D
 Signal(s) : FID1B.CH
 Acq On : 01 Jun 2021 11:39
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 01:03:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.770	300217	0.659 ug/ml
14) N-DOTRIACONTANE	18.604	377140	0.847 ug/ml
15) N-TETRATRIACONTANE	19.388	222155	0.517 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060121\
Data File : FE033847.D
Signal(s) : FID1B.CH
Acq On : 01 Jun 2021 11:39
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 01:03:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

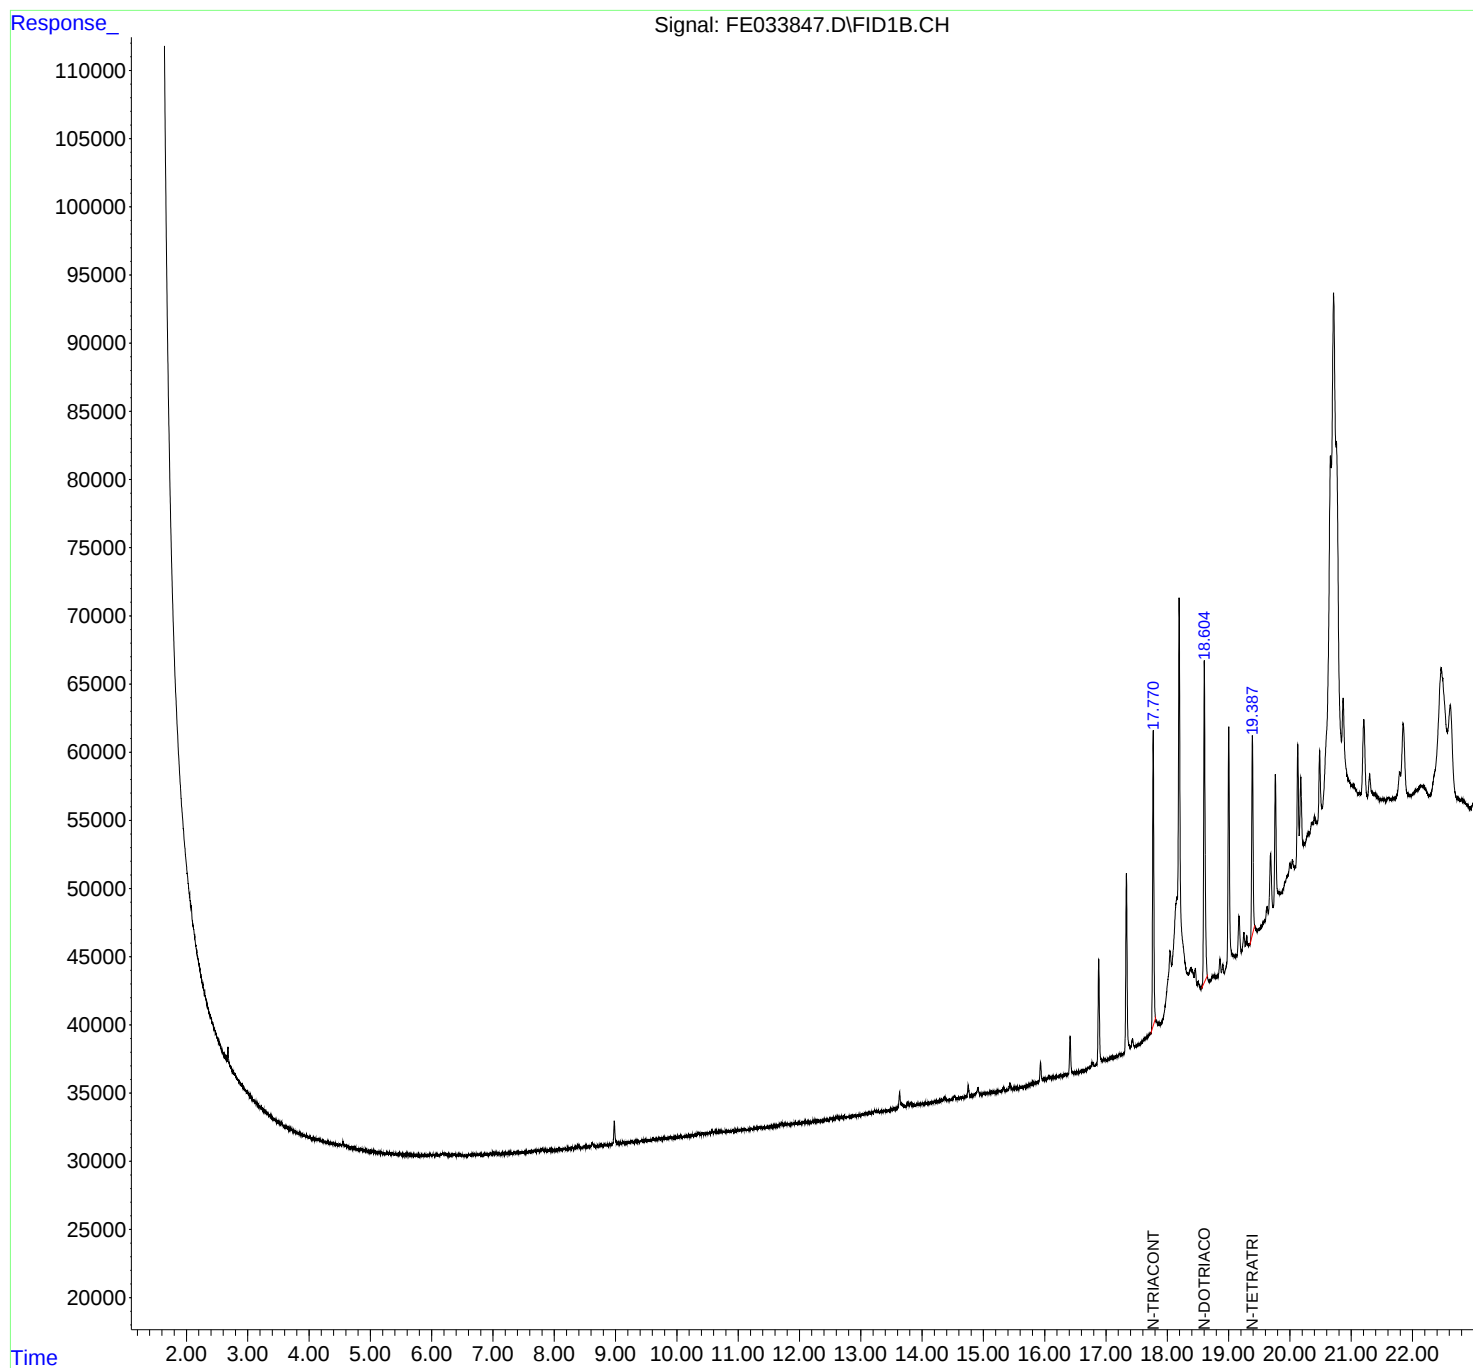


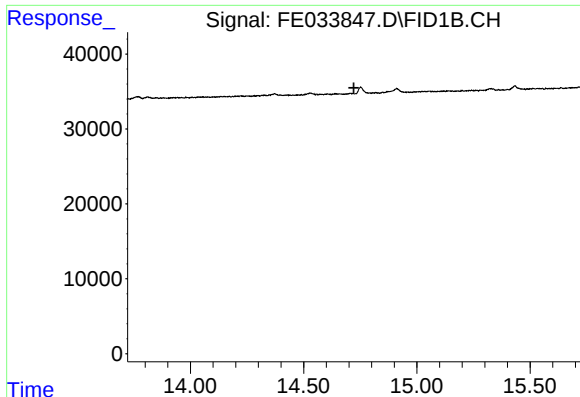

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.721 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

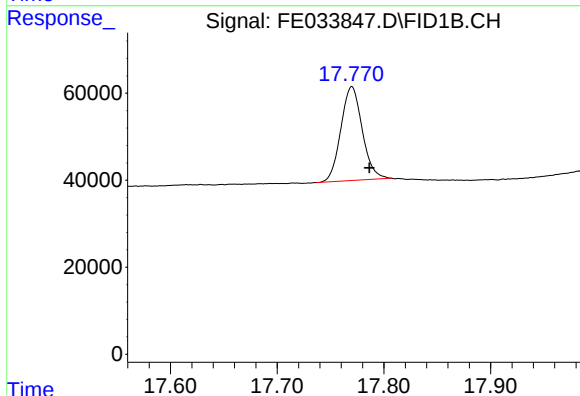


#13 N-TRIACONTANE

R.T.: 17.770 min
Delta R.T.: -0.017 min
Response: 300217
Conc: 0.66 ug/ml

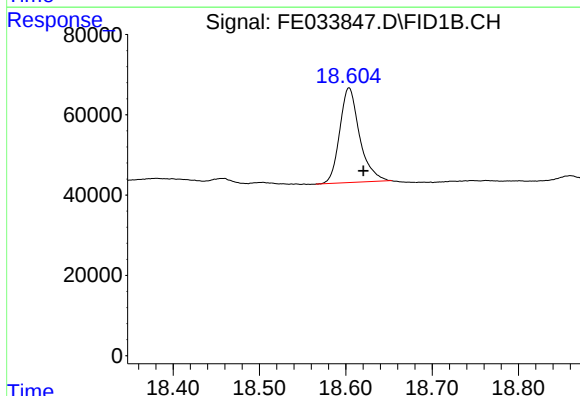

#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: -0.017 min
Response: 377140
Conc: 0.85 ug/ml

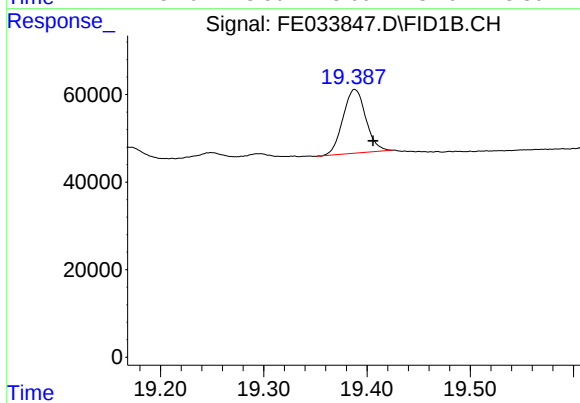

#15 N-TETRATRIACONTANE

R.T.: 19.388 min
Delta R.T.: -0.018 min
Response: 222155
Conc: 0.52 ug/ml