

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060122AL\
 Data File : FE035832.D
 Signal(s) : FID1B.CH
 Acq On : 01 Jun 2022 9:15
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 04:37:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 03:24:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	11.911	311168	2.608 ug/ml
11) T n-Heneicosane (C21)	12.537	350672	2.921 ug/ml
13) T n-Docosane (C22)	13.126	302634	2.513 ug/ml
14) T n-Tetracosane (C24)	14.210	842227	6.961 ug/ml
15) T n-Hexacosane (C26)	15.250	172319	1.424 ug/ml
16) T n-Octacosane (C28)	16.199	167079	1.379 ug/ml
17) T n-Tricontane (C30)	17.086	133628	1.111 ug/ml
18) T n-Dotriacontane (C32)	17.914	212412	1.848 ug/ml
19) T n-Tetratriacontane (C34)	18.700	109281	1.010 ug/ml
20) T n-Hexatriacontane (C36)	19.432	49665	<MDL ug/ml
22) T n-Tetracontane (C40)	21.086	6735	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060122AL\
Data File : FE035832.D
Signal(s) : FID1B.CH
Acq On : 01 Jun 2022 9:15
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 04:37:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
Quant Title : GC Extractables
QLast Update : Wed May 11 03:24:10 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

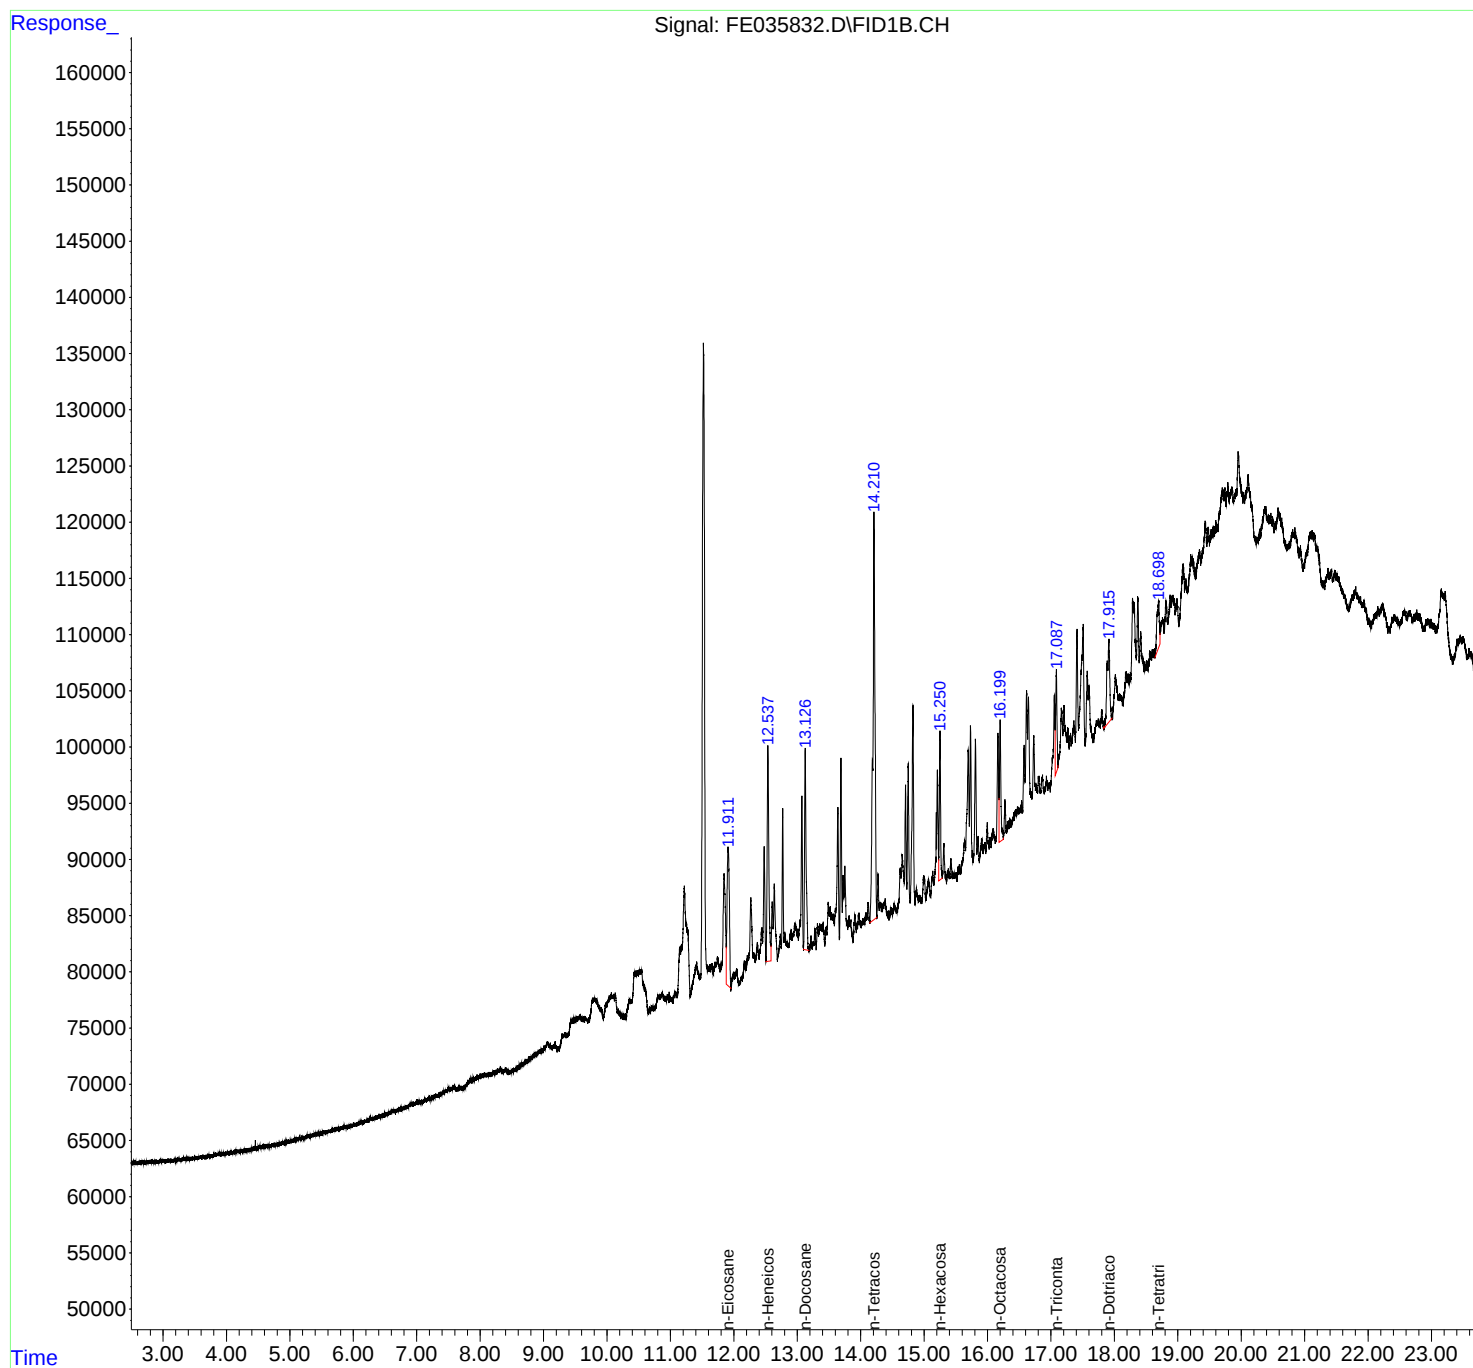


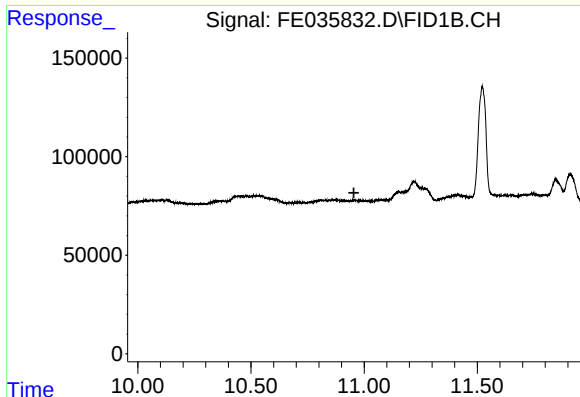

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.955 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

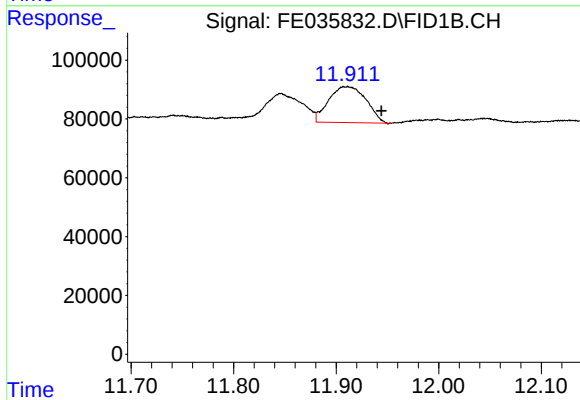


#10 n-Eicosane (C20)

R.T.: 11.911 min
Delta R.T.: -0.034 min
Response: 311168
Conc: 2.61 ug/ml

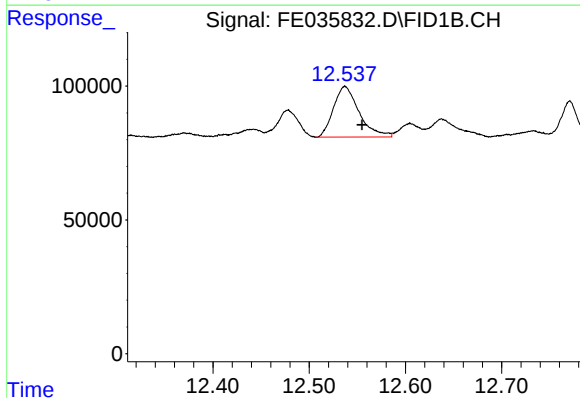


#11 n-Heneicosane (C21)

R.T.: 12.537 min
Delta R.T.: -0.018 min
Response: 350672
Conc: 2.92 ug/ml

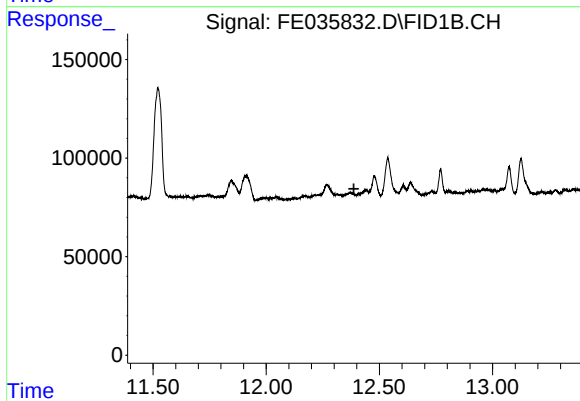

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.388 min
Response: 0
Conc: N.D.

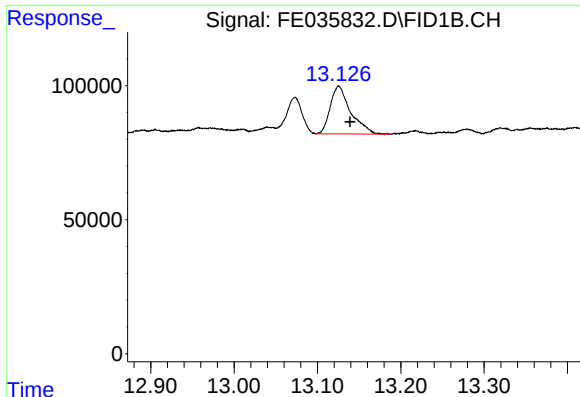

#13 n-Docosane (C22)


R.T.: 13.126 min
Delta R.T.: -0.014 min
Response: 302634
Conc: 2.51 ug/ml

Instrument :
FID_E
ClientSampleId :

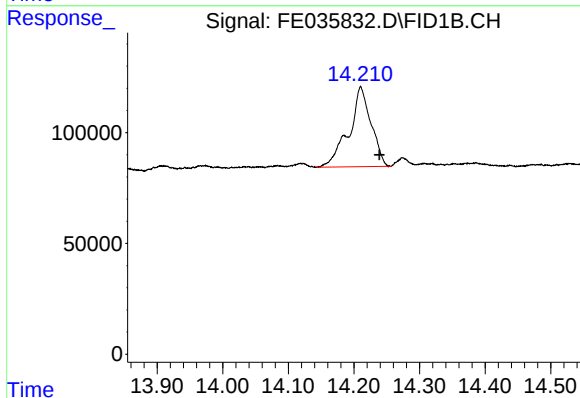


#14 n-Tetracosane (C24)

R.T.: 14.210 min
Delta R.T.: -0.029 min
Response: 842227
Conc: 6.96 ug/ml

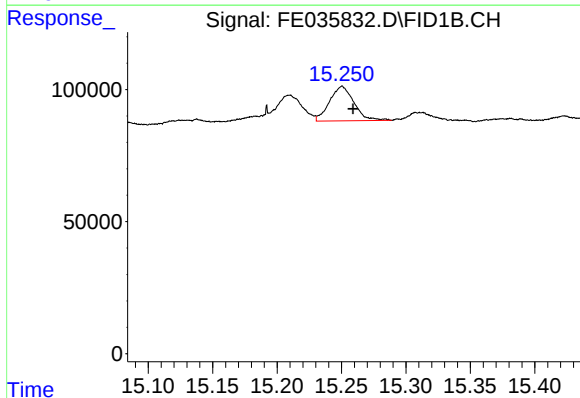


#15 n-Hexacosane (C26)

R.T.: 15.250 min
Delta R.T.: -0.009 min
Response: 172319
Conc: 1.42 ug/ml

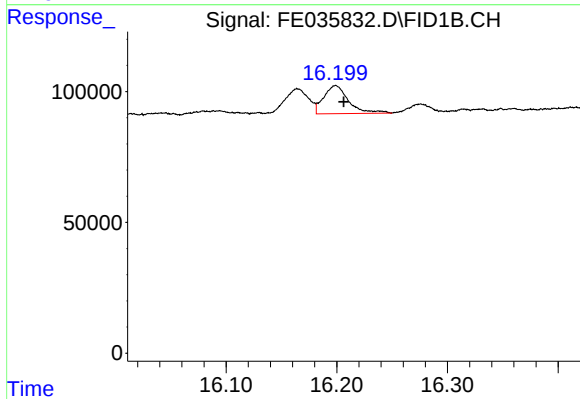

#16 n-Octacosane (C28)


R.T.: 16.199 min
Delta R.T.: -0.007 min
Response: 167079
Conc: 1.38 ug/ml

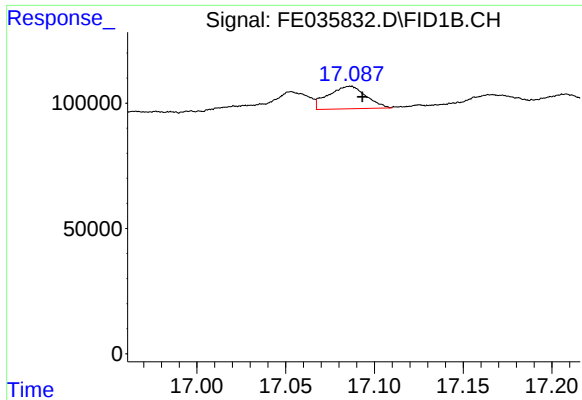

#17 n-Tricontane (C30)


R.T.: 17.086 min
Delta R.T.: -0.007 min
Response: 133628
Conc: 1.11 ug/ml

Instrument :
FID_E
ClientSampleId :

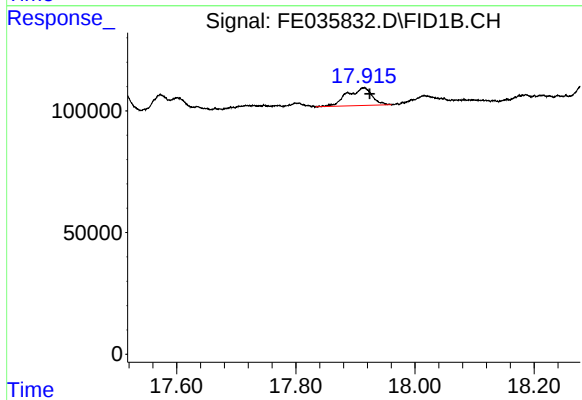

#18 n-Dotriacontane (C32)

R.T.: 17.914 min
Delta R.T.: -0.010 min
Response: 212412
Conc: 1.85 ug/ml

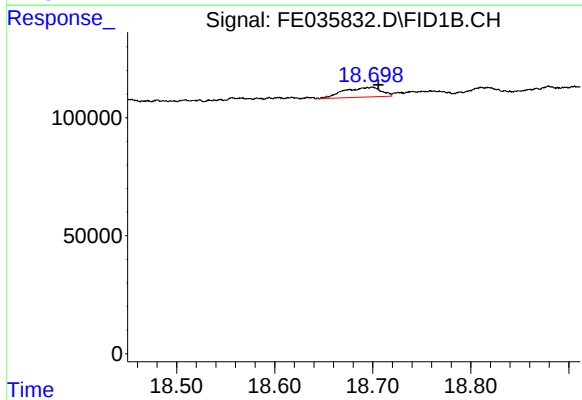

#19 n-Tetratriacontane (C34)

R.T.: 18.700 min
Delta R.T.: -0.006 min
Response: 109281
Conc: 1.01 ug/ml