

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE060220\  
 Data File : FE032111.D  
 Signal(s) : FID1B.CH  
 Acq On : 02 Jun 2020 10:51  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
 Quant Time: Jun 03 01:47:44 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE050720.M  
 Quant Title :  
 QLast Update : Thu May 07 13:58:31 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.118  | 8755268  | 21.661 ug/ml |
| 12) N-OCTACOSANE            | 16.523 | 9299907  | 21.416 ug/ml |
| 13) N-TRIACONTANE           | 17.409 | 517713   | 1.191 ug/ml  |
| 14) N-DOTRIACONTANE         | 18.240 | 577073   | 1.384 ug/ml  |
| 15) N-TETRATRIACONTANE      | 19.025 | 465164   | 1.177 ug/ml  |
| 16) N-HEXATRIACONTANE       | 19.766 | 348735   | 0.938 ug/ml  |
| 17) N-OCTATRIACONTANE       | 20.469 | 395062   | 1.175 ug/ml  |
| 18) N-TETRACONTANE          | 21.266 | 589319   | 1.742 ug/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE060220\  
Data File : FE032111.D  
Signal(s) : FID1B.CH  
Acq On : 02 Jun 2020 10:51  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jun 03 01:47:44 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE050720.M  
Quant Title :  
QLast Update : Thu May 07 13:58:31 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

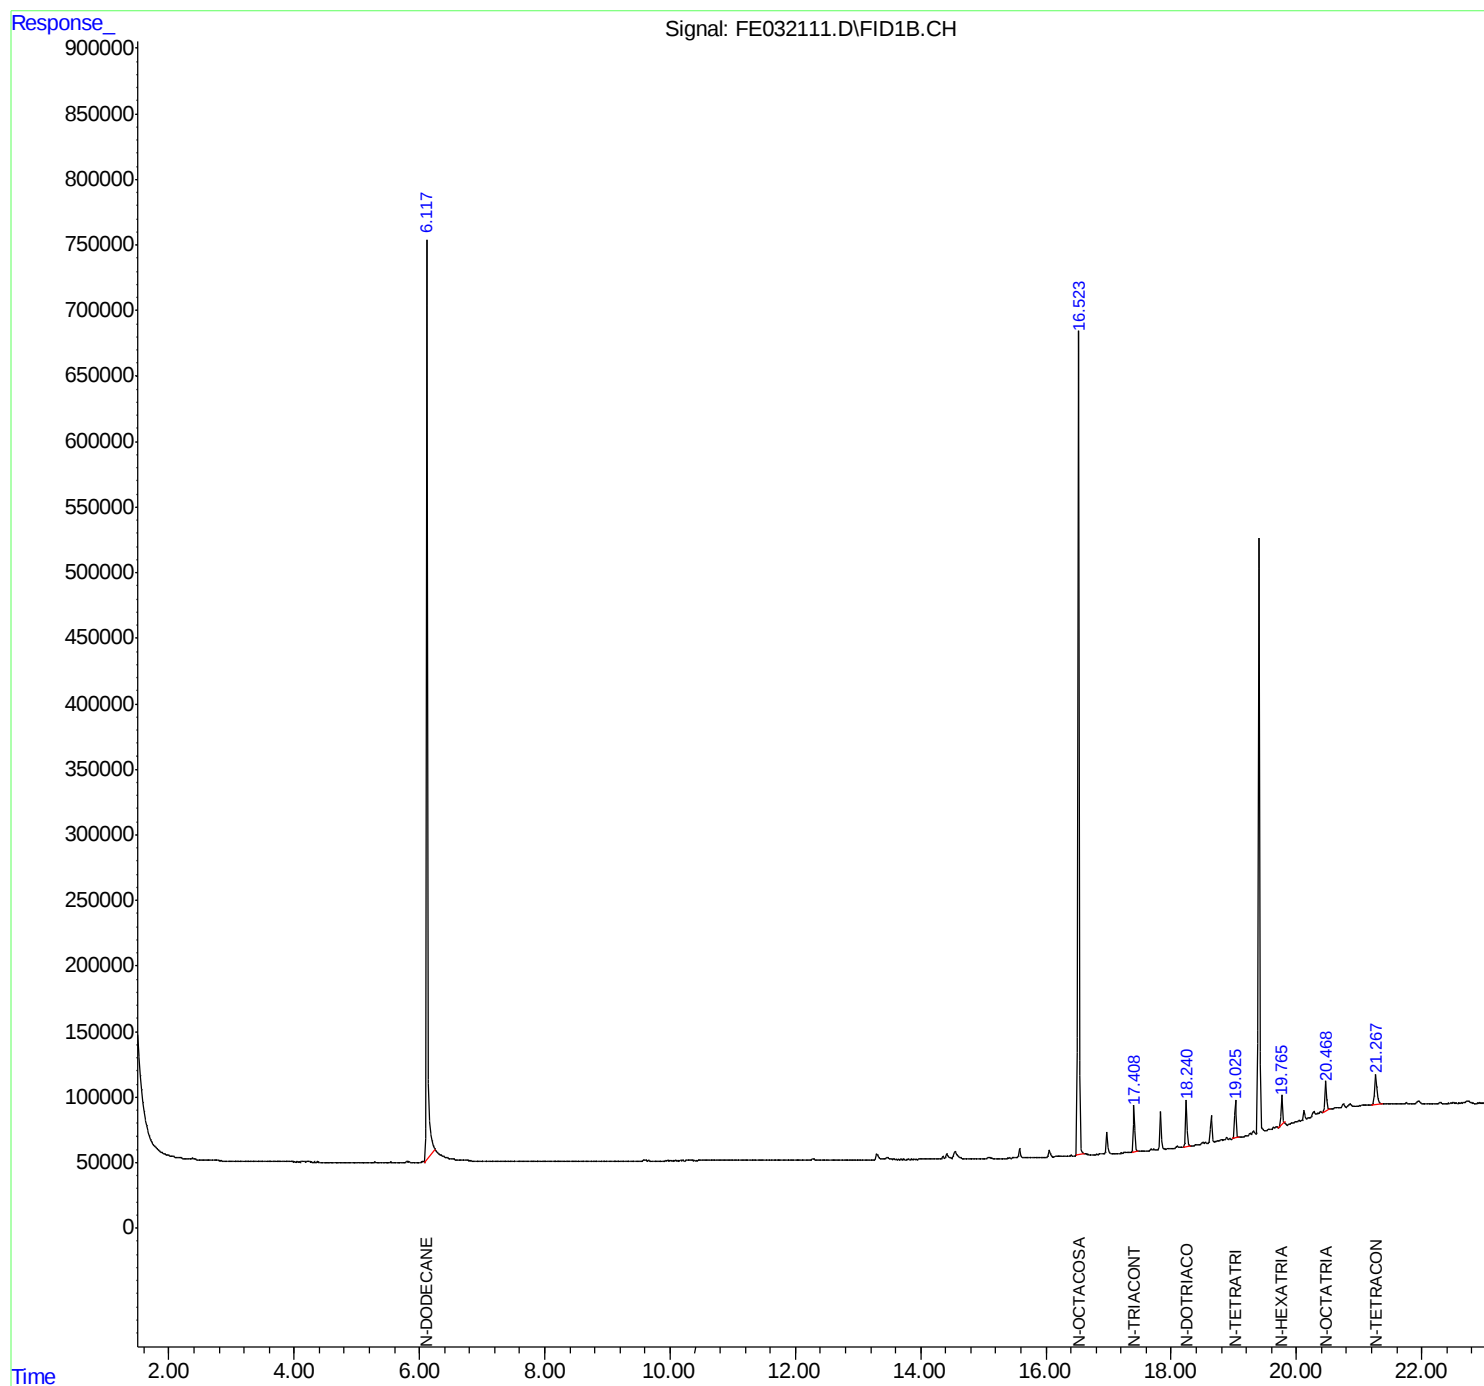

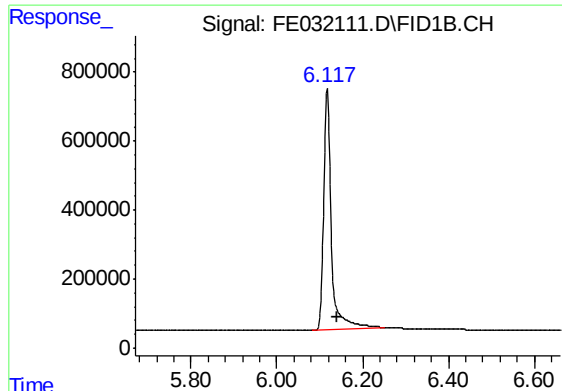


#3 N-DODECANE

R.T.: 6.118 min  
Delta R.T.: -0.024 min  
Response: 8755268  
Conc: 21.66 ug/ml

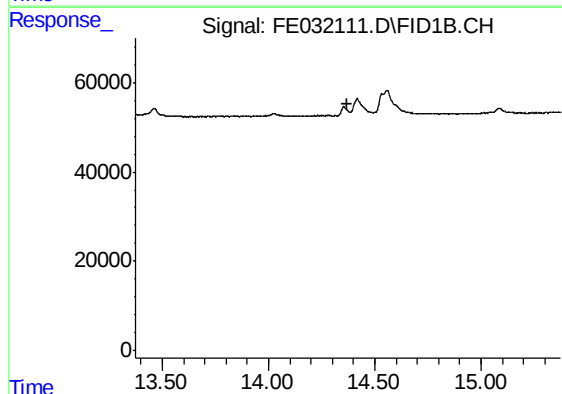


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.373 min  
Response: 0  
Conc: N.D.

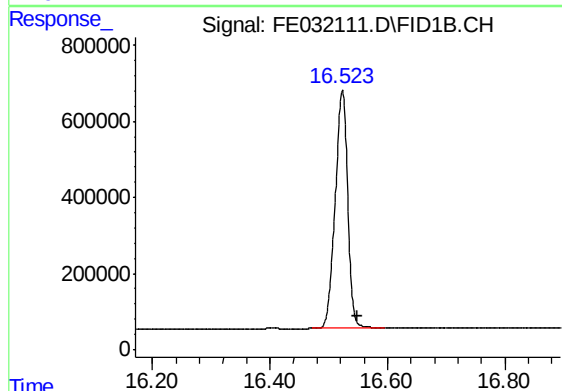


#12 N-OCTACOSANE

R.T.: 16.523 min  
Delta R.T.: -0.027 min  
Response: 9299907  
Conc: 21.42 ug/ml

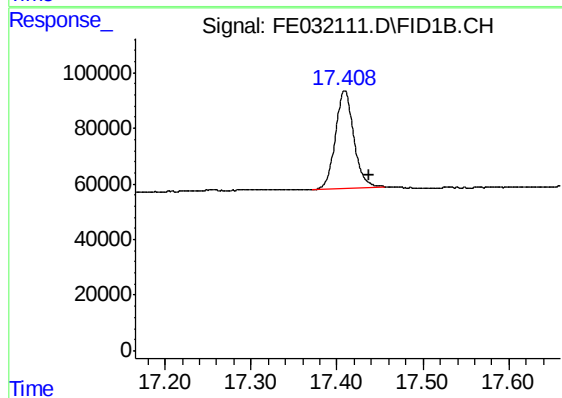


#13 N-TRIACONTANE

R.T.: 17.409 min  
Delta R.T.: -0.029 min  
Response: 517713  
Conc: 1.19 ug/ml

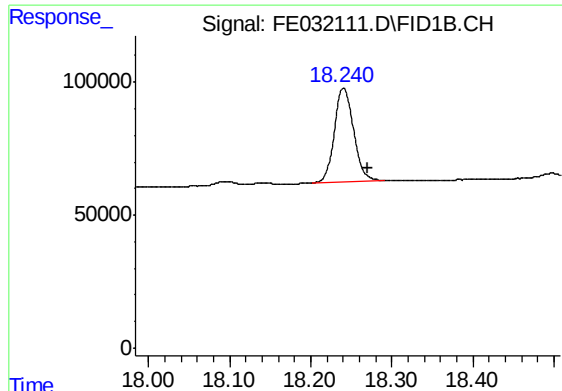


#14 N-DOTRIACONTANE

R.T.: 18.240 min  
Delta R.T.: -0.031 min  
Response: 577073  
Conc: 1.38 ug/ml

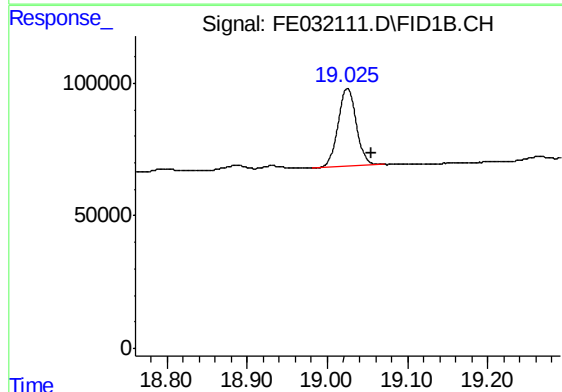


#15 N-TETRATRIACONTANE

R.T.: 19.025 min  
Delta R.T.: -0.029 min  
Response: 465164  
Conc: 1.18 ug/ml

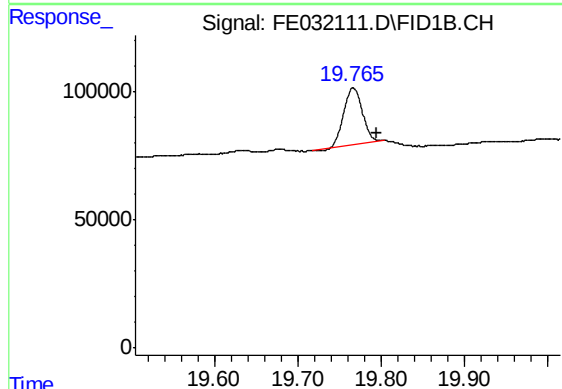


#16 N-HEXATRIACONTANE

R.T.: 19.766 min  
Delta R.T.: -0.029 min  
Response: 348735  
Conc: 0.94 ug/ml

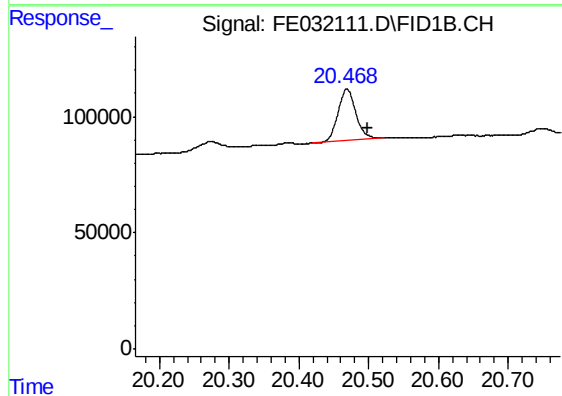

#17 N-OCTATRIACONTANE

R.T.: 20.469 min  
Delta R.T.: -0.029 min  
Response: 395062  
Conc: 1.18 ug/ml

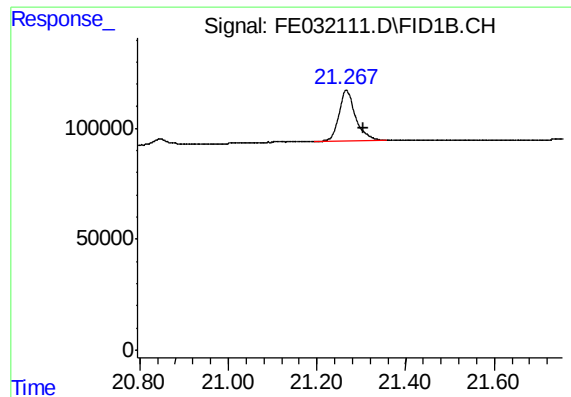

#18 N-TETRACONTANE

R.T.: 21.266 min  
Delta R.T.: -0.038 min  
Response: 589319  
Conc: 1.74 ug/ml