

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060220\
 Data File : FE032113.D
 Signal(s) : FID1B.CH
 Acq On : 02 Jun 2020 13:20
 Operator : DD\AJ
 Sample : PB129236BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 03 01:59:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050720.M
 Quant Title :
 QLast Update : Thu May 07 13:58:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.347	8108324	20.920 ug/ml
Target Compounds			
2) N-DECANE	4.119	8591138	21.551 ug/ml
3) N-DODECANE	6.116	8882118	21.974 ug/mlm
4) N-TETRADECANE	7.904	9435001	22.592 ug/mlm
5) N-HEXADECANE	9.502	9536357	22.291 ug/ml
6) N-OCTADECANE	10.942	9901408	22.073 ug/ml
7) N-EICOSANE	12.251	9679106	21.825 ug/ml
8) N-DOCOSANE	13.449	9666483	21.568 ug/ml
10) N-TETRACOSANE	14.553	9537449	21.547 ug/ml
11) N-HEXACOSANE	15.574	9103213	20.806 ug/ml
12) N-OCTACOSANE	16.525	8808343	20.284 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060220\
Data File : FE032113.D
Signal(s) : FID1B.CH
Acq On : 02 Jun 2020 13:20
Operator : DD\AJ
Sample : PB129236BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 03 01:59:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050720.M
Quant Title :
QLast Update : Thu May 07 13:58:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

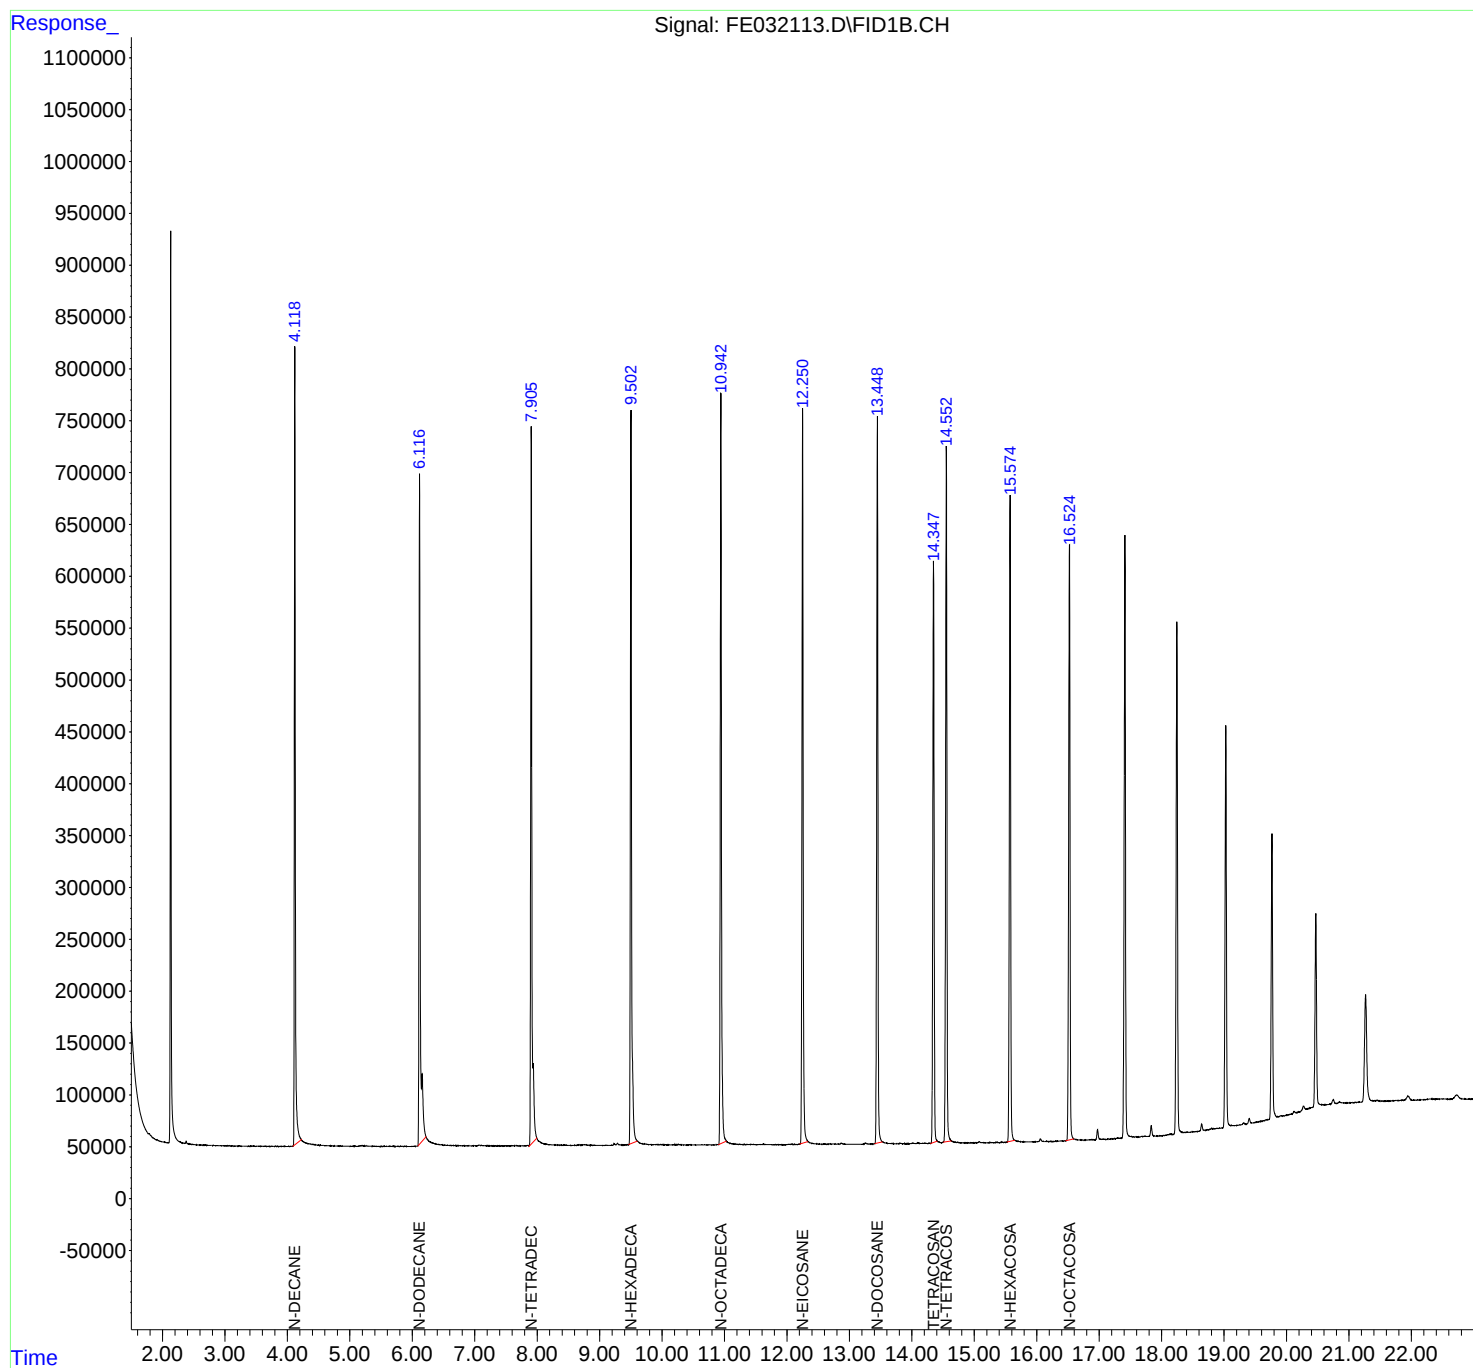

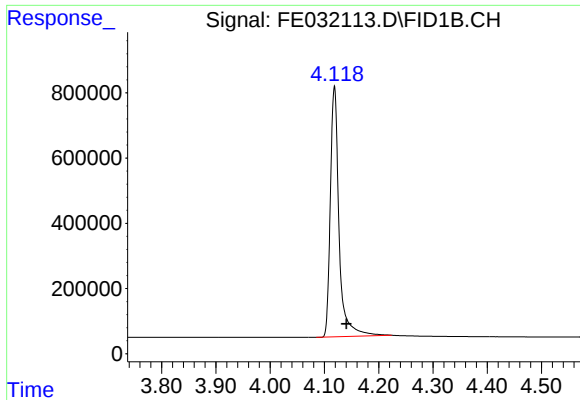


#2 N-DECANE

R.T.: 4.119 min
Delta R.T.: -0.022 min
Response: 8591138
Conc: 21.55 ug/ml

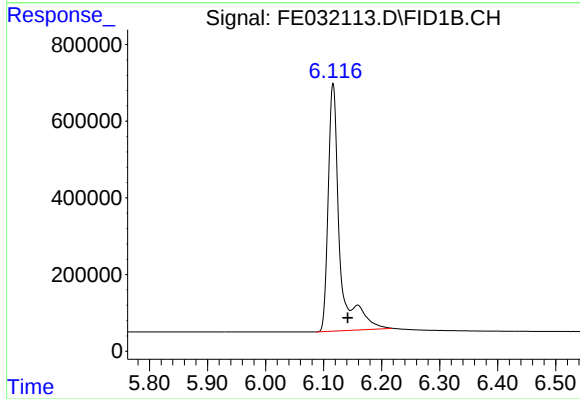


#3 N-DODECANE

R.T.: 6.116 min
Delta R.T.: -0.026 min
Response: 8882118
Conc: 21.97 ug/ml m

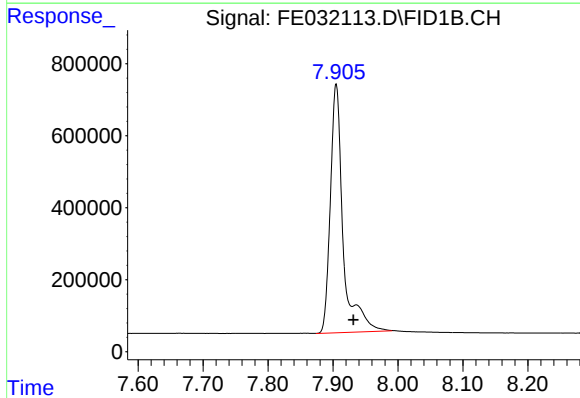


#4 N-TETRADECANE

R.T.: 7.904 min
Delta R.T.: -0.027 min
Response: 9435001
Conc: 22.59 ug/ml m

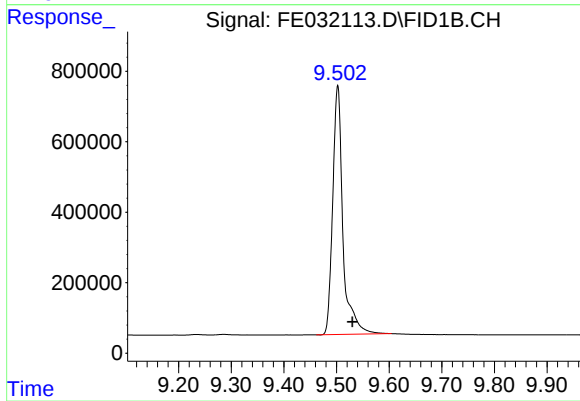


#5 N-HEXADECANE

R.T.: 9.502 min
Delta R.T.: -0.027 min
Response: 9536357
Conc: 22.29 ug/ml

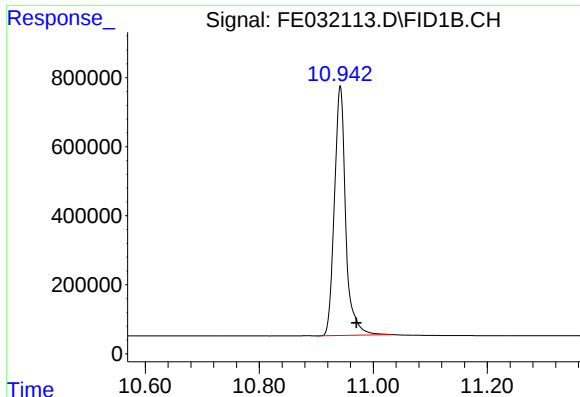


#6 N-OCTADECANE

R.T.: 10.942 min
Delta R.T.: -0.028 min
Response: 9901408
Conc: 22.07 ug/ml

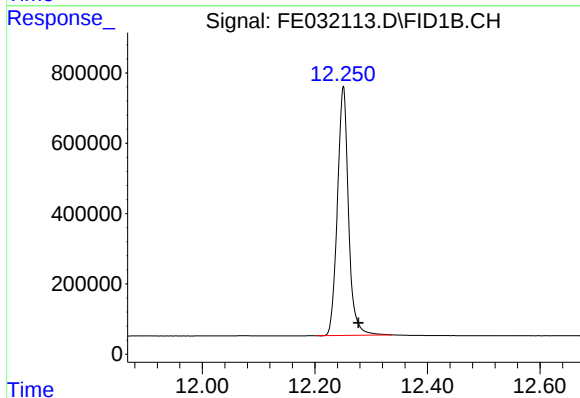


#7 N-EICOSANE

R.T.: 12.251 min
Delta R.T.: -0.027 min
Response: 9679106
Conc: 21.83 ug/ml

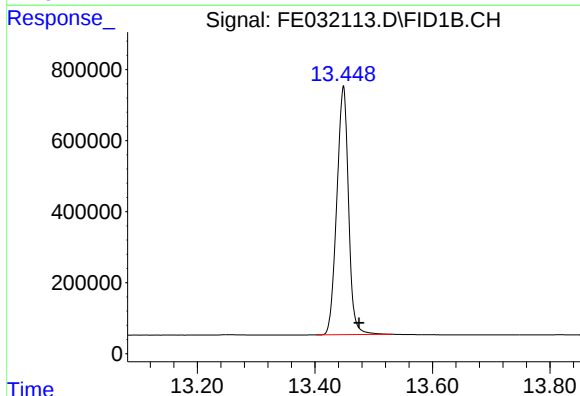


#8 N-DOCOSANE

R.T.: 13.449 min
Delta R.T.: -0.026 min
Response: 9666483
Conc: 21.57 ug/ml

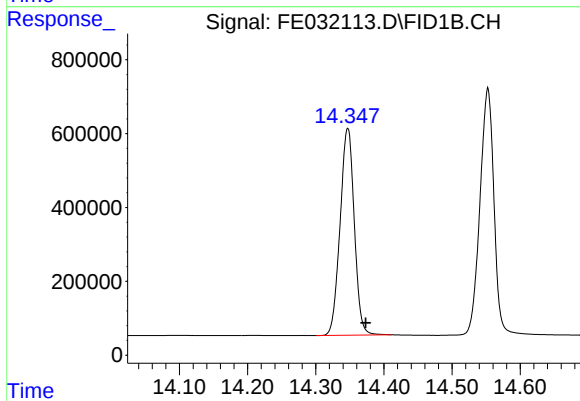


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.347 min
Delta R.T.: -0.026 min
Response: 8108324
Conc: 20.92 ug/ml

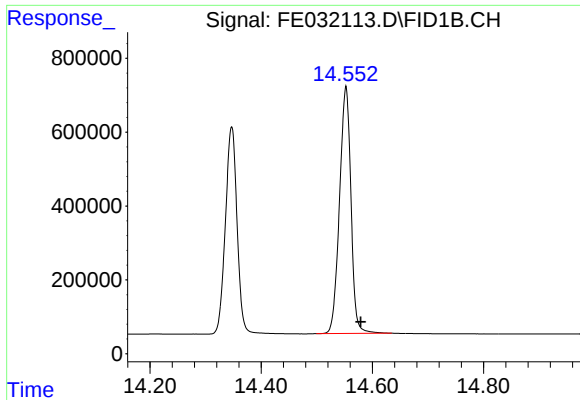


#10 N-TETRACOSANE

R.T.: 14.553 min
Delta R.T.: -0.027 min
Response: 9537449
Conc: 21.55 ug/ml

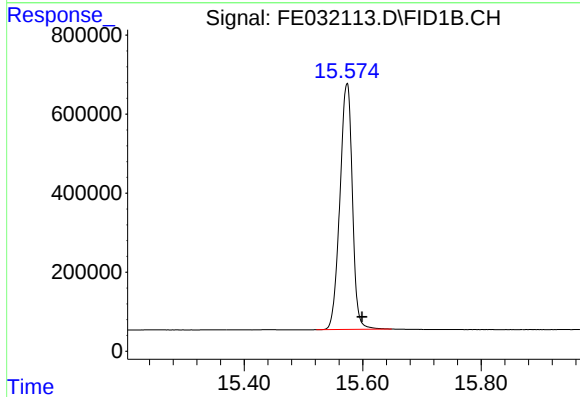

#11 N-HEXACOSANE

R.T.: 15.574 min
Delta R.T.: -0.025 min
Response: 9103213
Conc: 20.81 ug/ml

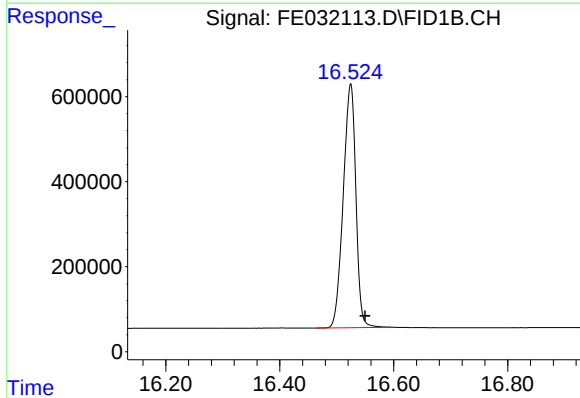

#12 N-OCTACOSANE

R.T.: 16.525 min
Delta R.T.: -0.025 min
Response: 8808343
Conc: 20.28 ug/ml