

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060222AL\
 Data File : FE035883.D
 Signal(s) : FID1B.CH
 Acq On : 03 Jun 2022 2:40
 Operator : YP\AJ
 Sample : N3069-02D
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 03 04:11:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 03:24:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.384	4163326	39.801 ug/ml
Spiked Amount 50.000		Recovery =	79.60%
Target Compounds			
4) T n-Dodecane (C12)	5.805	165488	1.381 ug/ml
6) T n-Tetradecane (C14)	7.594	124660	1.046 ug/ml
7) T n-Hexadecane (C16)	9.191	162203	1.360 ug/ml
8) T n-Octadecane (C18)	10.629	139944	1.167 ug/ml
10) T n-Eicosane (C20)	11.936	95728	<MDL ug/ml
11) T n-Heneicosane (C21)	12.546	68121	<MDL ug/ml
13) T n-Docosane (C22)	13.131	52785	<MDL ug/ml
17) T n-Tricontane (C30)	17.084	71203	<MDL ug/ml
18) T n-Dotriacontane (C32)	17.915	65341	<MDL ug/ml
19) T n-Tetratriacontane (C34)	18.697	43384	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060222AL\
Data File : FE035883.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2022 2:40
Operator : YP\AJ
Sample : N3069-02D
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 03 04:11:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
Quant Title : GC Extractables
QLast Update : Wed May 11 03:24:10 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

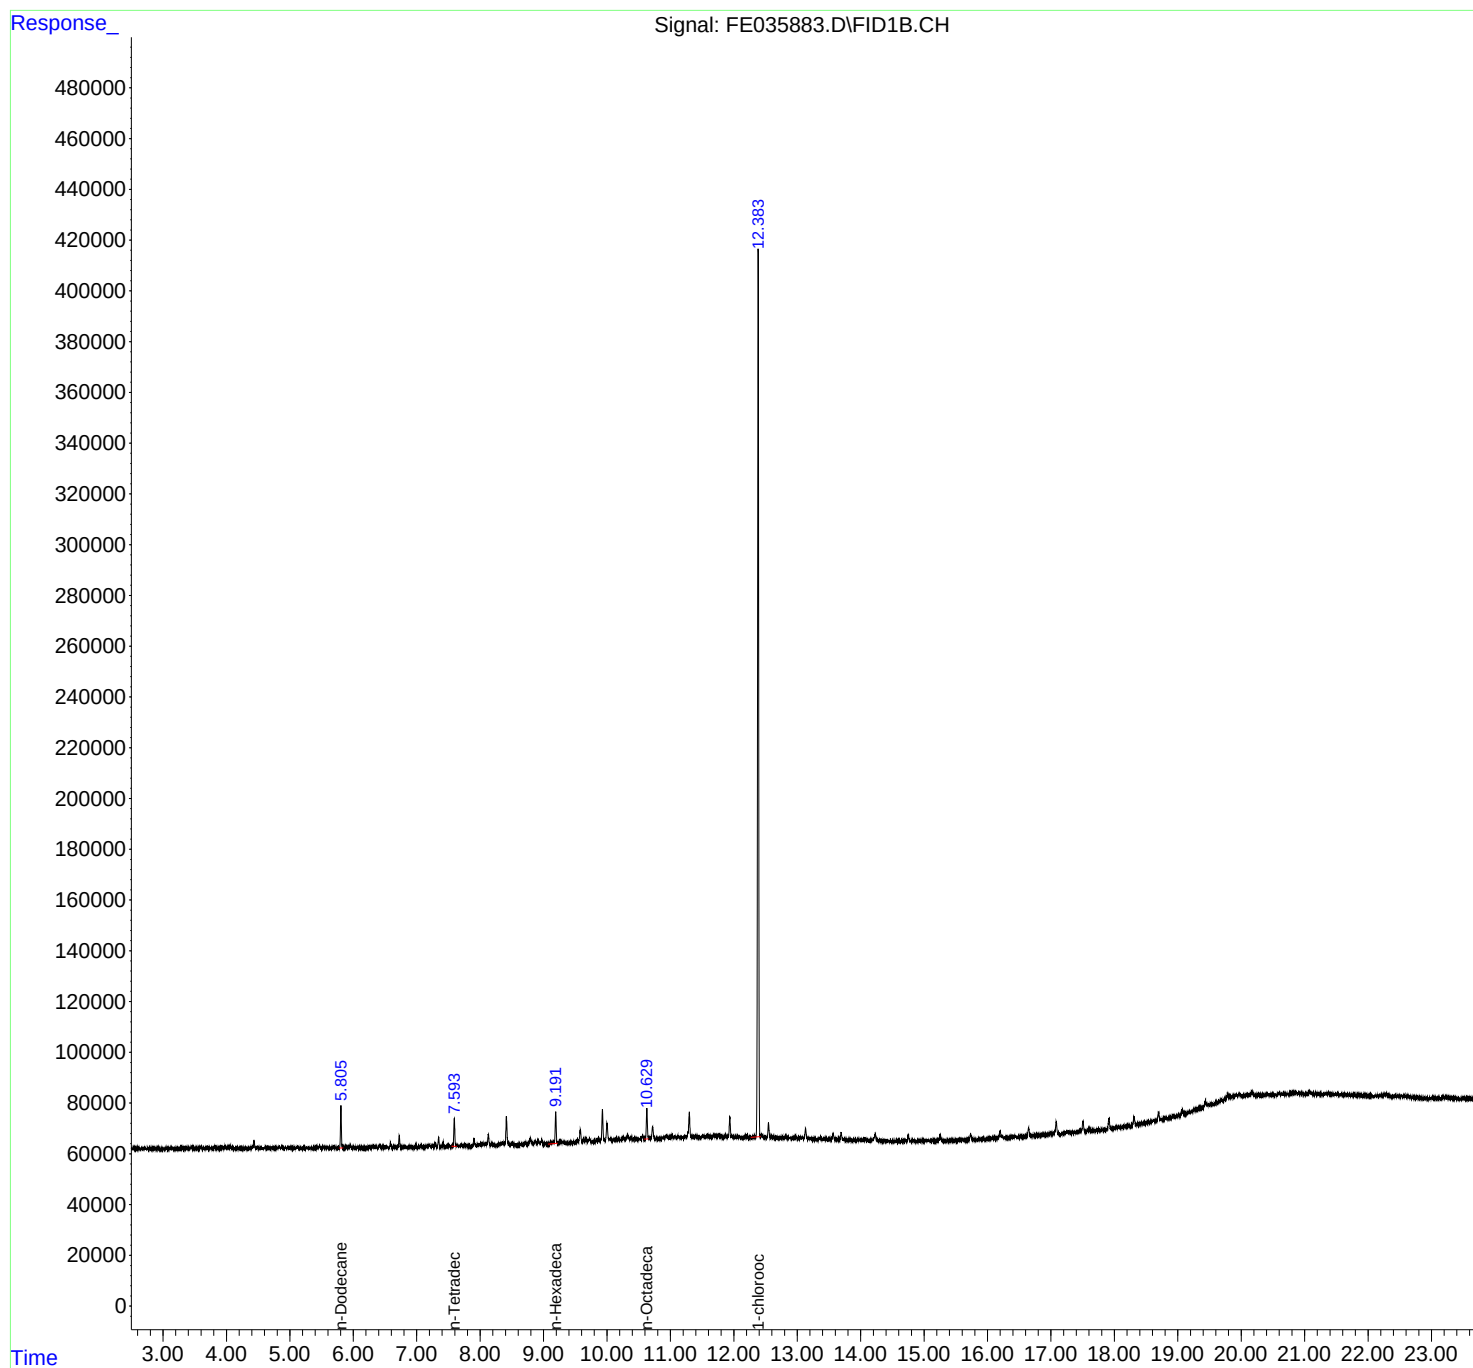


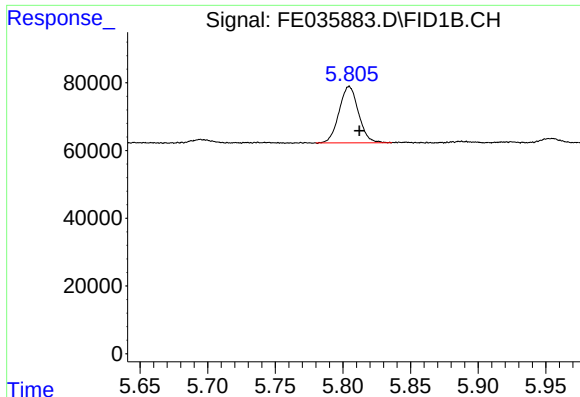

#4 n-Dodecane (C12)


R.T.: 5.805 min
Delta R.T.: -0.008 min
Response: 165488
Conc: 1.38 ug/ml

Instrument :
FID_E
ClientSampleId :

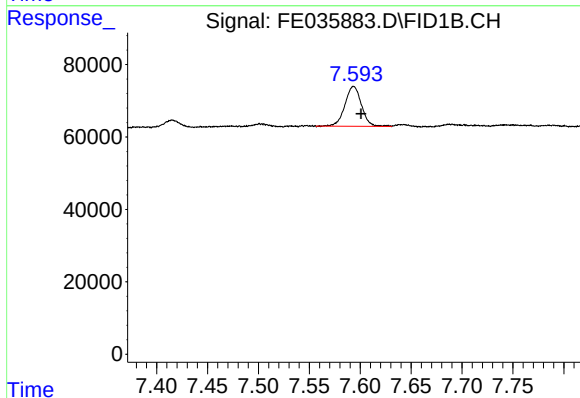


#6 n-Tetradecane (C14)

R.T.: 7.594 min
Delta R.T.: -0.007 min
Response: 124660
Conc: 1.05 ug/ml

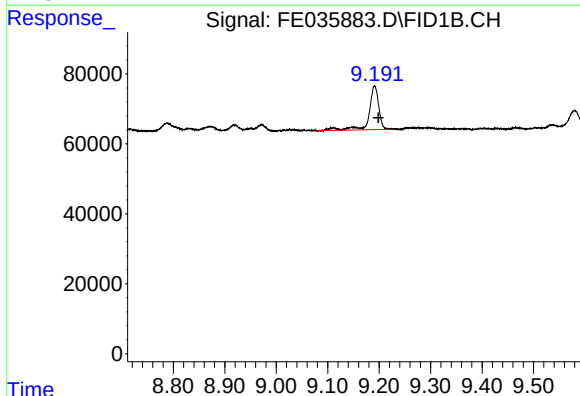


#7 n-Hexadecane (C16)

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 162203
Conc: 1.36 ug/ml

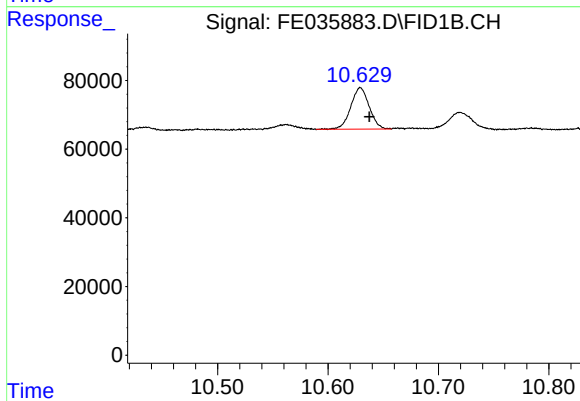

#8 n-Octadecane (C18)


R.T.: 10.629 min
Delta R.T.: -0.008 min
Response: 139944
Conc: 1.17 ug/ml

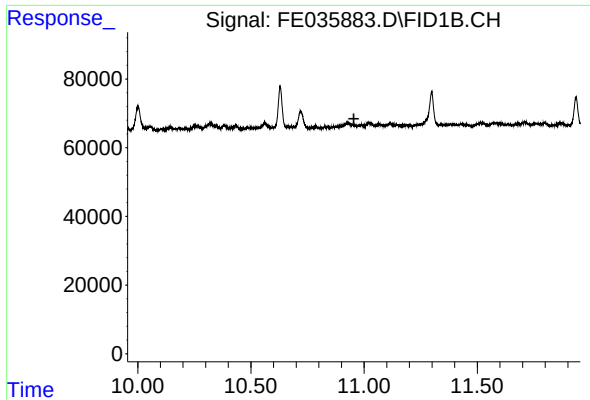

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 10.955 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

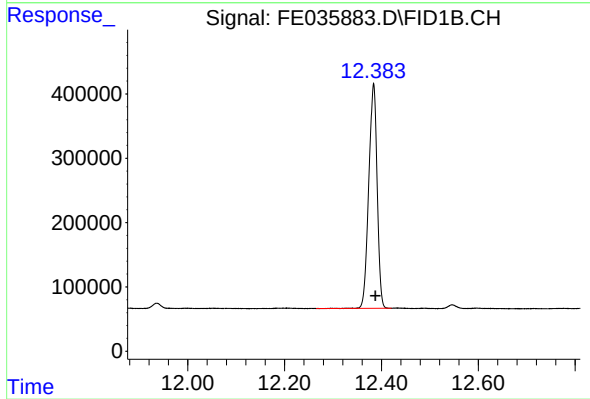

#12 1-chlorooctadecane (SURR)

R.T.: 12.384 min
Delta R.T.: -0.004 min
Response: 4163326
Conc: 39.80 ug/ml