

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
 Data File : FE033858.D
 Signal(s) : FID1B.CH
 Acq On : 03 Jun 2021 7:25
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 03:26:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.598	221778	0.483 ug/ml
8) N-DOCOSANE	13.803	229241	0.497 ug/ml
10) N-TETRACOSANE	14.888	451581	0.978 ug/ml
12) N-OCTACOSANE	16.883	251686	0.549 ug/ml
13) N-TRIACONTANE	17.773	326520	0.716 ug/ml
14) N-DOTRIACONTANE	18.612	537154	1.207 ug/ml
15) N-TETRATRIACONTANE	19.394	190837	0.444 ug/ml
16) N-HEXATRIACONTANE	20.127	171202	0.427 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
Data File : FE033858.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2021 7:25
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 04 03:26:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

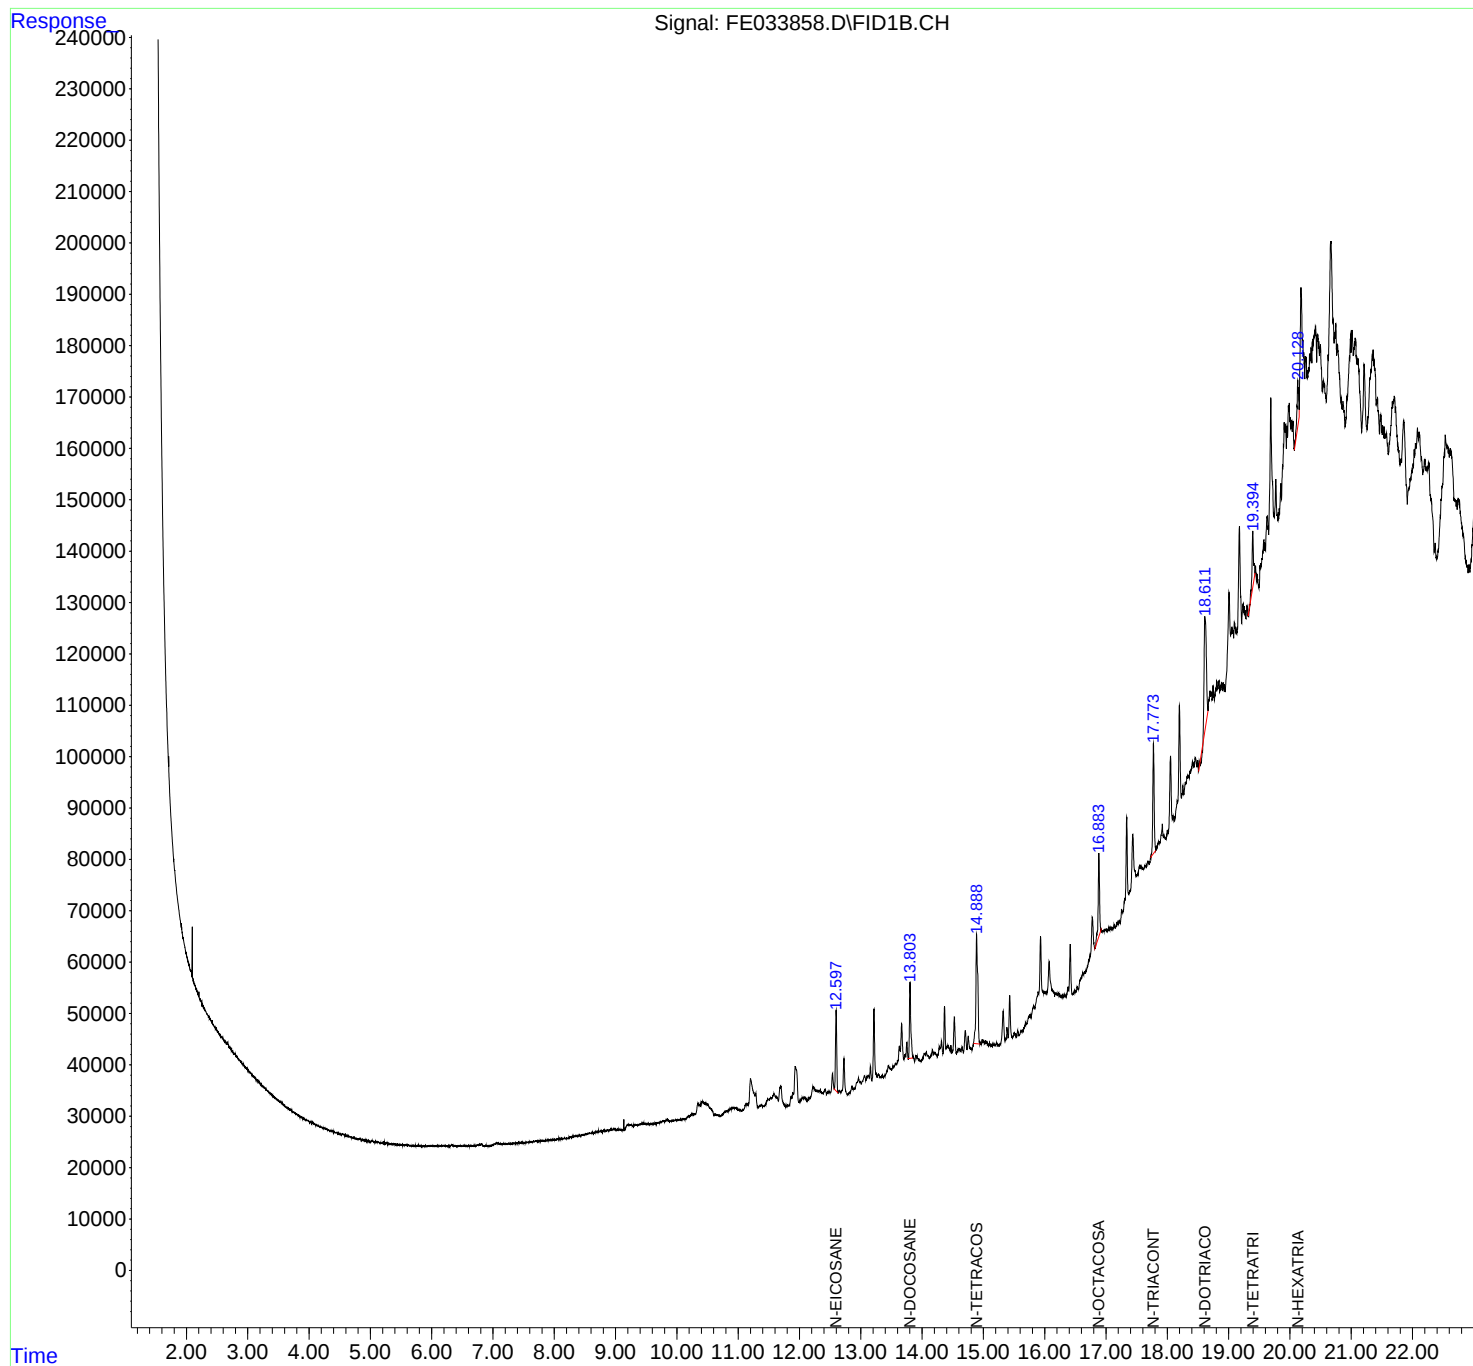


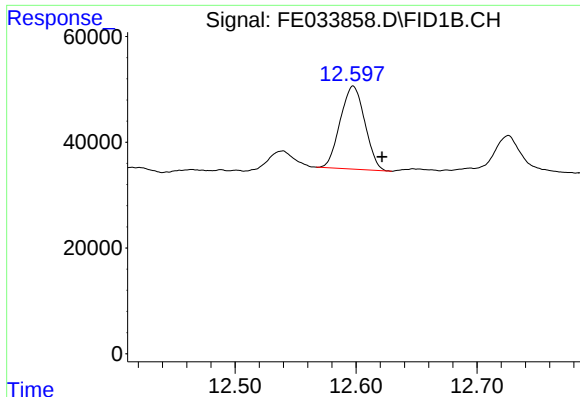

#7 N-EICOSANE


R.T.: 12.598 min
Delta R.T.: -0.024 min
Response: 221778
Conc: 0.48 ug/ml

Instrument :
FID_E
ClientSampleId :

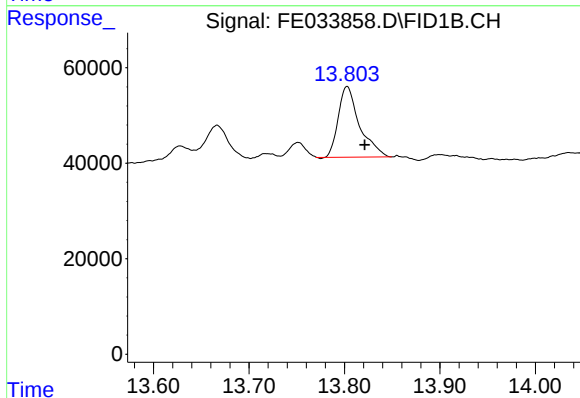


#8 N-DOCOSANE

R.T.: 13.803 min
Delta R.T.: -0.018 min
Response: 229241
Conc: 0.50 ug/ml

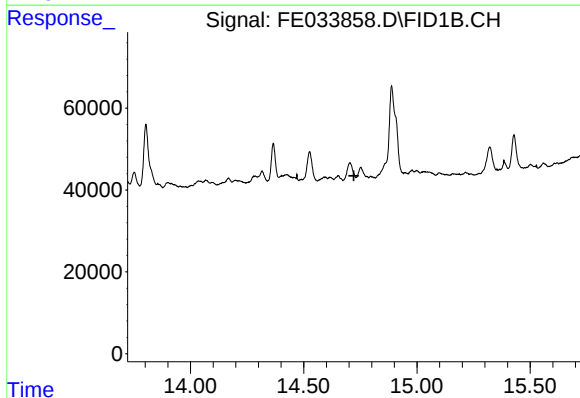


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.721 min
Response: 0
Conc: N.D.

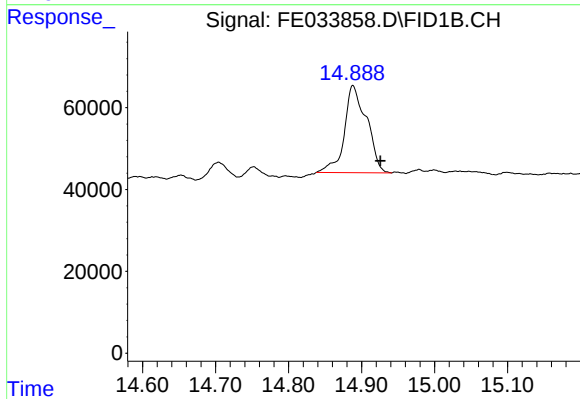

#10 N-TETRACOSANE


R.T.: 14.888 min
Delta R.T.: -0.038 min
Response: 451581
Conc: 0.98 ug/ml

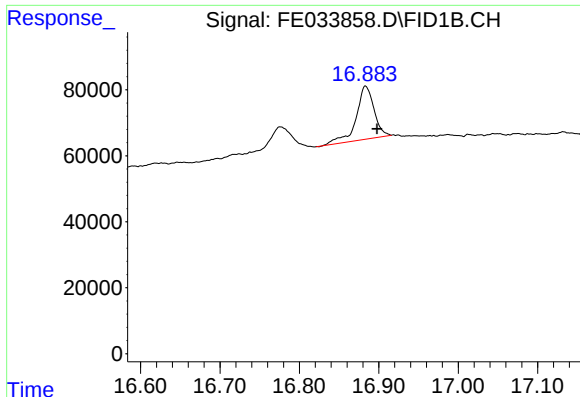

#12 N-OCTACOSANE


R.T.: 16.883 min
Delta R.T.: -0.015 min
Response: 251686
Conc: 0.55 ug/ml

Instrument :
FID_E
ClientSampleId :

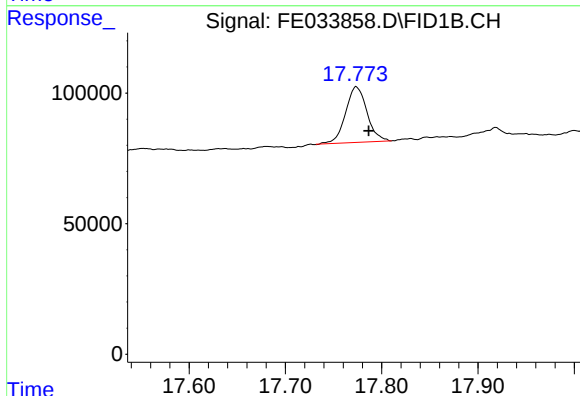


#13 N-TRIACONTANE

R.T.: 17.773 min
Delta R.T.: -0.013 min
Response: 326520
Conc: 0.72 ug/ml

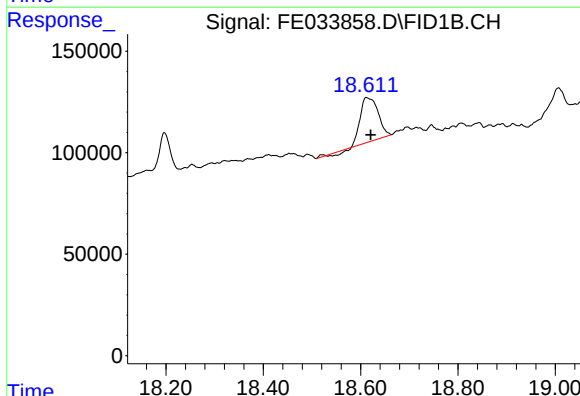


#14 N-DOTRIACONTANE

R.T.: 18.612 min
Delta R.T.: -0.009 min
Response: 537154
Conc: 1.21 ug/ml

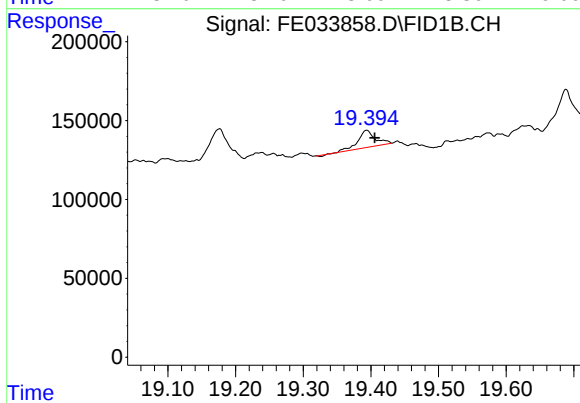

#15 N-TETRATRIACONTANE

R.T.: 19.394 min
Delta R.T.: -0.012 min
Response: 190837
Conc: 0.44 ug/ml

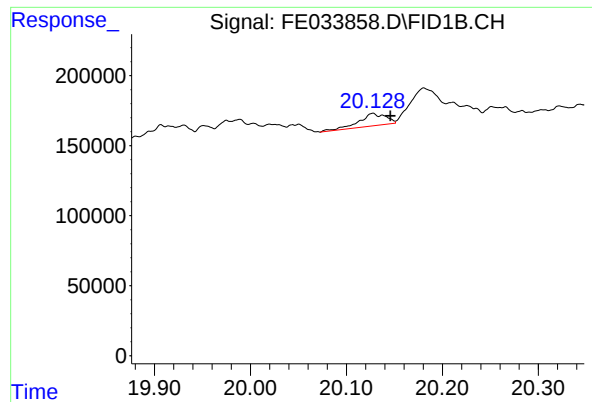

#16 N-HEXATRIACONTANE

R.T.: 20.127 min
Delta R.T.: -0.018 min
Response: 171202
Conc: 0.43 ug/ml

Instrument :
FID_E
ClientSampleId :