

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
 Data File : FE033871.D
 Signal(s) : FID1B.CH
 Acq On : 03 Jun 2021 14:57
 Operator : DD\AJ
 Sample : M2580-07 50X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 03:29:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.686f	542585	1.182 ug/ml
10) N-TETRACOSANE	14.908	318829	0.691 ug/ml
13) N-TRIACONTANE	17.789	274745	0.603 ug/ml
14) N-DOTRIACONTANE	18.623	167424	0.376 ug/ml
15) N-TETRATRIACONTANE	19.408	4239	0.010 ug/ml
16) N-HEXATRIACONTANE	20.151	555292	1.385 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
Data File : FE033871.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2021 14:57
Operator : DD\AJ
Sample : M2580-07 50X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 03:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

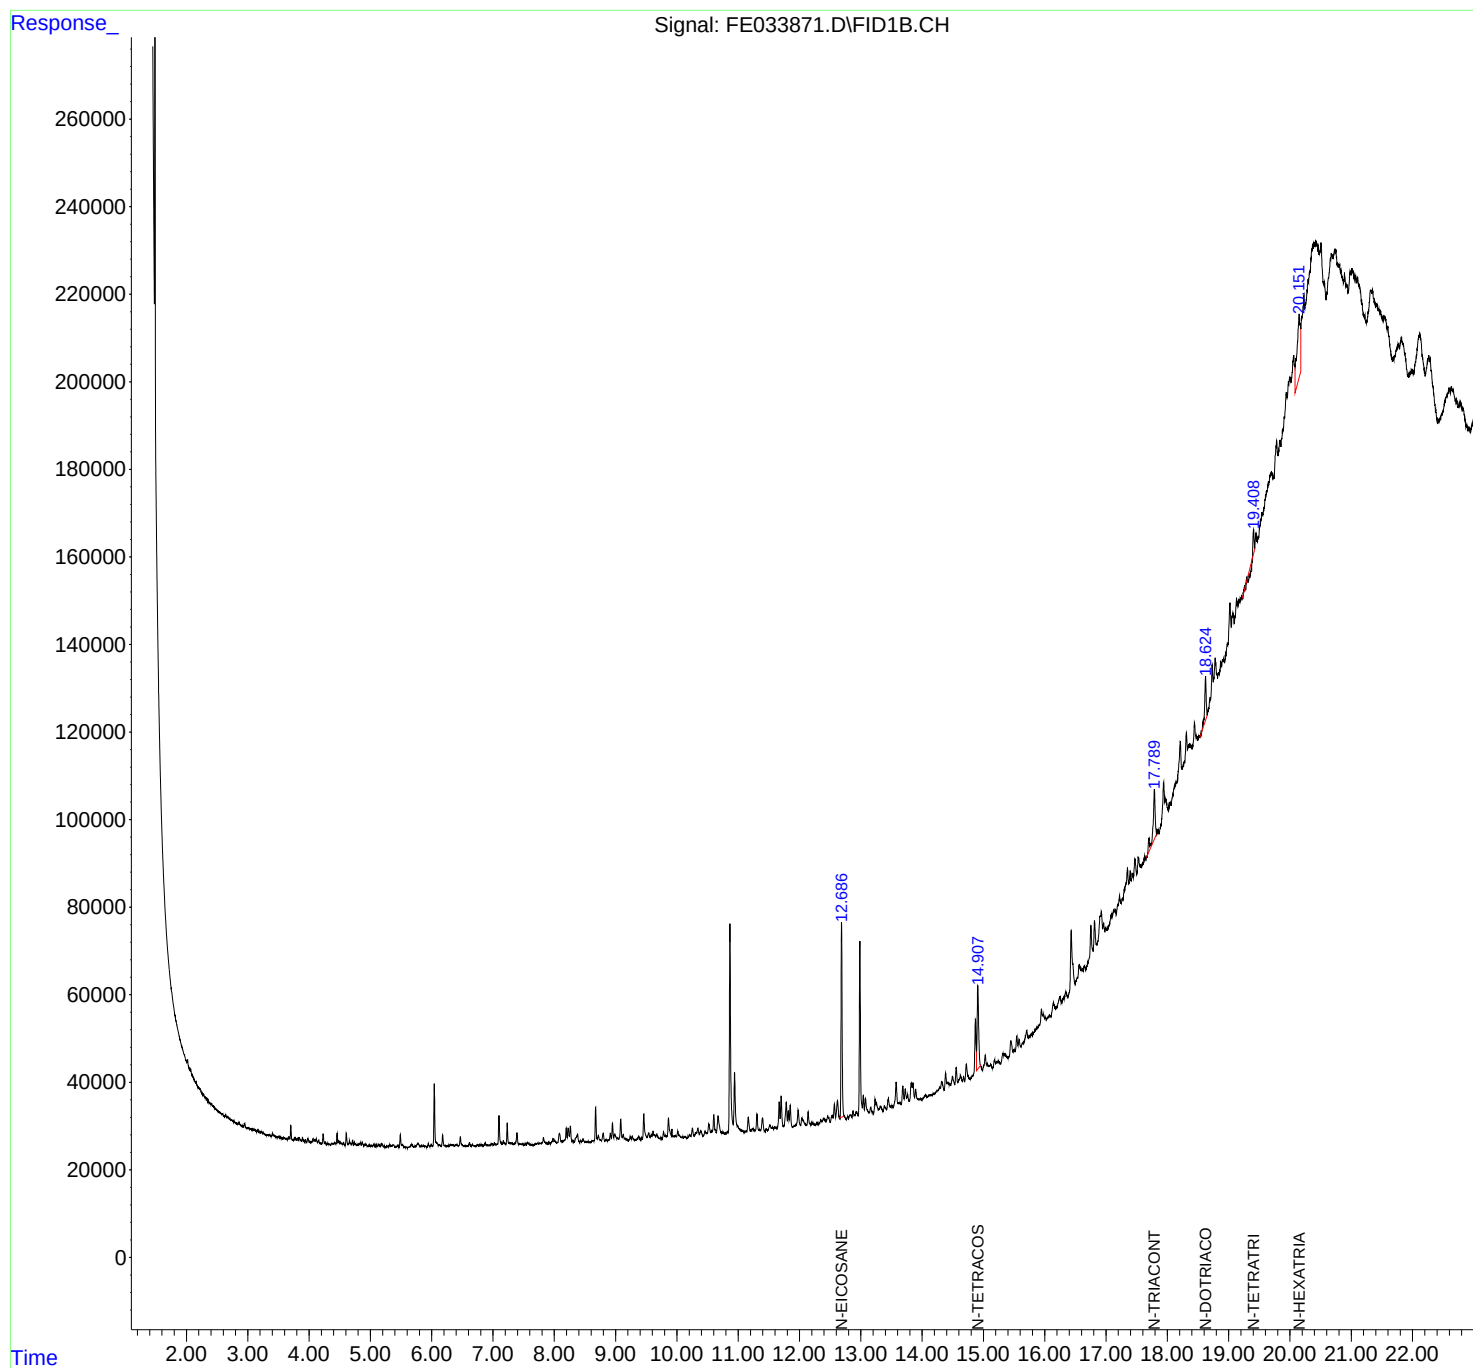


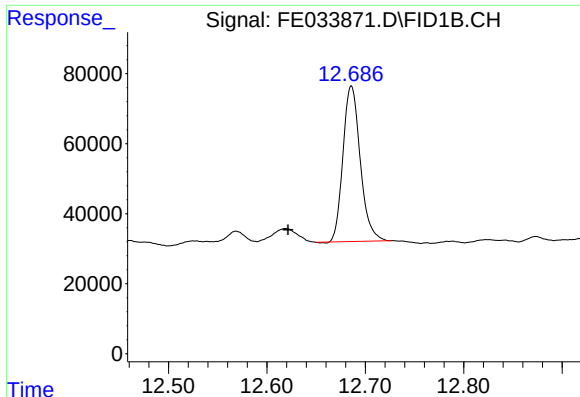

#7 N-EICOSANE


R.T.: 12.686 min
Delta R.T.: 0.064 min
Response: 542585
Conc: 1.18 ug/ml

Instrument :
FID_E
ClientSampleId :

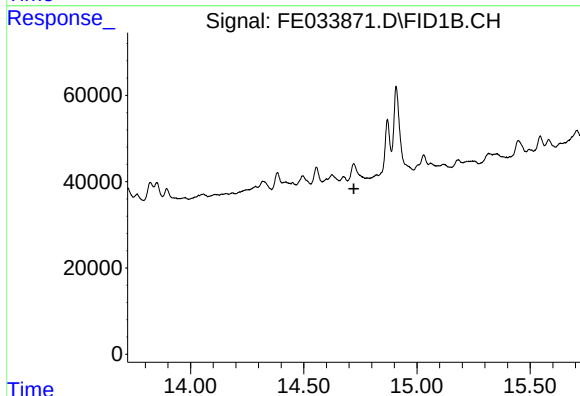


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.721 min
Response: 0
Conc: N.D.

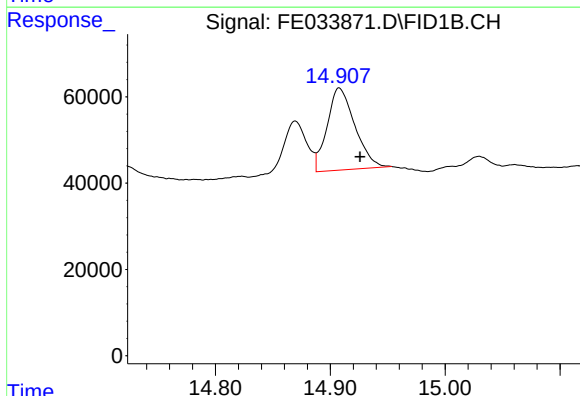


#10 N-TETRACOSANE

R.T.: 14.908 min
Delta R.T.: -0.018 min
Response: 318829
Conc: 0.69 ug/ml

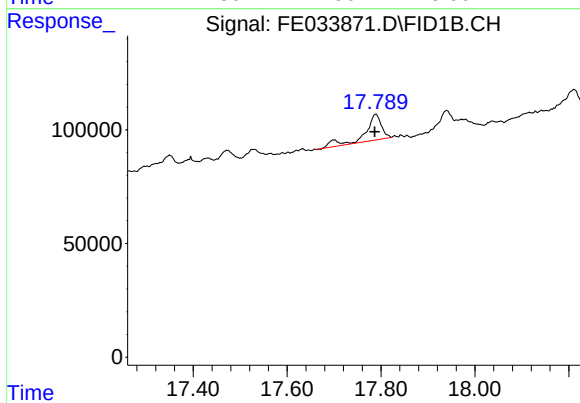

#13 N-TRIACONTANE


R.T.: 17.789 min
Delta R.T.: 0.002 min
Response: 274745
Conc: 0.60 ug/ml

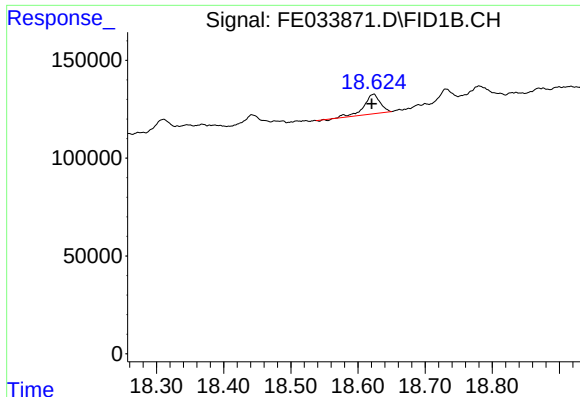

#14 N-DOTRIACONTANE


R.T.: 18.623 min
Delta R.T.: 0.003 min
Response: 167424
Conc: 0.38 ug/ml

Instrument :
FID_E
ClientSampleId :

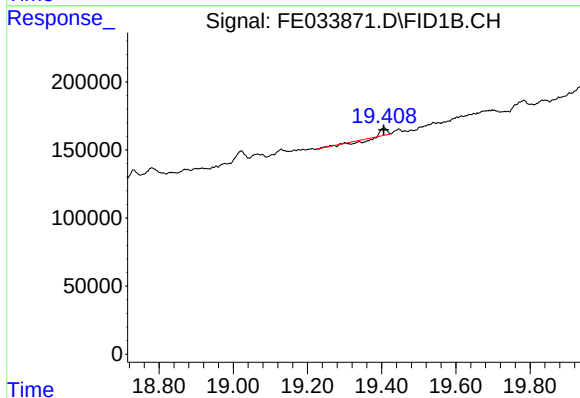

#15 N-TETRATRIACONTANE

R.T.: 19.408 min
Delta R.T.: 0.002 min
Response: 4239
Conc: 0.01 ug/ml

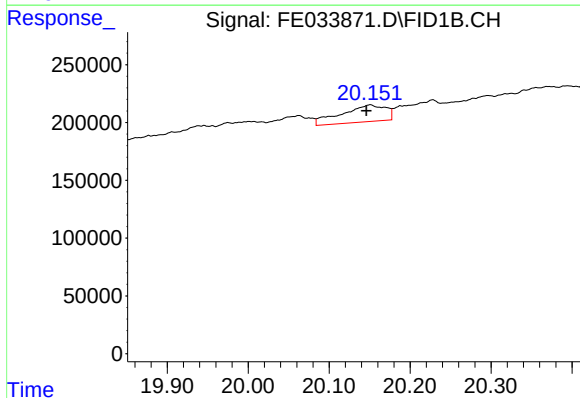

#16 N-HEXATRIACONTANE

R.T.: 20.151 min
Delta R.T.: 0.005 min
Response: 555292
Conc: 1.39 ug/ml