

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
 Data File : FE033874.D
 Signal(s) : FID1B.CH
 Acq On : 03 Jun 2021 16:41
 Operator : DD\AJ
 Sample : M2580-02 50X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 03:29:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.786	290604	0.637 ug/ml
16) N-HEXATRIACONTANE	20.143	93288	0.233 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
Data File : FE033874.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2021 16:41
Operator : DD\AJ
Sample : M2580-02 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 03:29:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

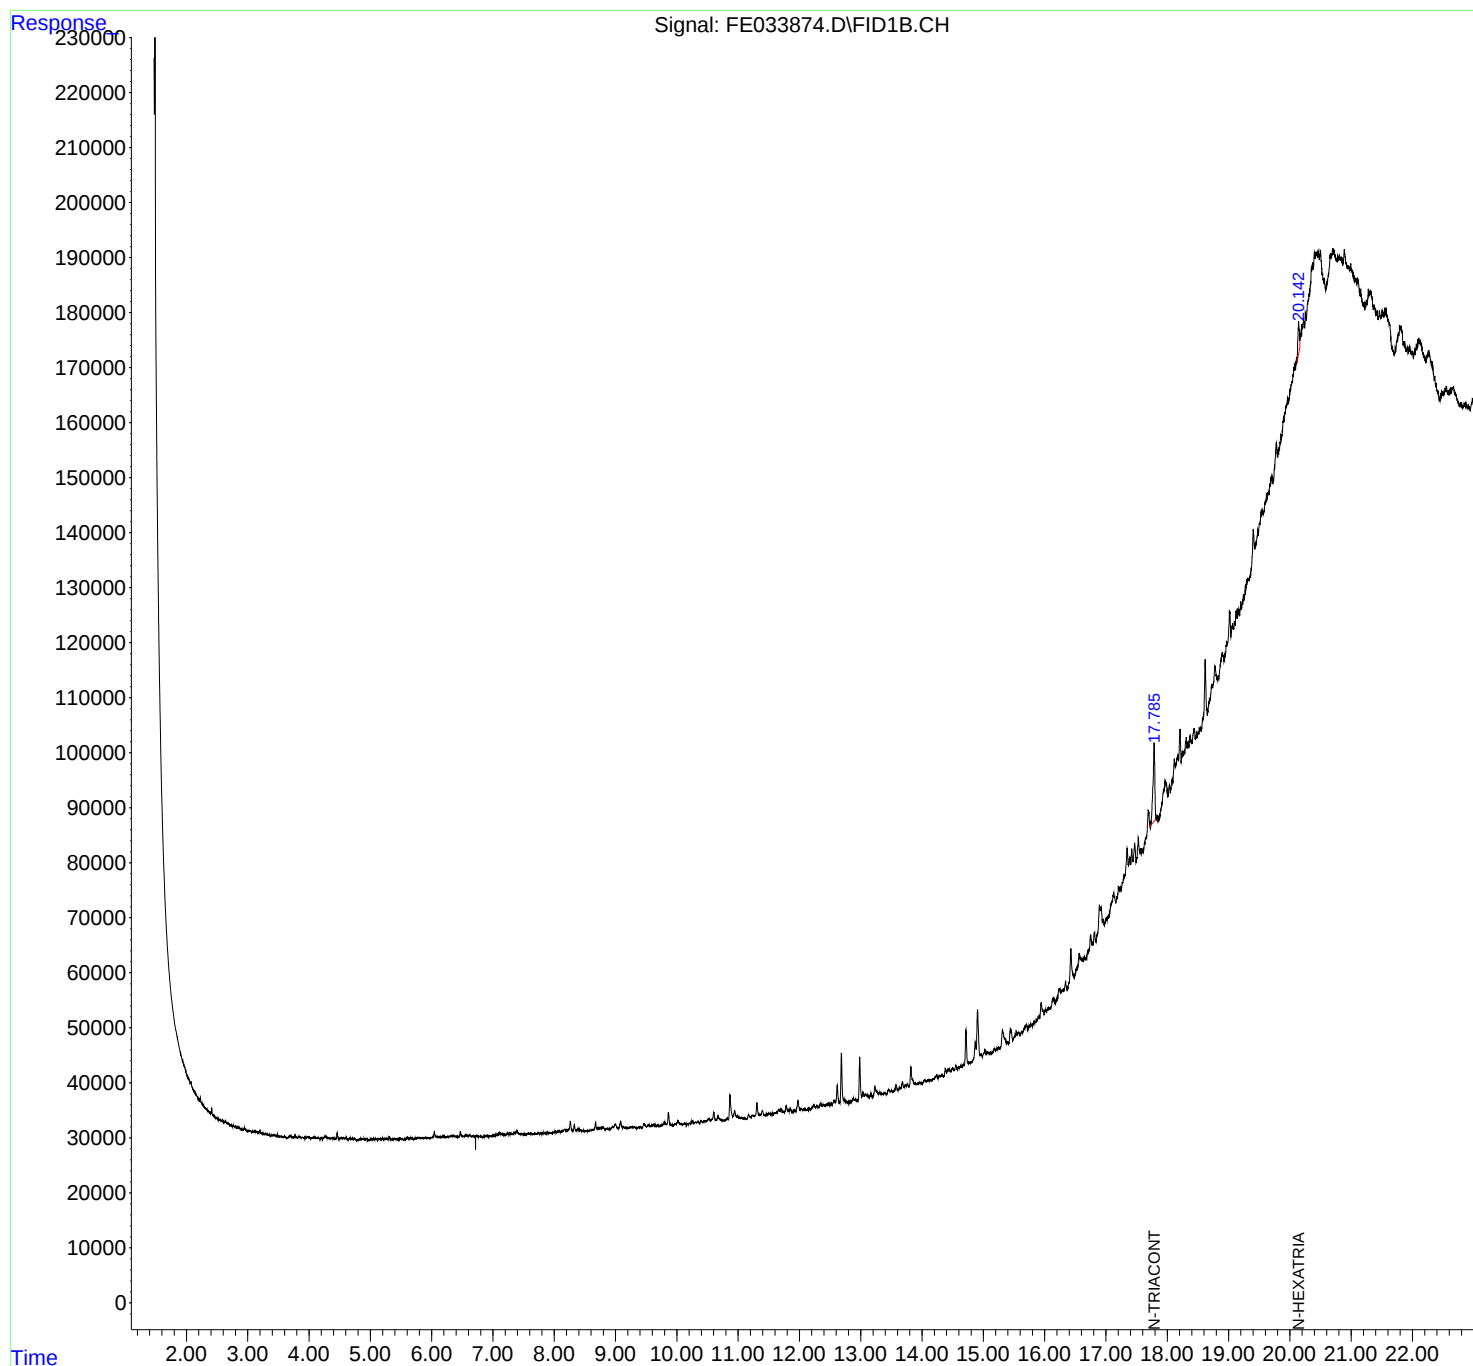


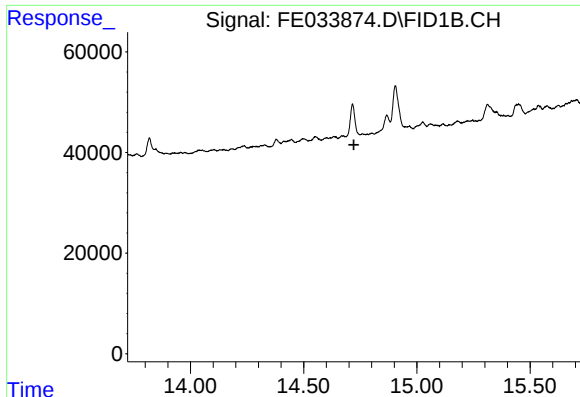

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.721 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

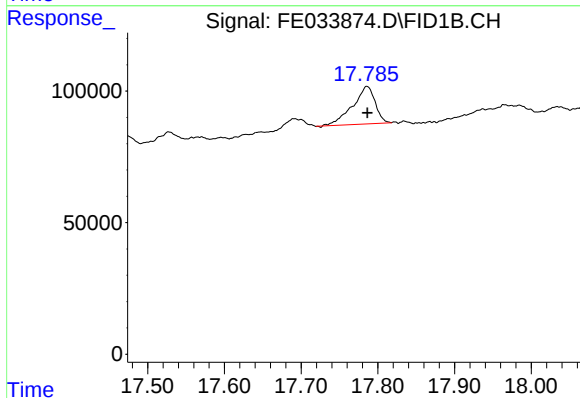

#13 N-TRIACONTANE

R.T.: 17.786 min
Delta R.T.: -0.001 min
Response: 290604
Conc: 0.64 ug/ml

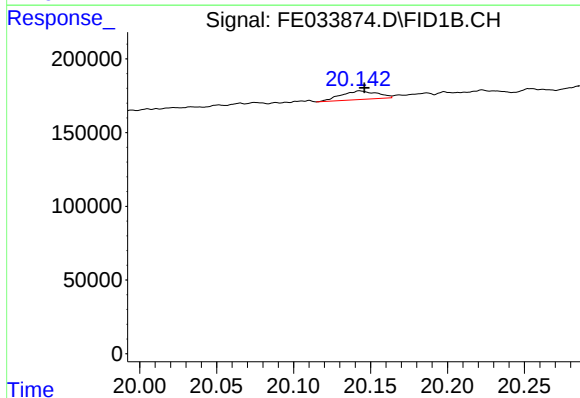

#16 N-HEXATRIACONTANE

R.T.: 20.143 min
Delta R.T.: -0.003 min
Response: 93288
Conc: 0.23 ug/ml