

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
Data File : FE033874.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2021 16:41
Operator : DD\AJ
Sample : M2580-02 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
18-B1(2-4)

Manual Integrations
APPROVED

Ankita
6/4/2021 3:31:16 PM

Integration File: autoint1.e
Quant Time: Jun 04 03:29:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060321\
Data File : FE033874.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2021 16:41
Operator : DD\AJ
Sample : M2580-02 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
18-B1(2-4)


Manual Integrations
APPROVED

Ankita
6/4/2021 3:31:16 PM

Integration File: autoint1.e
Quant Time: Jun 04 03:29:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

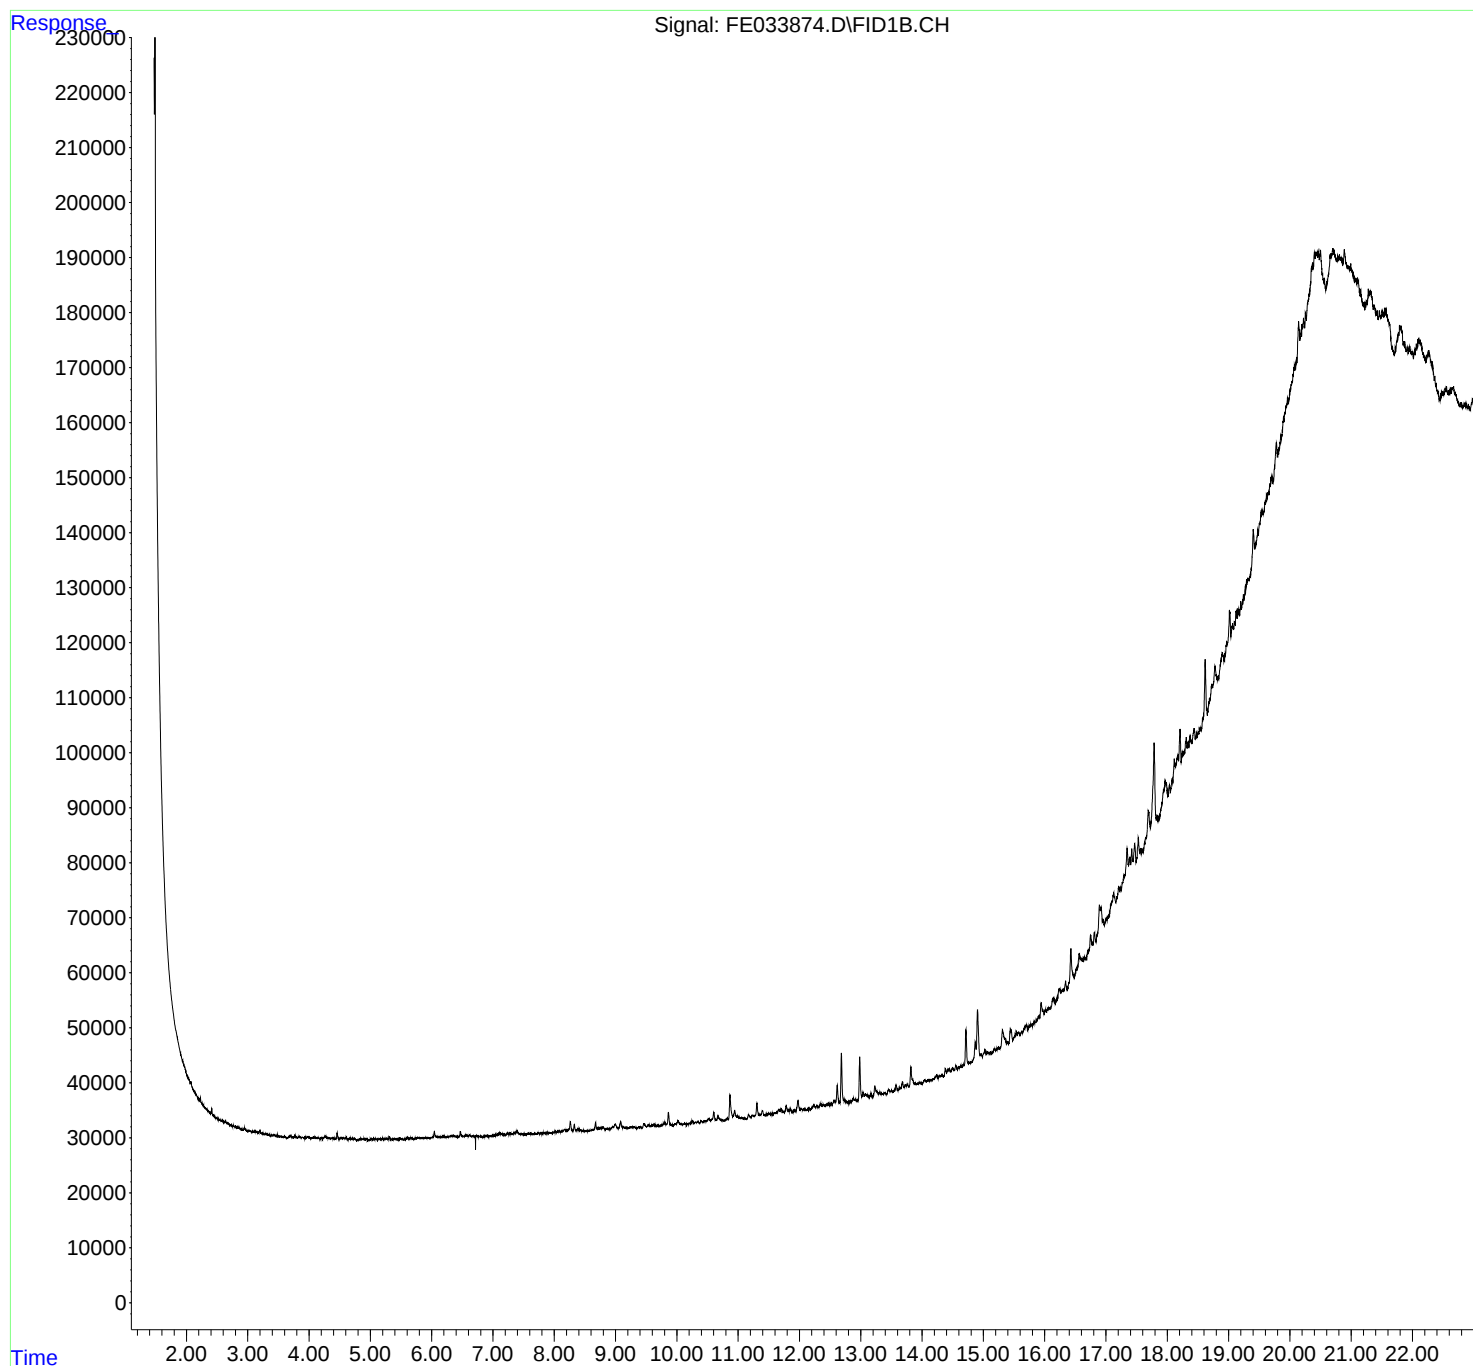

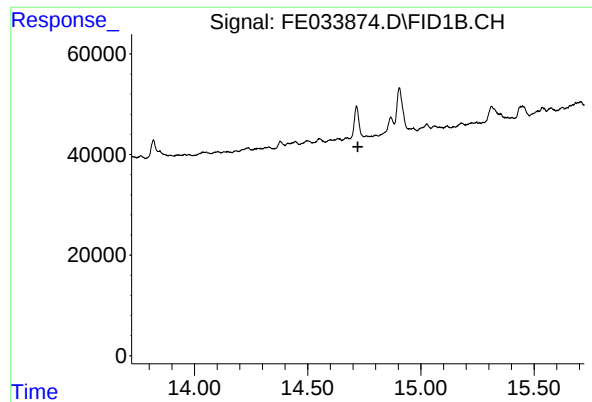

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.721 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
18-B1(2-4)

Manual Integrations
APPROVED

Ankita
6/4/2021 3:31:16 PM