

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060322AL\
 Data File : FE035894.D
 Signal(s) : FID1B.CH
 Acq On : 03 Jun 2022 8:57
 Operator : YP\AJ
 Sample : N3113-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 03 23:13:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 03:24:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.951	5274343	39.761 ug/ml
Spiked Amount 50.000		Recovery =	79.52%
12) S 1-chlorooctadecane (S...	12.382	4889173	46.739 ug/ml
Spiked Amount 50.000		Recovery =	93.48%
Target Compounds			
10) T n-Eicosane (C20)	11.996	200569	1.681 ug/ml
14) T n-Tetracosane (C24)	14.207	152131	1.257 ug/ml
16) T n-Octacosane (C28)	16.198	71624	<MDL ug/ml
17) T n-Tricontane (C30)	17.082	79321	<MDL ug/ml
18) T n-Dotriacontane (C32)	17.913	64771	<MDL ug/ml
19) T n-Tetratriacontane (C34)	18.759	54699	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060322AL\
Data File : FE035894.D
Signal(s) : FID1B.CH
Acq On : 03 Jun 2022 8:57
Operator : YP\AJ
Sample : N3113-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 03 23:13:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
Quant Title : GC Extractables
QLast Update : Wed May 11 03:24:10 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

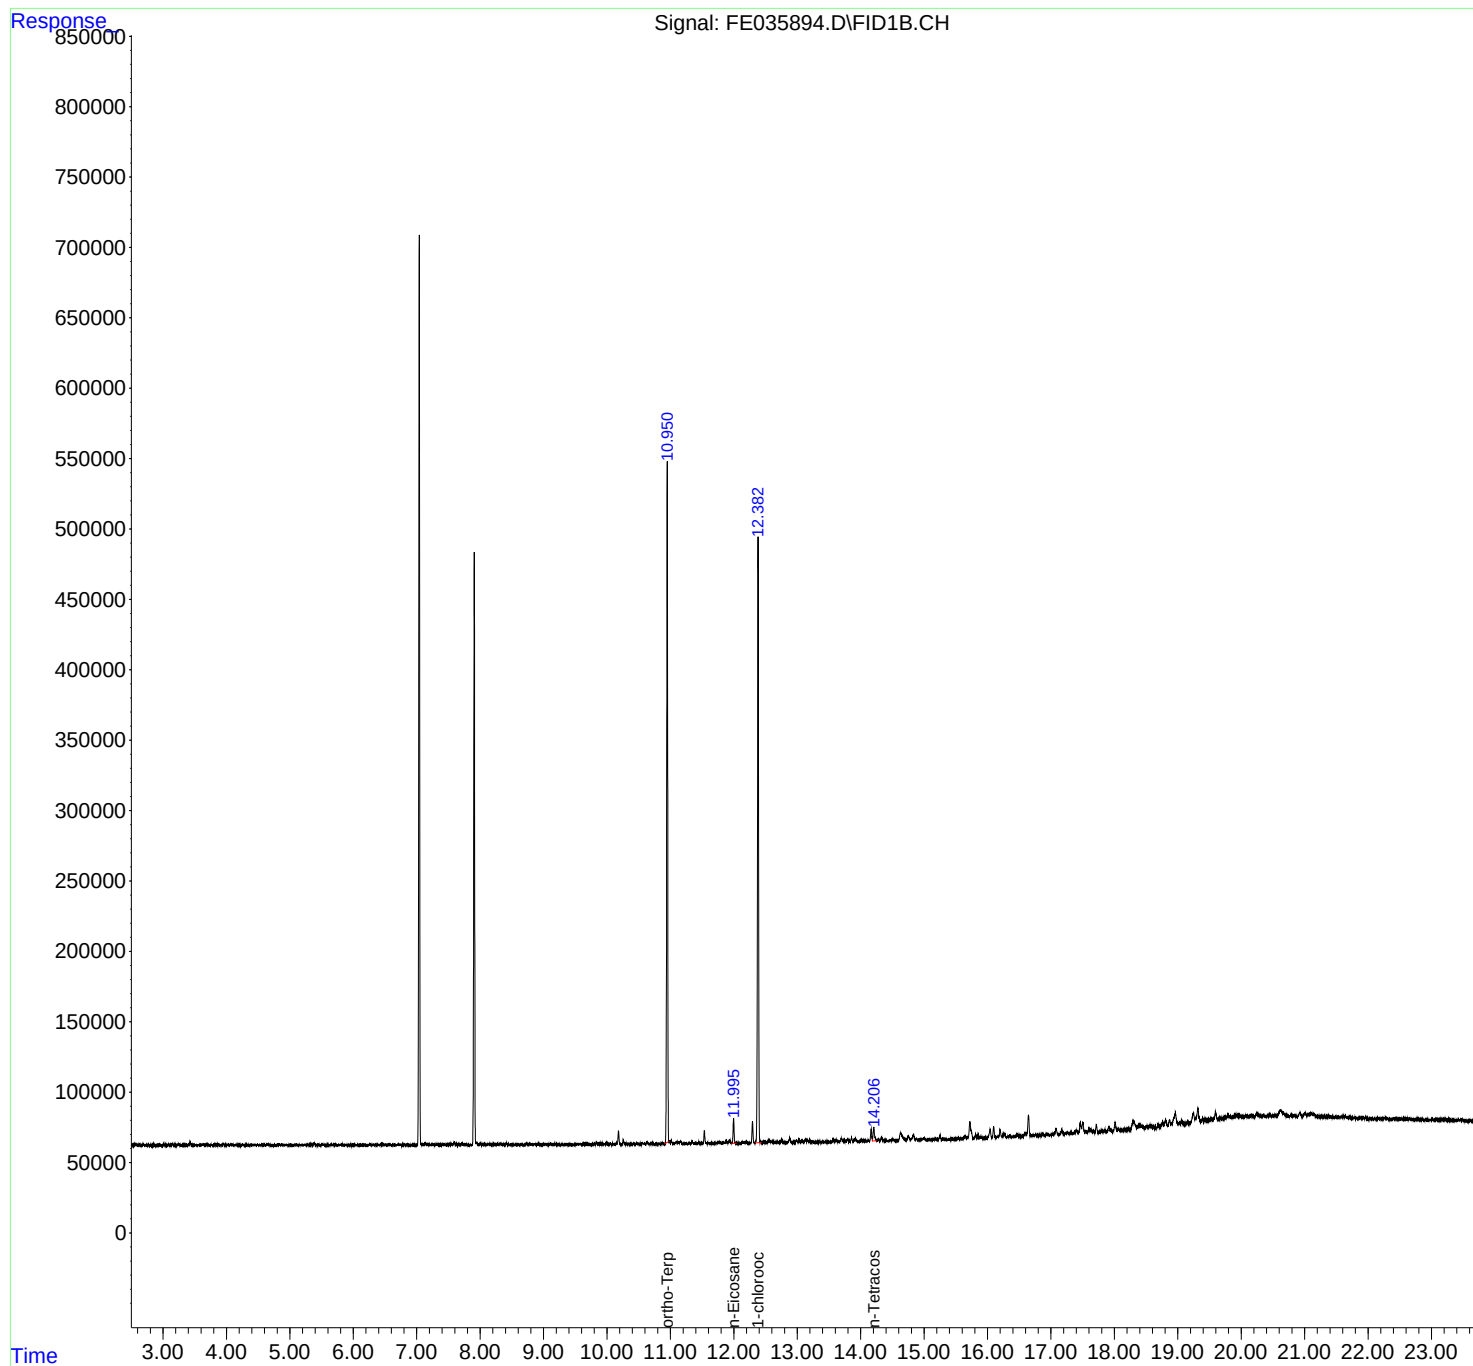


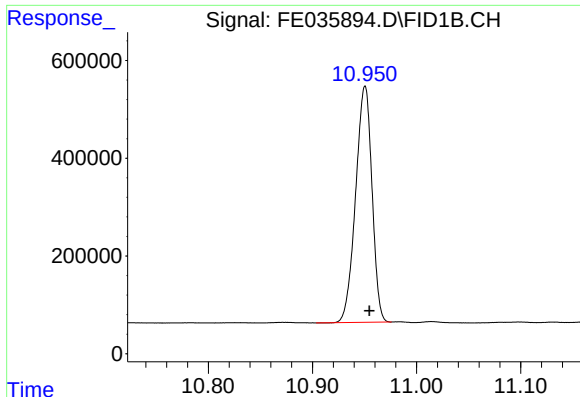

#9 ortho-Terphenyl (SURR)


R.T.: 10.951 min
Delta R.T.: -0.004 min
Response: 5274343
Conc: 39.76 ug/ml

Instrument :
FID_E
ClientSampleId :

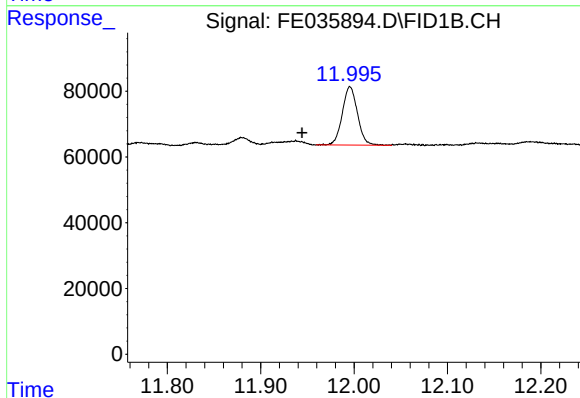


#10 n-Eicosane (C20)

R.T.: 11.996 min
Delta R.T.: 0.051 min
Response: 200569
Conc: 1.68 ug/ml

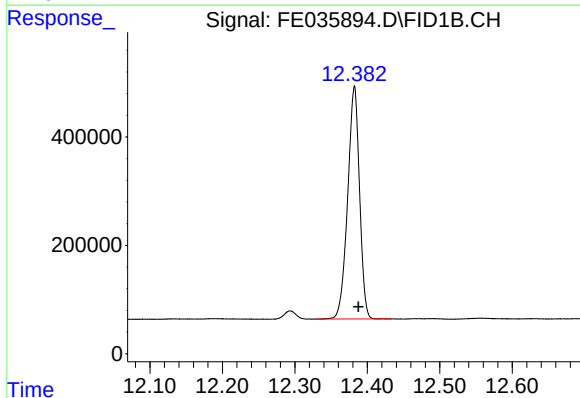

#12 1-chlorooctadecane (SURR)

R.T.: 12.382 min
Delta R.T.: -0.005 min
Response: 4889173
Conc: 46.74 ug/ml

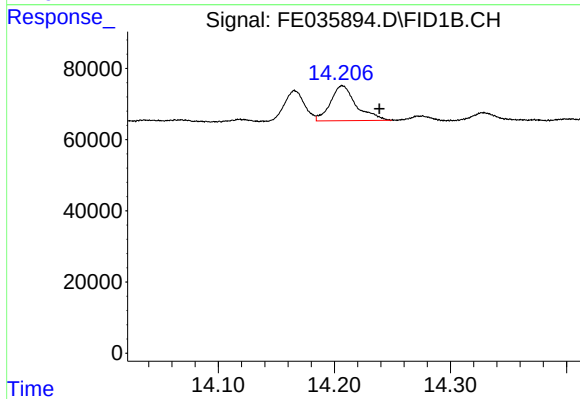

#14 n-Tetracosane (C24)

R.T.: 14.207 min
Delta R.T.: -0.032 min
Response: 152131
Conc: 1.26 ug/ml