

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060420\
 Data File : FE032122.D
 Signal(s) : FID1B.CH
 Acq On : 04 Jun 2020 7:13
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Jun 05 01:01:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050720.M
 Quant Title :
 QLast Update : Thu May 07 13:58:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.236	512173	1.155 ug/ml
8) N-DOCOSANE	13.441	318069	0.710 ug/ml
10) N-TETRACOSANE	14.515f	5750310	12.991 ug/ml
11) N-HEXACOSANE	15.567	248014	0.567 ug/ml
12) N-OCTACOSANE	16.523	261036	0.601 ug/ml
13) N-TRIACONTANE	17.415	314975	0.725 ug/ml
14) N-DOTRIACONTANE	18.250	441701	1.059 ug/ml
15) N-TETRATRIACONTANE	19.034	275839	0.698 ug/ml
16) N-HEXATRIACONTANE	19.776	128021	0.344 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060420\
Data File : FE032122.D
Signal(s) : FID1B.CH
Acq On : 04 Jun 2020 7:13
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 05 01:01:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050720.M
Quant Title :
QLast Update : Thu May 07 13:58:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

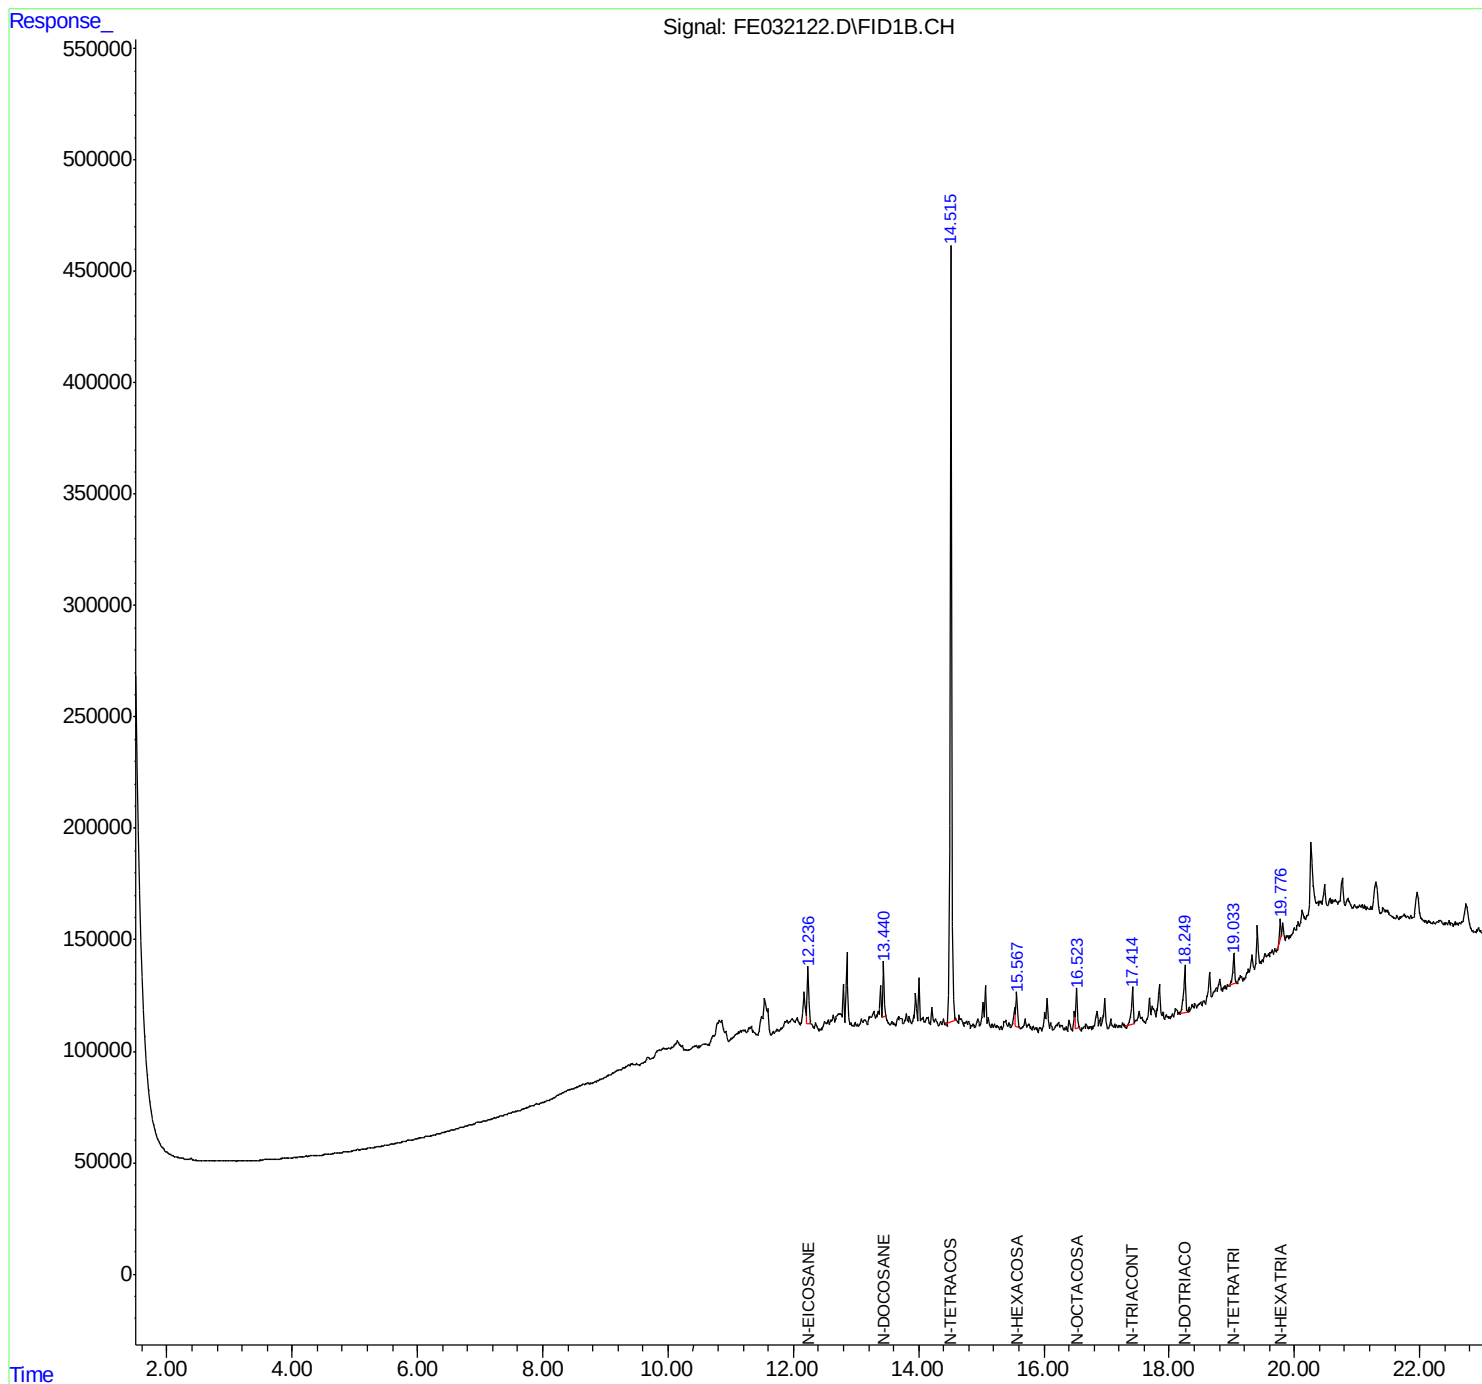


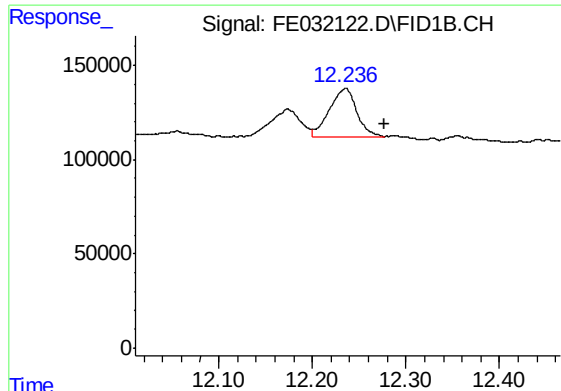

#7 N-EICOSANE


R.T.: 12.236 min
Delta R.T.: -0.042 min
Response: 512173
Conc: 1.15 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

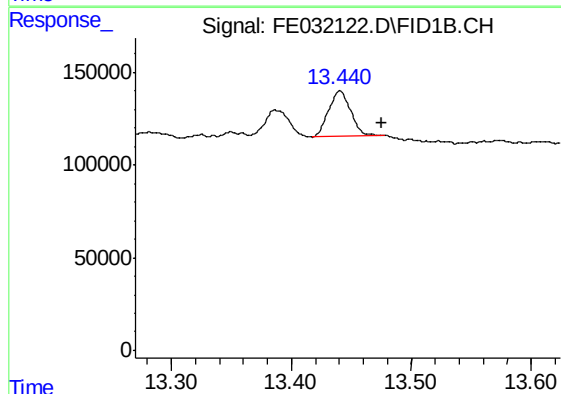


#8 N-DOCOSANE

R.T.: 13.441 min
Delta R.T.: -0.035 min
Response: 318069
Conc: 0.71 ug/ml

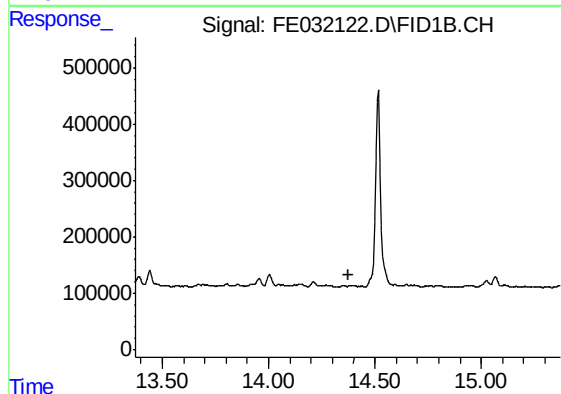


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.373 min
Response: 0
Conc: N.D.

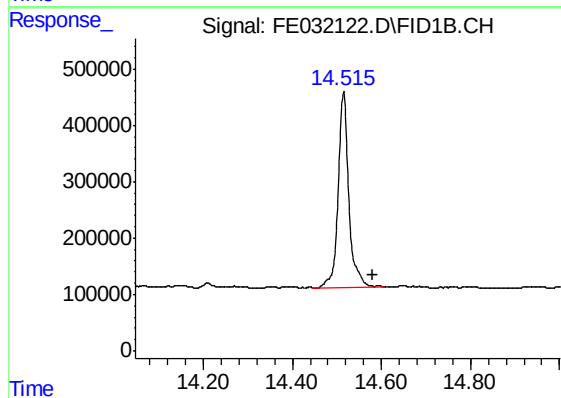

#10 N-TETRACOSANE


R.T.: 14.515 min
Delta R.T.: -0.064 min
Response: 5750310
Conc: 12.99 ug/ml

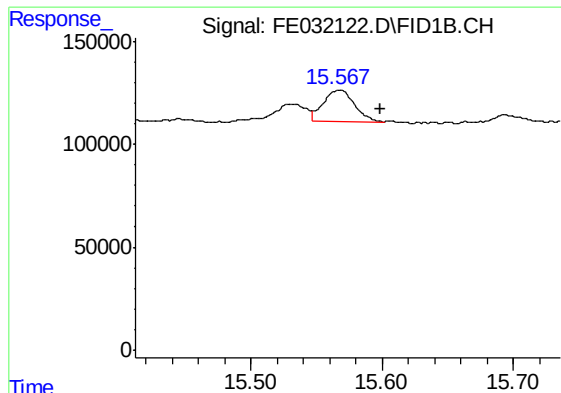

#11 N-HEXACOSANE


R.T.: 15.567 min
Delta R.T.: -0.032 min
Response: 248014
Conc: 0.57 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

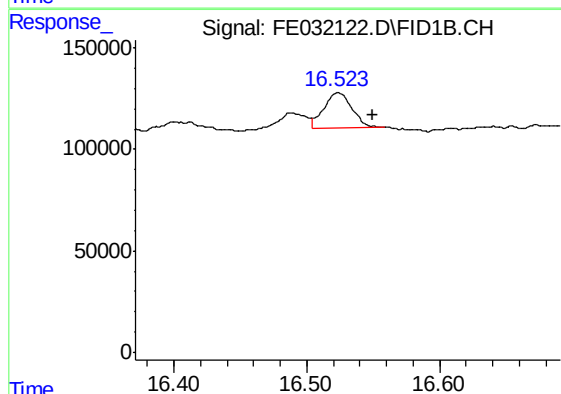


#12 N-OCTACOSANE

R.T.: 16.523 min
Delta R.T.: -0.027 min
Response: 261036
Conc: 0.60 ug/ml

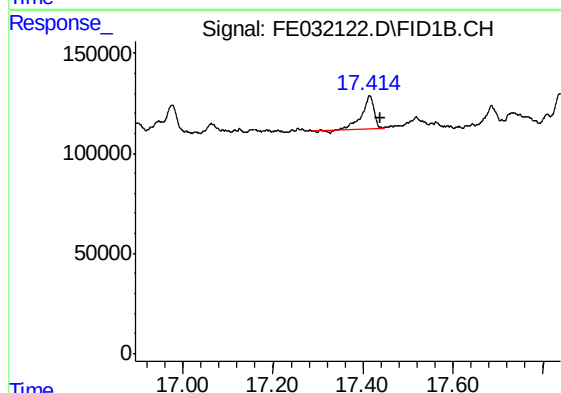


#13 N-TRIACONTANE

R.T.: 17.415 min
Delta R.T.: -0.023 min
Response: 314975
Conc: 0.72 ug/ml

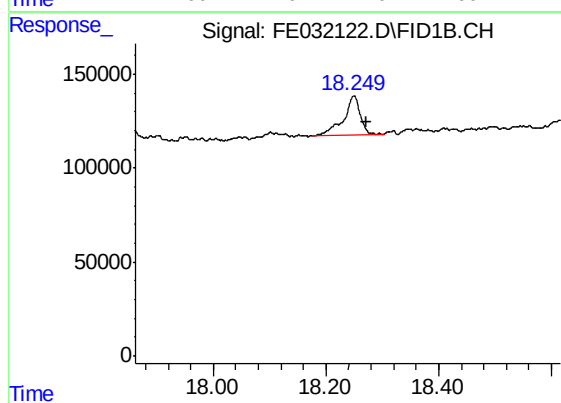

#14 N-DOTRIACONTANE


R.T.: 18.250 min
Delta R.T.: -0.022 min
Response: 441701
Conc: 1.06 ug/ml

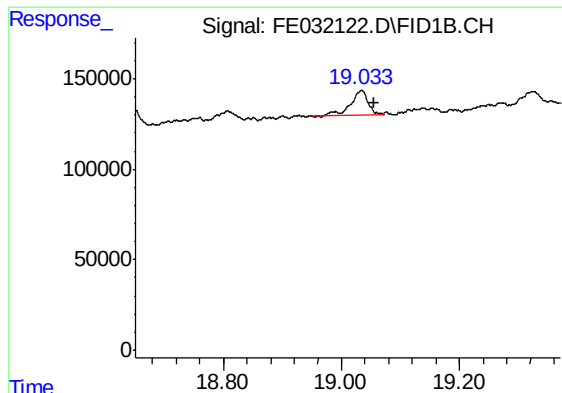

#15 N-TETRATRIACONTANE

R.T.: 19.034 min
Delta R.T.: -0.020 min
Response: 275839
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

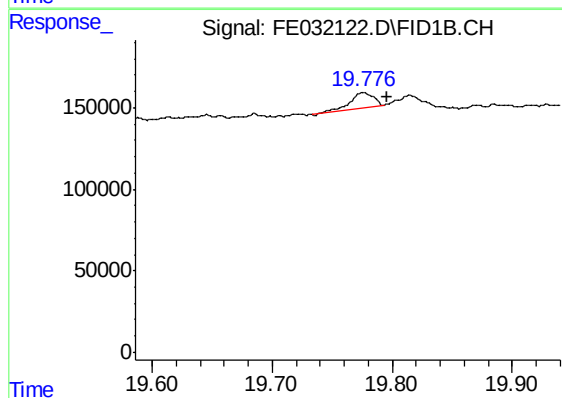

#16 N-HEXATRIACONTANE

R.T.: 19.776 min
Delta R.T.: -0.019 min
Response: 128021
Conc: 0.34 ug/ml