

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060421\
 Data File : FE033878.D
 Signal(s) : FID1B.CH
 Acq On : 04 Jun 2021 7:38
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 22:57:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.604	396423	0.864 ug/ml
8) N-DOCOSANE	13.808	405195	0.879 ug/ml
10) N-TETRACOSANE	14.894	2376627	5.147 ug/ml
11) N-HEXACOSANE	15.940	221931	0.484 ug/ml
12) N-OCTACOSANE	16.891	273064	0.595 ug/ml
13) N-TRIACONTANE	17.780	280653	0.616 ug/ml
14) N-DOTRIACONTANE	18.619	397189	0.892 ug/ml
16) N-HEXATRIACONTANE	20.183	261237	0.652 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060421\
Data File : FE033878.D
Signal(s) : FID1B.CH
Acq On : 04 Jun 2021 7:38
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 04 22:57:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

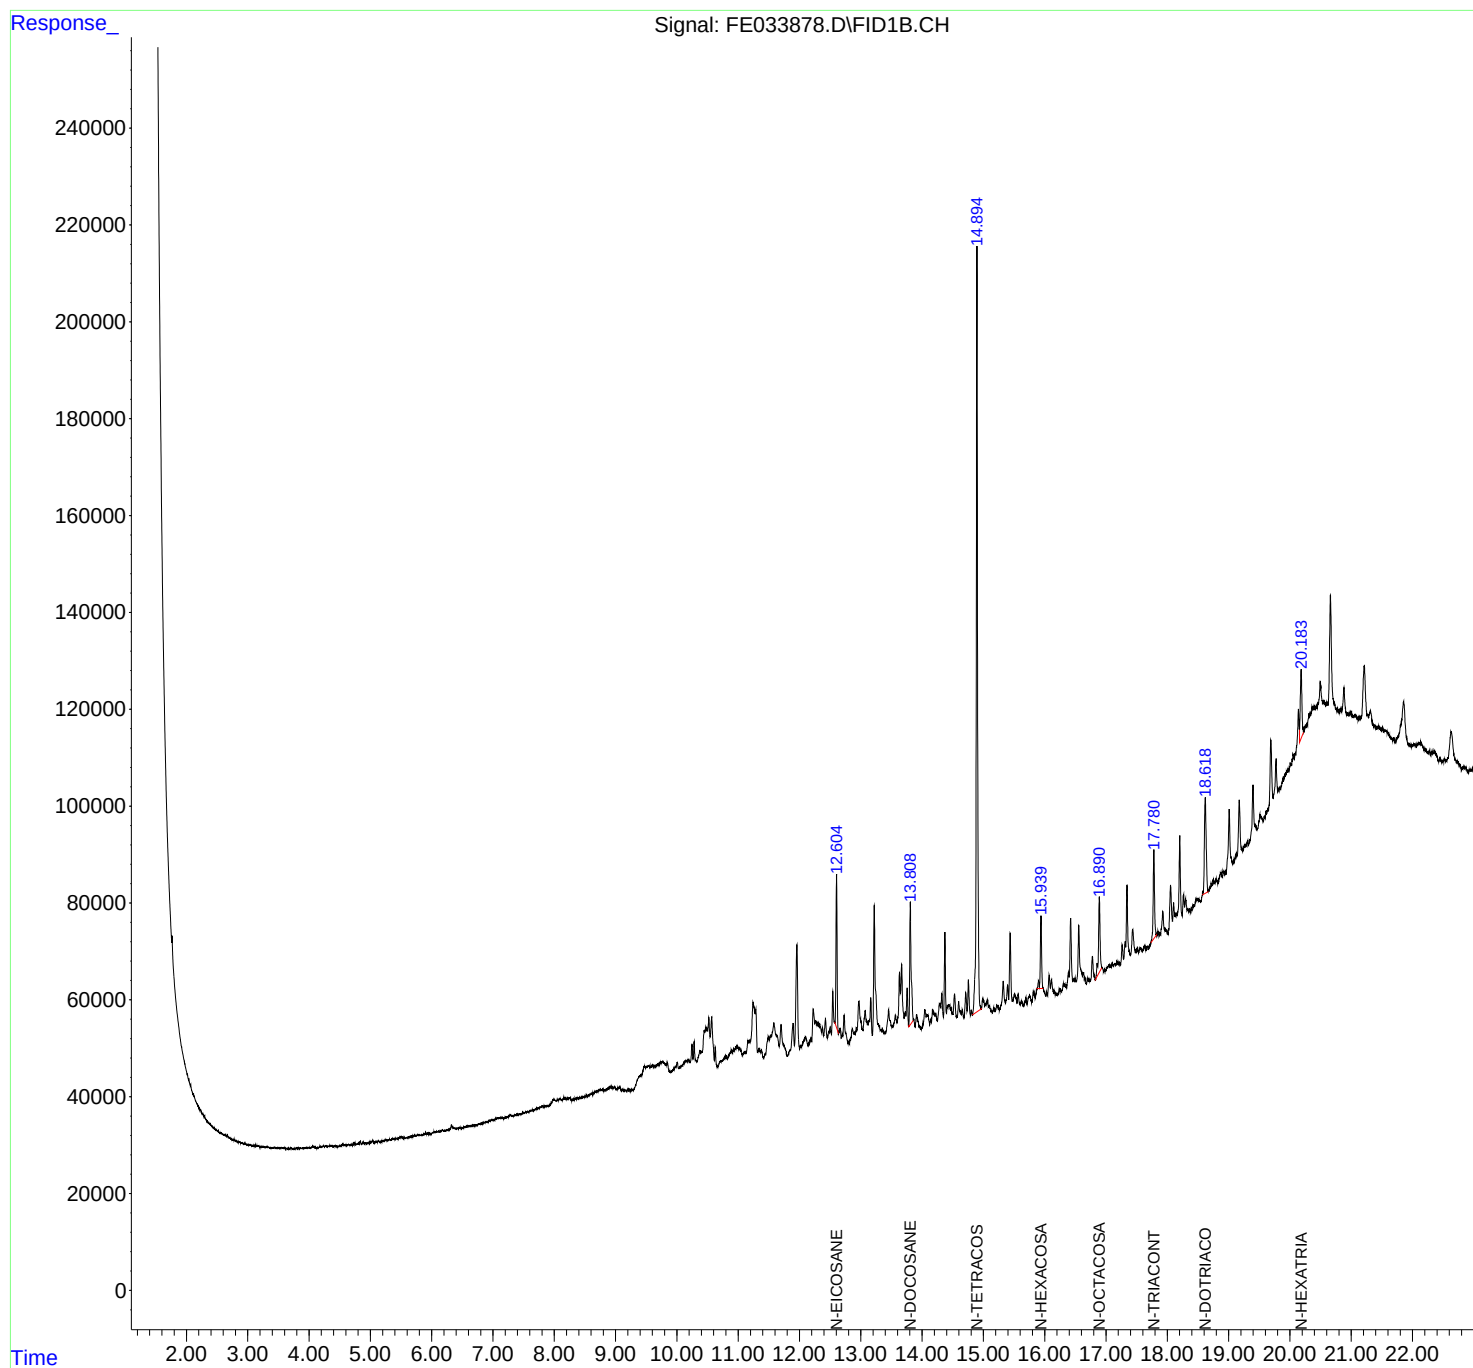


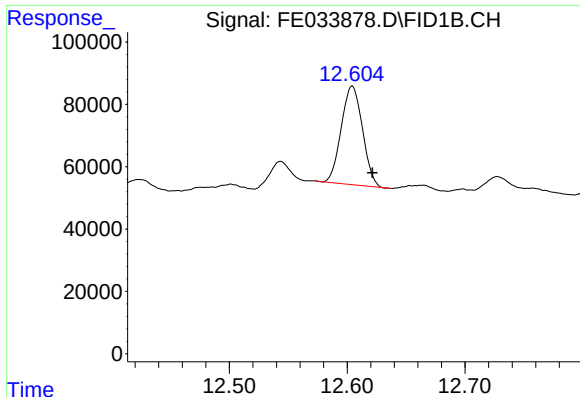

#7 N-EICOSANE


R.T.: 12.604 min
Delta R.T.: -0.017 min
Response: 396423
Conc: 0.86 ug/ml

Instrument :
FID_E
ClientSampleId :

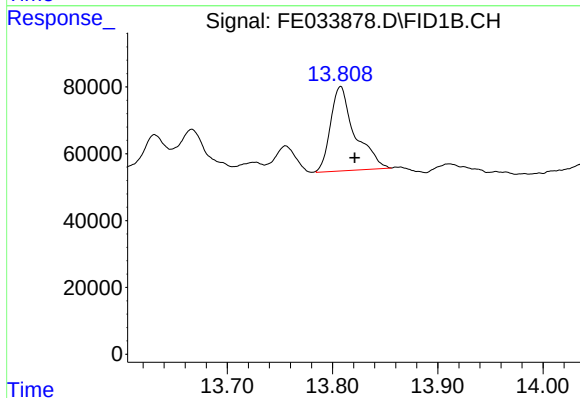


#8 N-DOCOSANE

R.T.: 13.808 min
Delta R.T.: -0.013 min
Response: 405195
Conc: 0.88 ug/ml

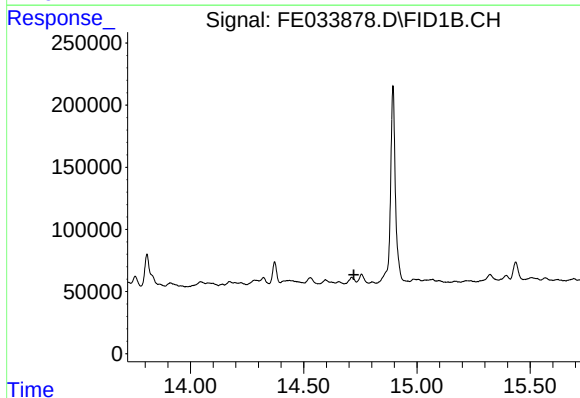


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.721 min
Response: 0
Conc: N.D.

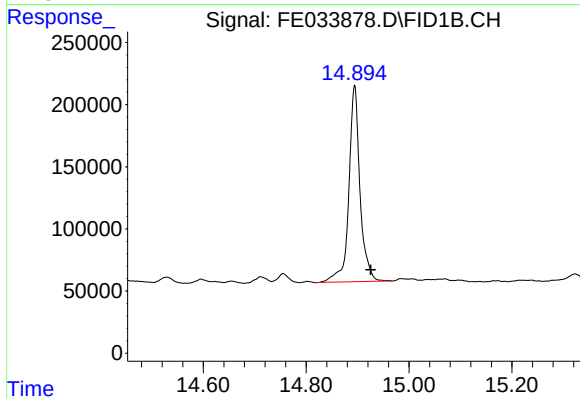

#10 N-TETRACOSANE


R.T.: 14.894 min
Delta R.T.: -0.031 min
Response: 2376627
Conc: 5.15 ug/ml

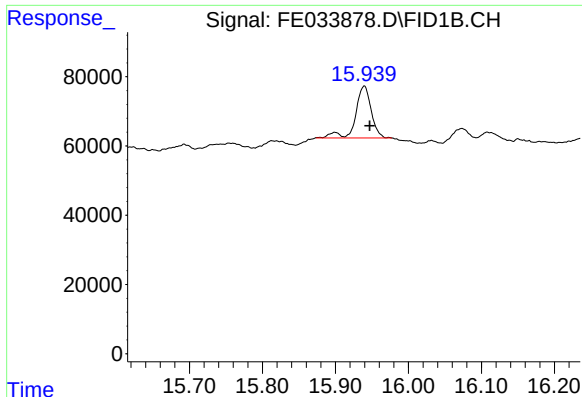

#11 N-HEXACOSANE


R.T.: 15.940 min
Delta R.T.: -0.007 min
Response: 221931
Conc: 0.48 ug/ml

Instrument :
FID_E
ClientSampleId :

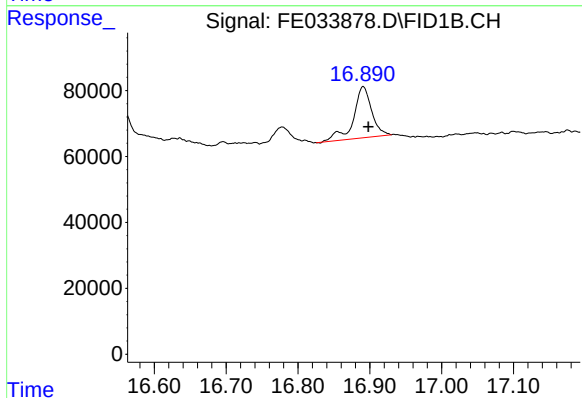


#12 N-OCTACOSANE

R.T.: 16.891 min
Delta R.T.: -0.007 min
Response: 273064
Conc: 0.60 ug/ml

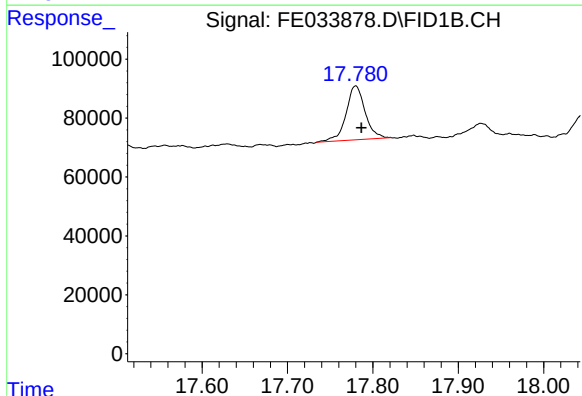


#13 N-TRIACONTANE

R.T.: 17.780 min
Delta R.T.: -0.007 min
Response: 280653
Conc: 0.62 ug/ml

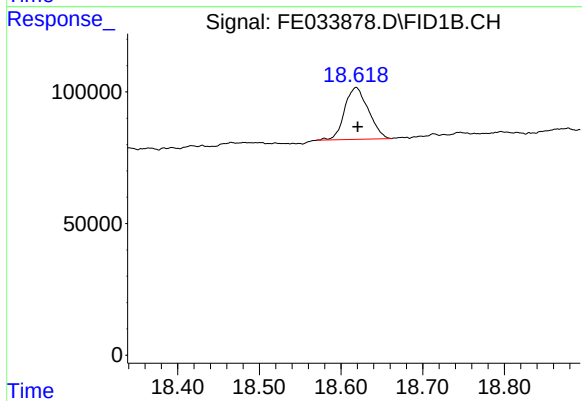

#14 N-DOTRIACONTANE

R.T.: 18.619 min
Delta R.T.: -0.002 min
Response: 397189
Conc: 0.89 ug/ml

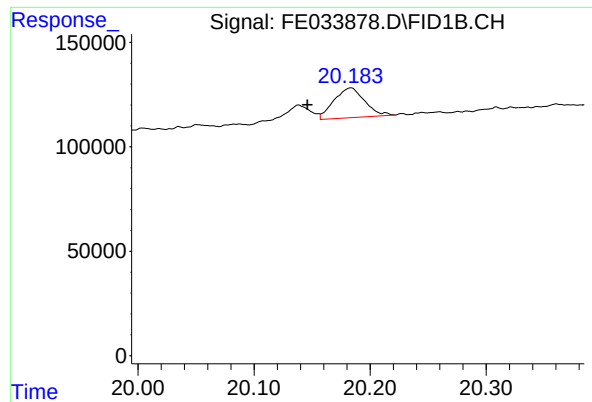

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: 0.038 min
Response: 261237
Conc: 0.65 ug/ml

Instrument :
FID_E
ClientSampleId :