

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060421\
 Data File : FE033884.D
 Signal(s) : FID1B.CH
 Acq On : 04 Jun 2021 11:10
 Operator : DD\AJ
 Sample : M2589-19 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 18-B12(2-4)

Manual Integrations
 APPROVED

Ankita
 6/7/2021 10:40:51 AM

Integration File: autoint1.e
 Quant Time: Jun 04 22:58:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	254229	0.629 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060421\
Data File : FE033884.D
Signal(s) : FID1B.CH
Acq On : 04 Jun 2021 11:10
Operator : DD\AJ
Sample : M2589-19 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
18-B12(2-4)


Manual Integrations
APPROVED

Ankita
6/7/2021 10:40:51 AM

Integration File: autoint1.e
Quant Time: Jun 04 22:58:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

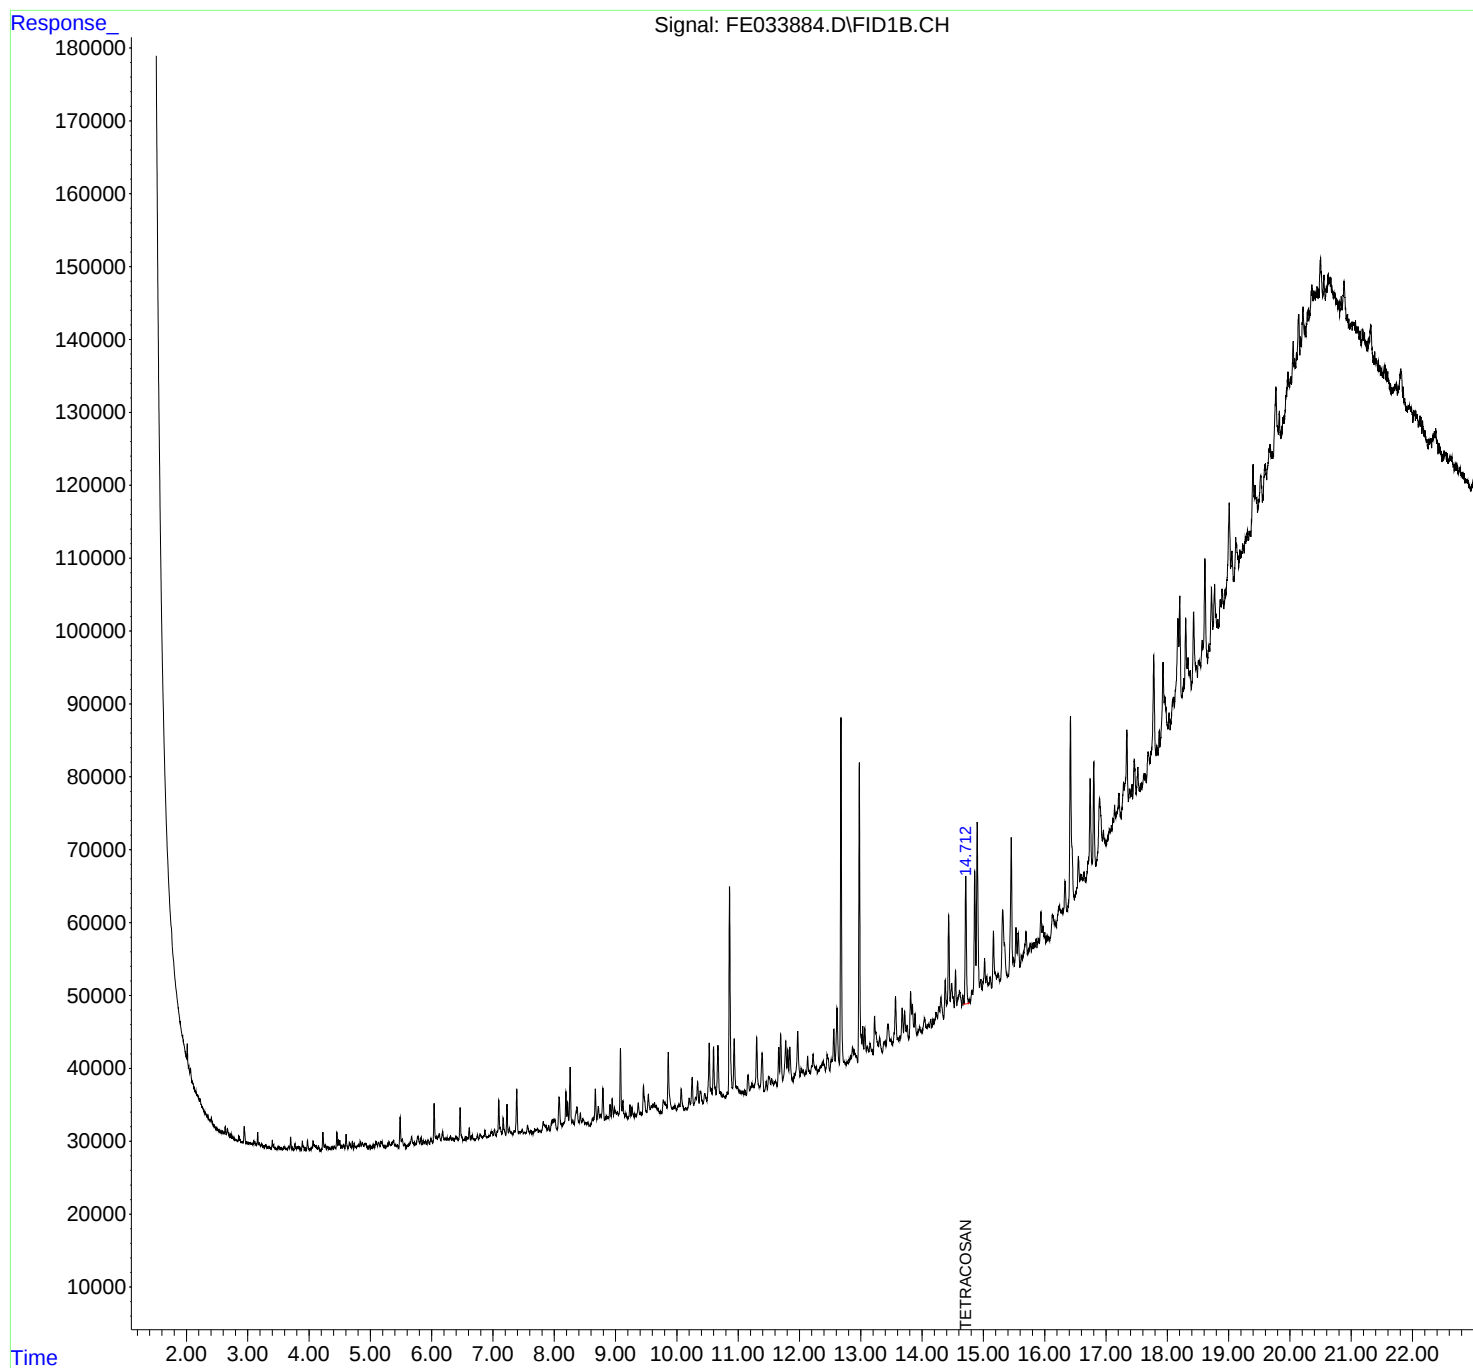

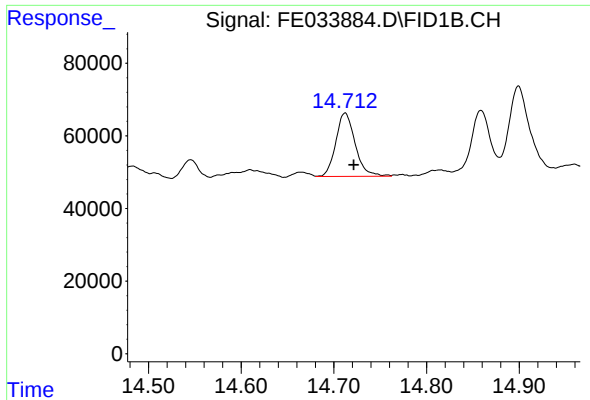

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.009 min
Response: 254229
Conc: 0.63 ug/ml m

Instrument :
FID_E
ClientSampleId :
18-B12(2-4)

Manual Integrations
APPROVED

Ankita
6/7/2021 10:40:51 AM