

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060424AL\
Data File : FE048534.D
Signal(s) : FID1B.ch
Acq On : 04 Jun 2024 13:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 01:50:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.925	65024	0.491 ug/ml
11) T	n-Heneicosane (C21)	13.541	90918	0.702 ug/ml
13) T	n-Docosane (C22)	14.128	71593	0.556 ug/ml
14) T	n-Tetracosane (C24)	15.229	93664	0.723 ug/ml
15) T	n-Hexacosane (C26)	16.252	49717	0.384 ug/ml
18) T	n-Dotriacontane (C32)	18.921	114721	0.845 ug/ml
19) T	n-Tetratriacontane (C34)	19.697	80164	0.586 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060424AL\
Data File : FE048534.D
Signal(s) : FID1B.ch
Acq On : 04 Jun 2024 13:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 01:50:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

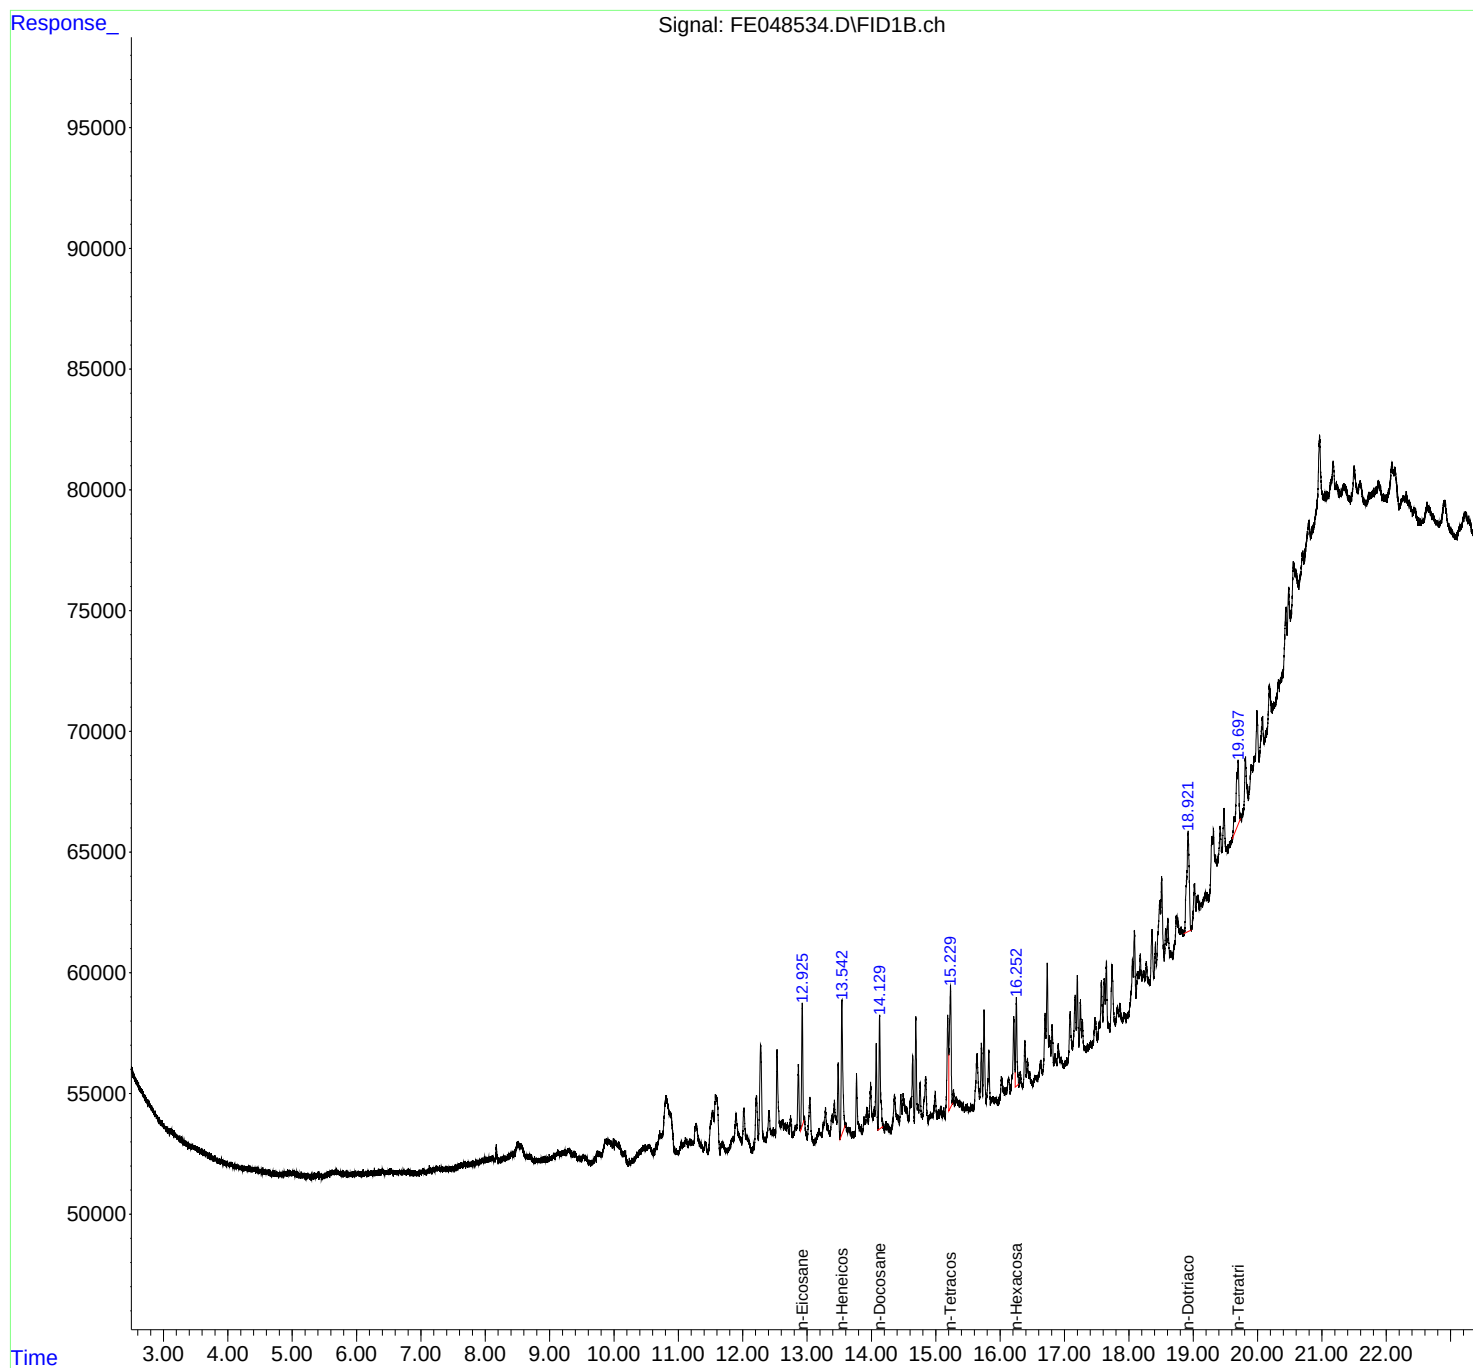


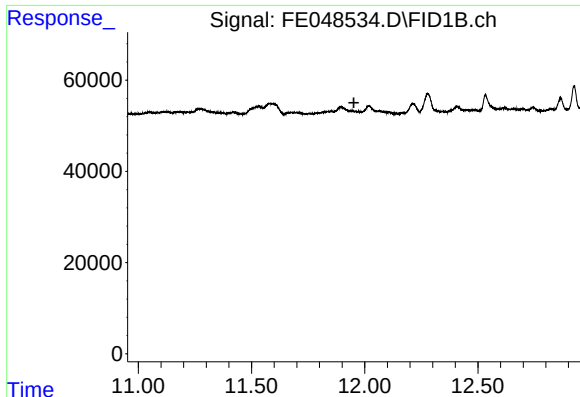

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.952 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

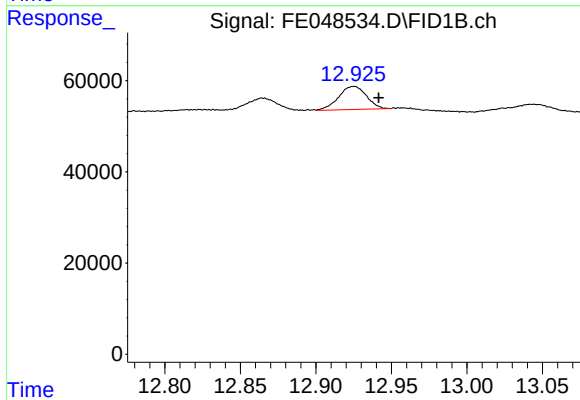


#10 n-Eicosane (C20)

R.T.: 12.925 min
Delta R.T.: -0.016 min
Response: 65024
Conc: 0.49 ug/ml

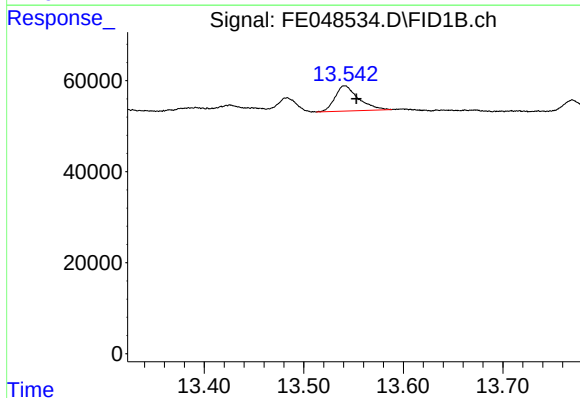


#11 n-Heneicosane (C21)

R.T.: 13.541 min
Delta R.T.: -0.011 min
Response: 90918
Conc: 0.70 ug/ml

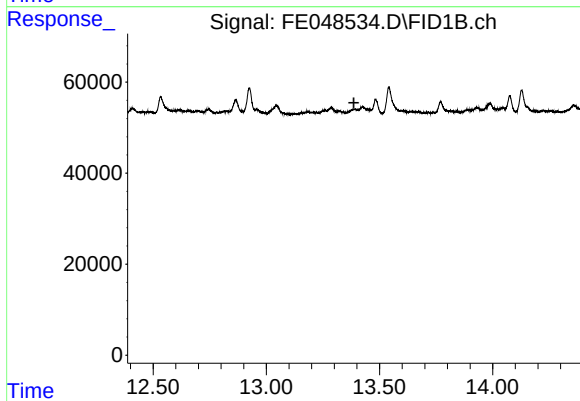

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.387 min
Response: 0
Conc: N.D.

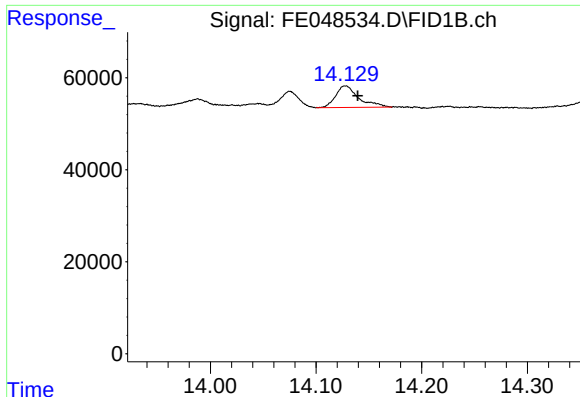

#13 n-Docosane (C22)


R.T.: 14.128 min
Delta R.T.: -0.011 min
Response: 71593
Conc: 0.56 ug/ml

Instrument :
FID_E
ClientSampleId :

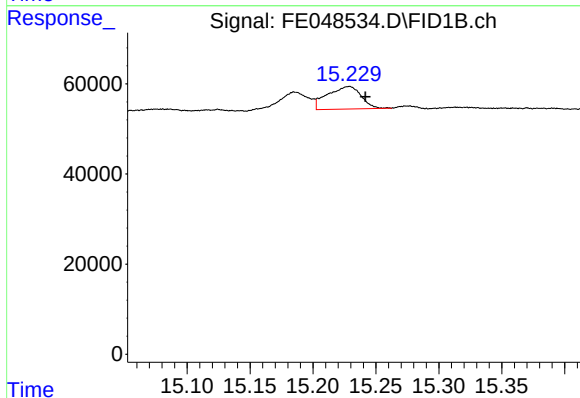


#14 n-Tetracosane (C24)

R.T.: 15.229 min
Delta R.T.: -0.013 min
Response: 93664
Conc: 0.72 ug/ml

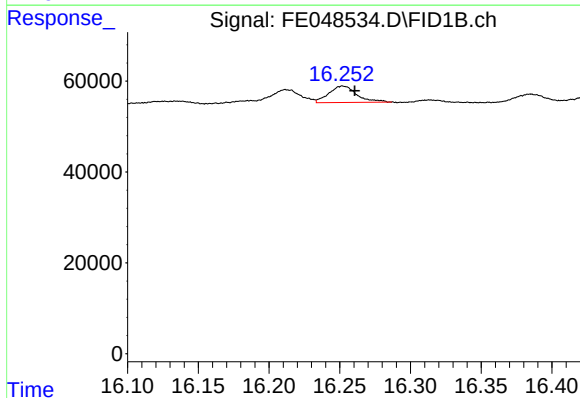


#15 n-Hexacosane (C26)

R.T.: 16.252 min
Delta R.T.: -0.009 min
Response: 49717
Conc: 0.38 ug/ml

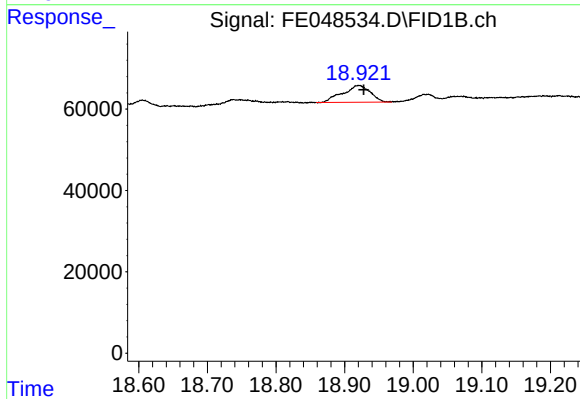

#18 n-Dotriacontane (C32)

R.T.: 18.921 min
Delta R.T.: -0.007 min
Response: 114721
Conc: 0.85 ug/ml

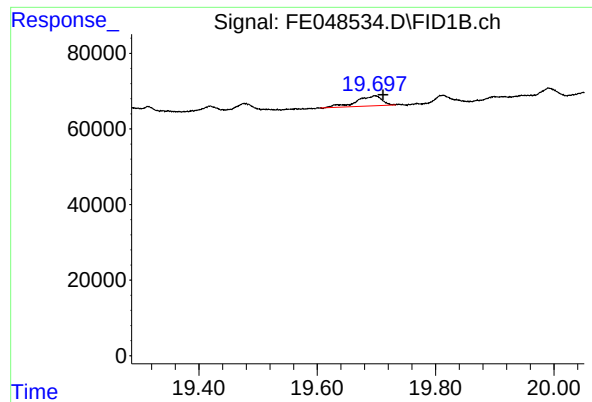

#19 n-Tetratriacontane (C34)

R.T.: 19.697 min
Delta R.T.: -0.014 min
Response: 80164
Conc: 0.59 ug/ml

Instrument :
FID_E
ClientSampleId :